


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA_N\Data\BN021318\
 Data File : BN000065.D
 Acq On : 13 Feb 2018 08:26
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_N\METHODS\8270-BN020718.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Feb 07 18:24:45 2018

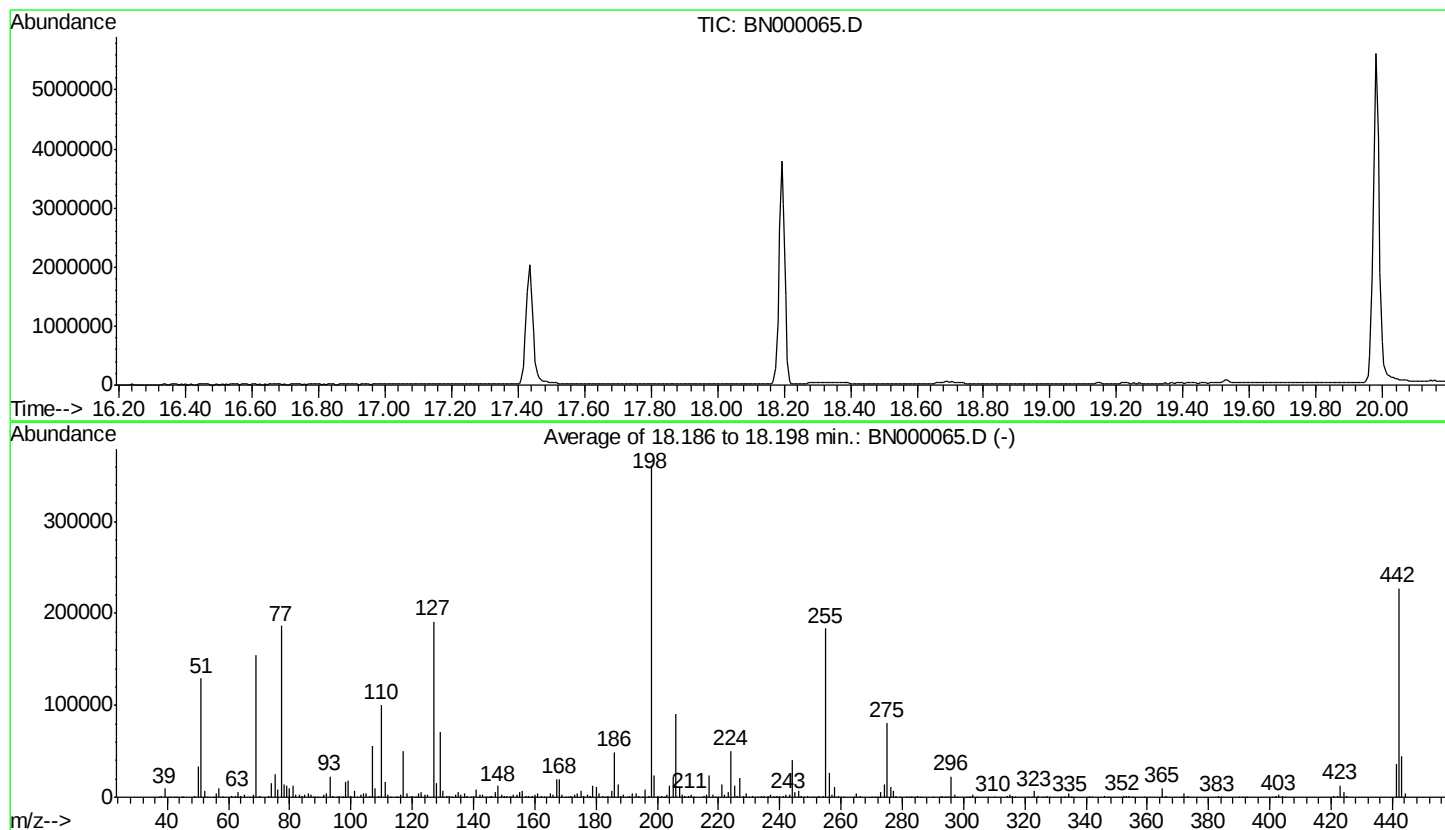

AutoFind: Scans 2584, 2585, 2586; Background Corrected with Scan 2577

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.8	129053	PASS
68	69	0.00	2	2.0	3111	PASS
69	198	0.00	100	43.0	155264	PASS
70	69	0.00	2	0.6	896	PASS
127	198	10	80	52.9	190912	PASS
197	198	0.00	2	0.5	1645	PASS
198	198	100	100	100.0	360810	PASS
199	198	5	9	6.5	23597	PASS
275	198	10	60	22.5	81125	PASS
365	198	1	100	2.8	9941	PASS
441	443	0.01	100	82.4	36357	PASS
442	198	50	100	63.1	227669	PASS
443	442	15	24	19.4	44106	PASS