

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021323\
 Data File : BN024010.D
 Acq On : 13 Feb 2023 11:48
 Operator : CG/JU
 Sample : PB150763BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Feb 14 01:15:41 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN013023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 14 01:13:07 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.834	152	4032	0.400	ng/ul	0.00
4) Naphthalene-d8	10.639	136	10883	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.488	164	6613	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.238	188	14985	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.432	240	12707	0.400	ng/ul	# 0.00
23) Perylene-d12	23.829	264	10550	0.400	ng/ul	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.227	96	20762	4.804	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.234	152	4213	0.247	ng/ul	0.00
18) Fluoranthene-d10	19.267	212	10769	0.315	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.634	202	1800	0.041	ng/ul#	1
26) Benzo(a)pyrene	23.668	252	3726	0.096	ng/ul#	53


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021323\
Data File : BN024010.D
Acq On : 13 Feb 2023 11:48
Operator : CG/JU
Sample : PB150763BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Feb 14 01:15:41 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN013023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 14 01:13:07 2023
Response via : Initial Calibration

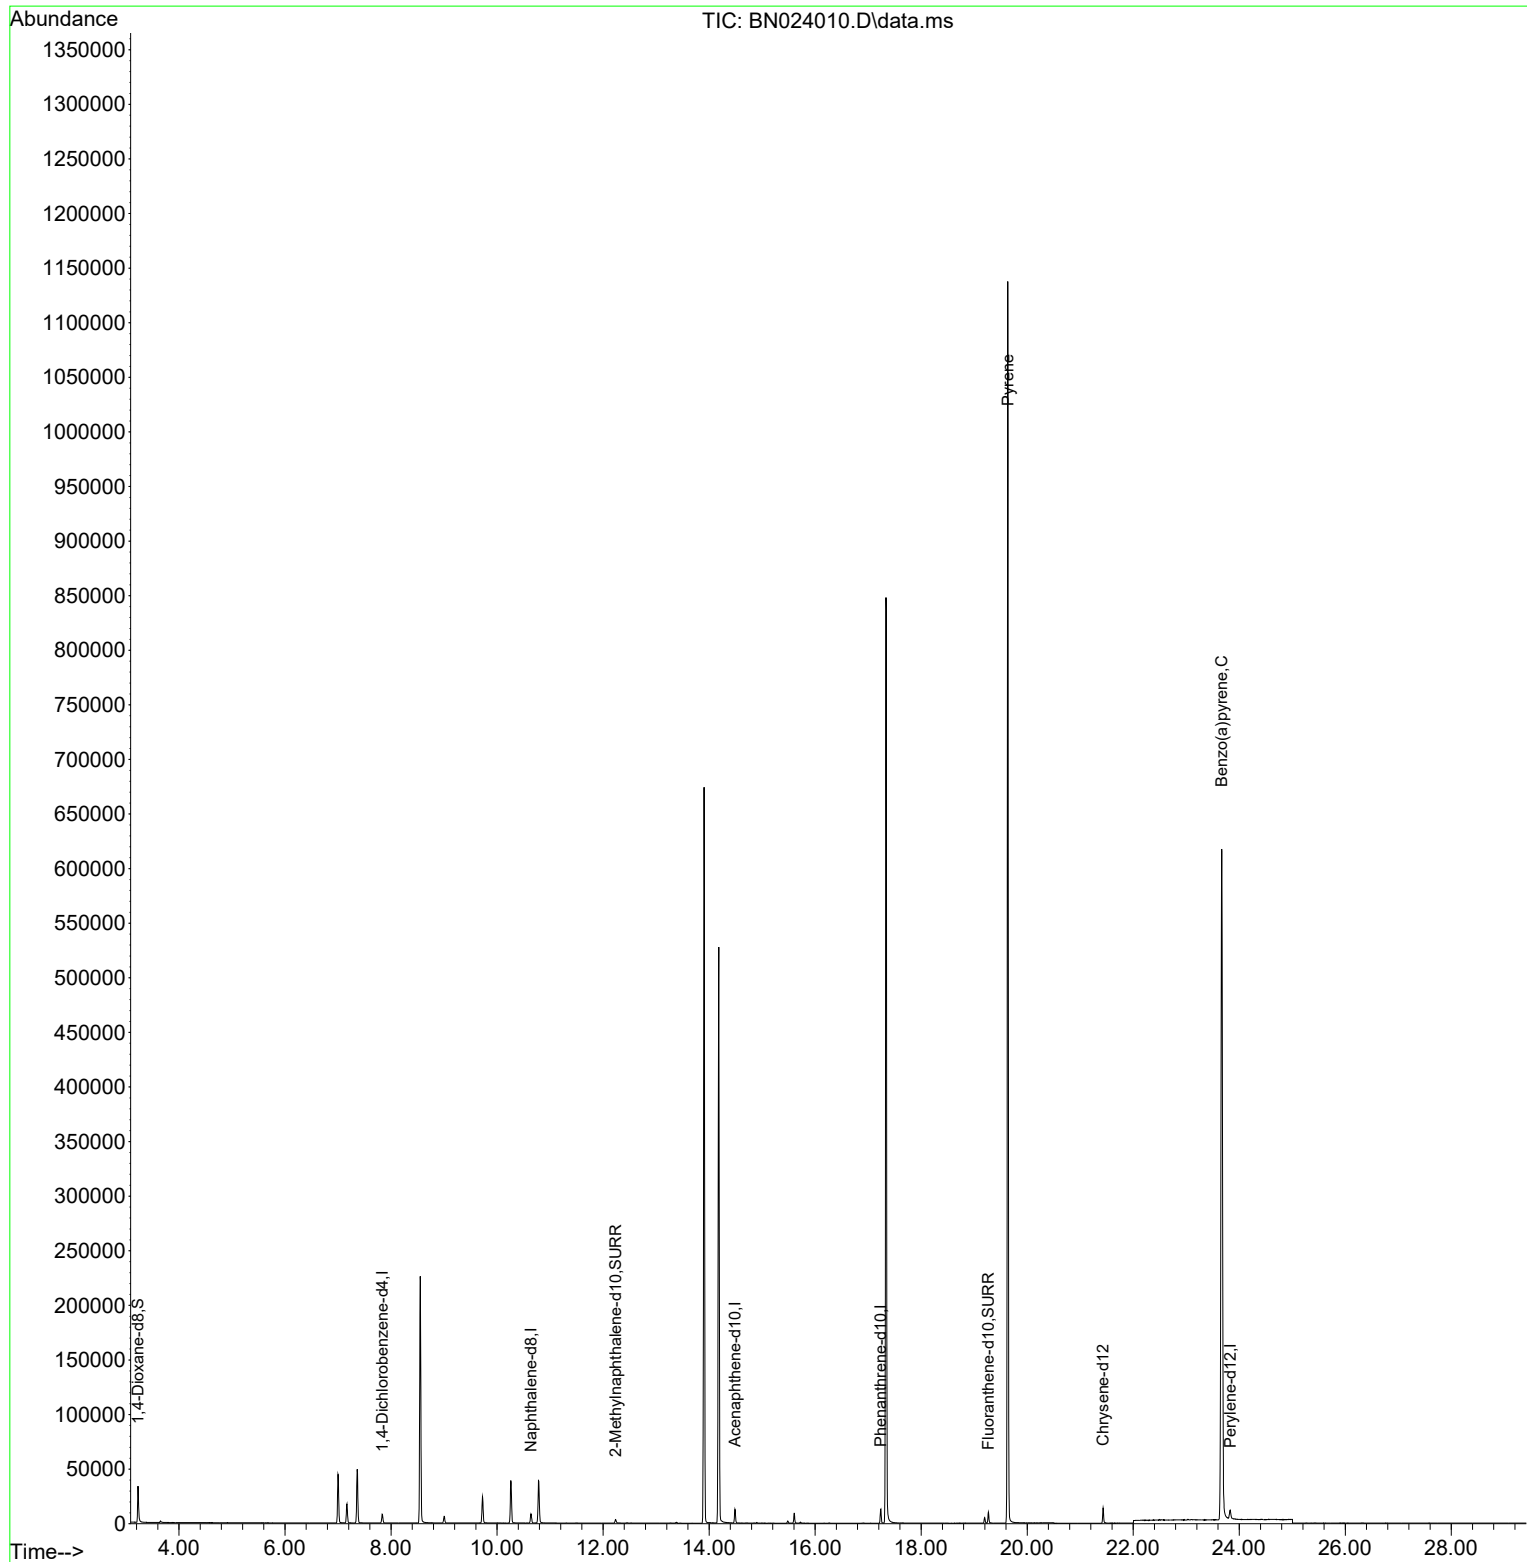

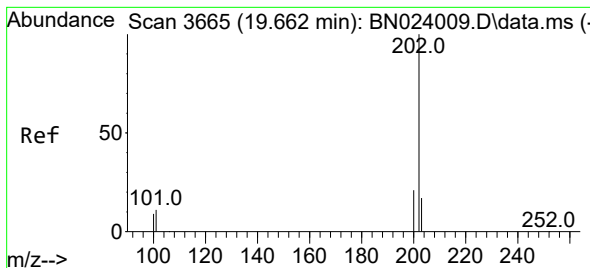

#20

Pyrene

Concen: 0.041 ng/ul

RT: 19.634 min Scan# 3659

Delta R.T. -0.028 min


Lab File: BN024010.D

Acq: 13 Feb 2023 11:48

Instrument :




BNA_N

ClientSampleId :

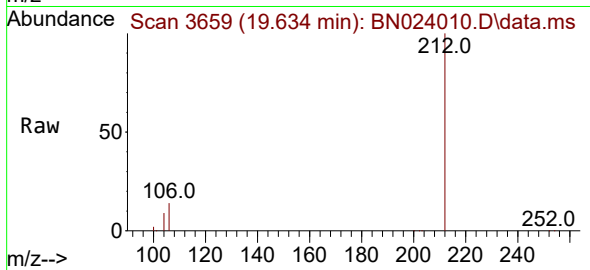

Tgt Ion:202 Resp: 1800

Ion	Ratio	Lower	Upper
202	100		
101	165.0	8.1	12.1#
100	1269.5	6.2	9.4#

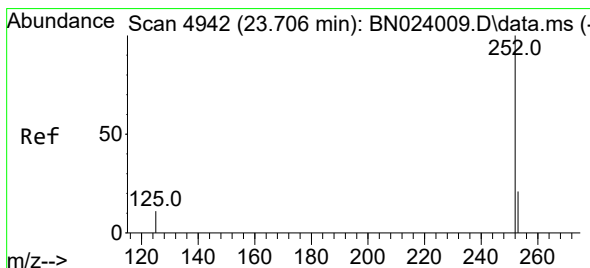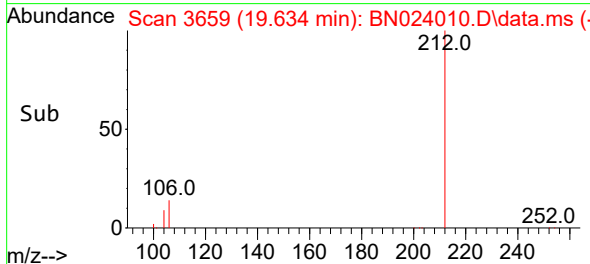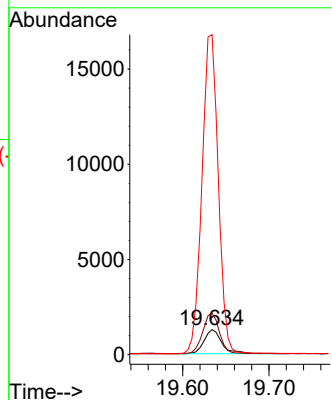

#26

Benzo(a)pyrene

Concen: 0.096 ng/ul

RT: 23.668 min Scan# 4929

Delta R.T. -0.038 min

Lab File: BN024010.D

Acq: 13 Feb 2023 11:48

Tgt Ion:252 Resp: 3726

Ion	Ratio	Lower	Upper
252	100		
253	49.0	21.5	32.3#
125	37.1	11.2	16.8#

