

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021323\
 Data File : BN024012.D
 Acq On : 13 Feb 2023 14:12
 Operator : CG/JU
 Sample : 01422-05
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Feb 14 01:15:47 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN013023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 14 01:13:07 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.834	152	4527	0.400	ng/ul	0.00
4) Naphthalene-d8	10.639	136	12247	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.488	164	7523	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.238	188	17104	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.435	240	16493	0.400	ng/ul	0.00
23) Perylene-d12	23.829	264	12747	0.400	ng/ul	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.222	96	20688	4.263	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.234	152	4377	0.228	ng/ul	0.00
18) Fluoranthene-d10	19.272	212	10946	0.247	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.634	202	1934	0.034	ng/ul#	1
26) Benzo(a)pyrene	23.665	252	3620	0.077	ng/ul#	47


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021323\
Data File : BN024012.D
Acq On : 13 Feb 2023 14:12
Operator : CG/JU
Sample : 01422-05
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :


Quant Time: Feb 14 01:15:47 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN013023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 14 01:13:07 2023
Response via : Initial Calibration

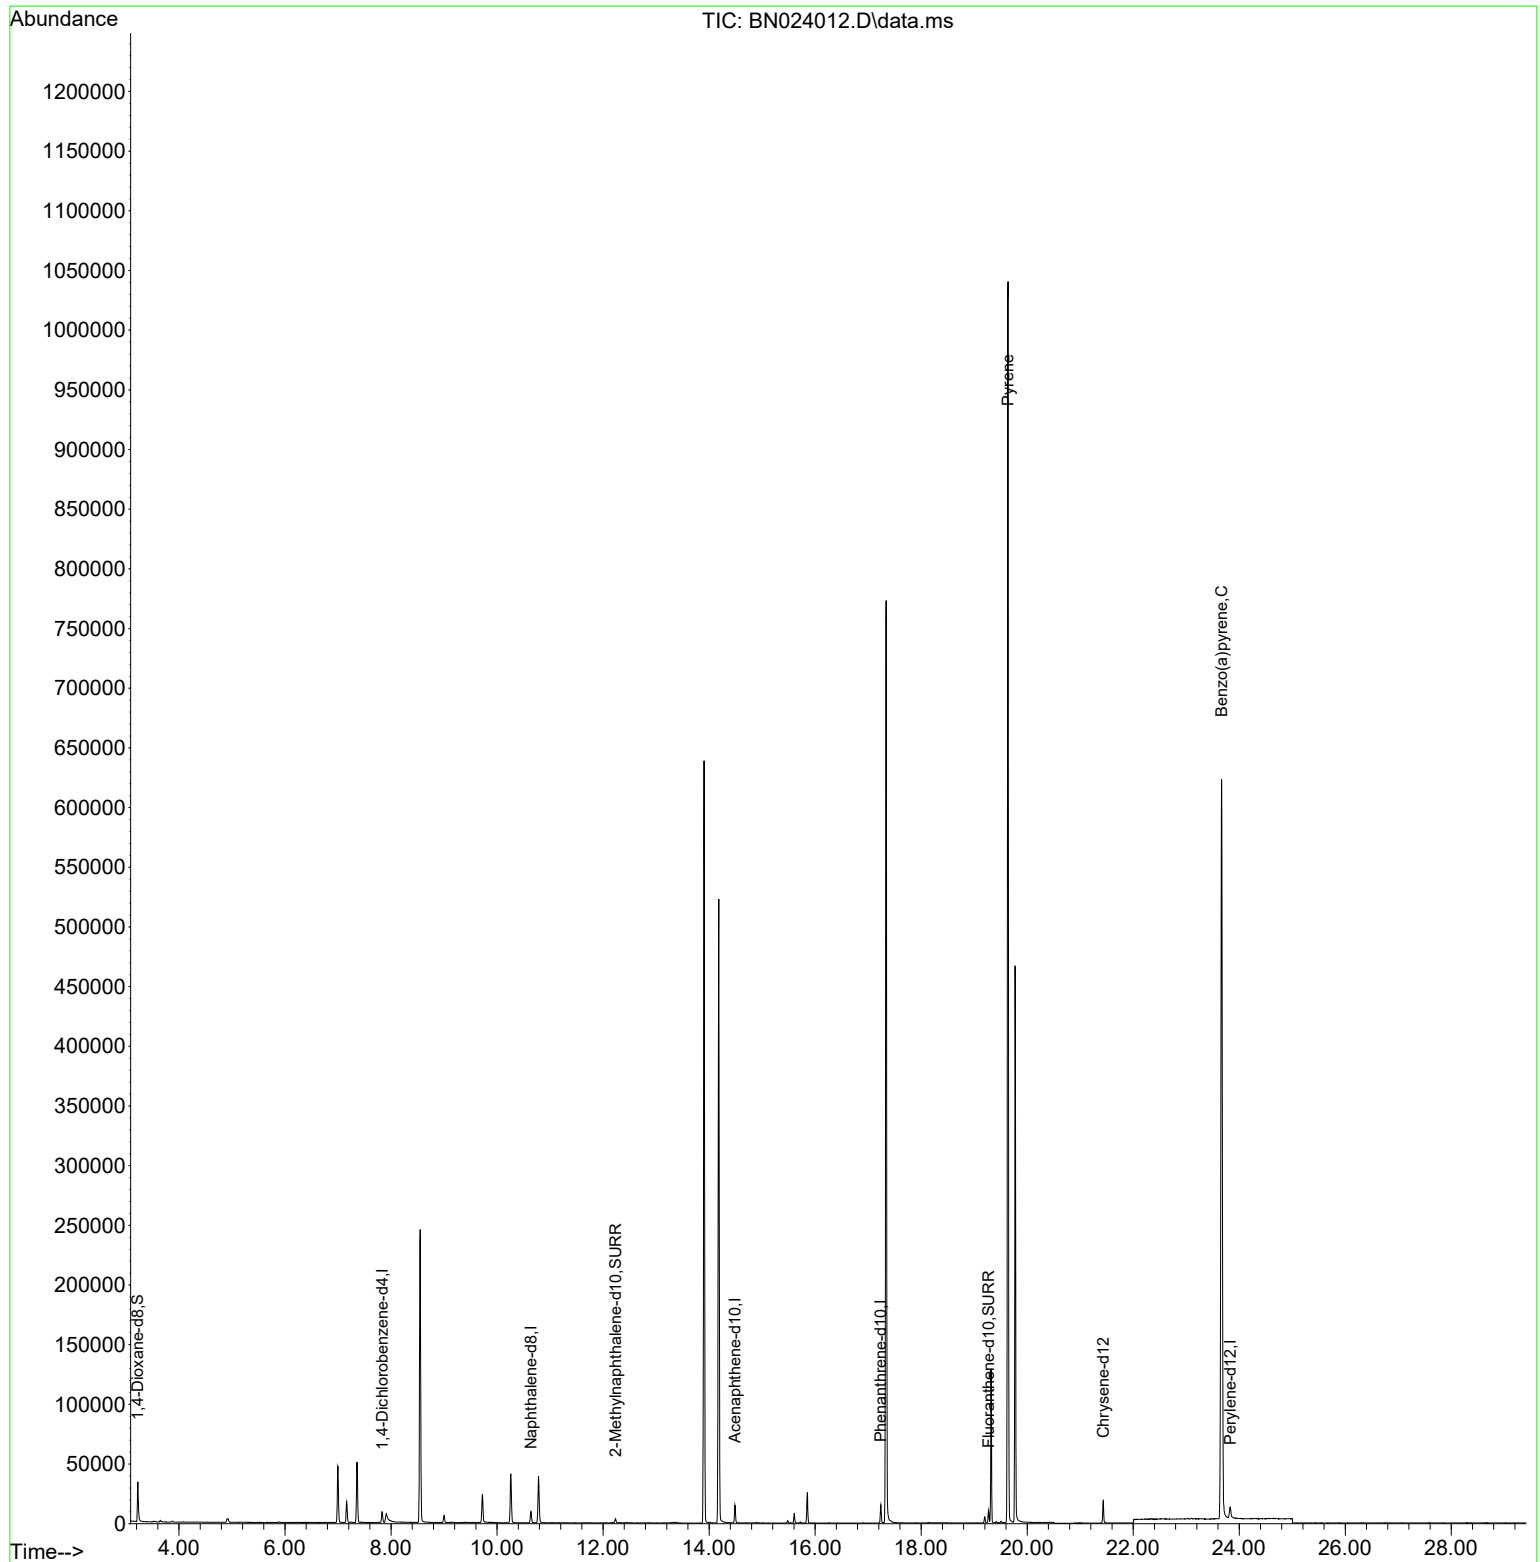



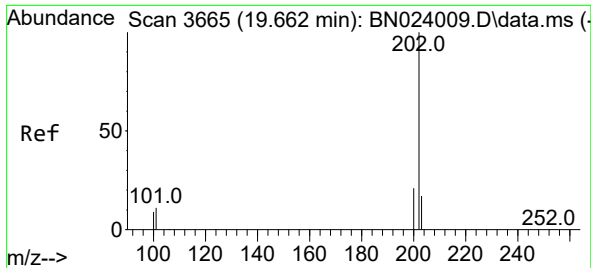


#20
Pyrene
Concen: 0.034 ng/ul
RT: 19.634 min Scan# 3659
Delta R.T. -0.028 min
Lab File: BN024012.D
Acq: 13 Feb 2023 14:12

Instrument :
BNA_N
ClientSampleId :

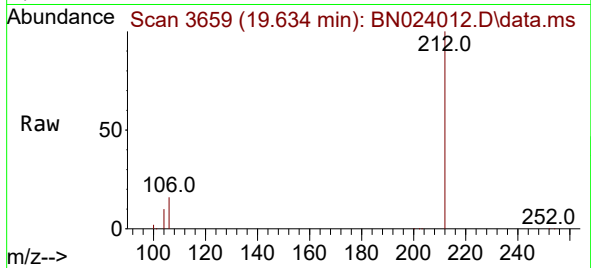

Tgt Ion:202 Resp: 1934
Ion Ratio Lower Upper
202 100
101 164.7 8.1 12.1#
100 1296.7 6.2 9.4#

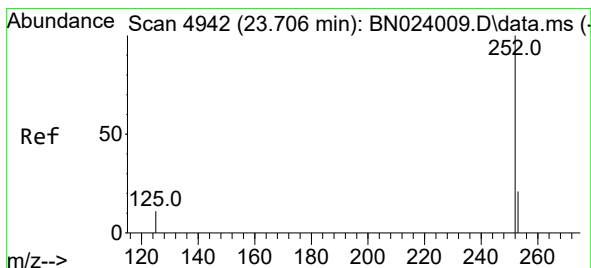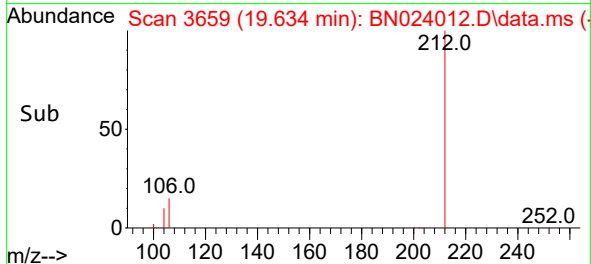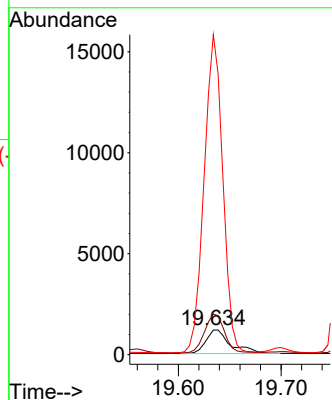

#26
Benzo(a)pyrene
Concen: 0.077 ng/ul
RT: 23.665 min Scan# 4928
Delta R.T. -0.041 min
Lab File: BN024012.D
Acq: 13 Feb 2023 14:12

Tgt Ion:252 Resp: 3620
Ion Ratio Lower Upper
252 100
253 51.5 21.5 32.3#
125 39.9 11.2 16.8#

