
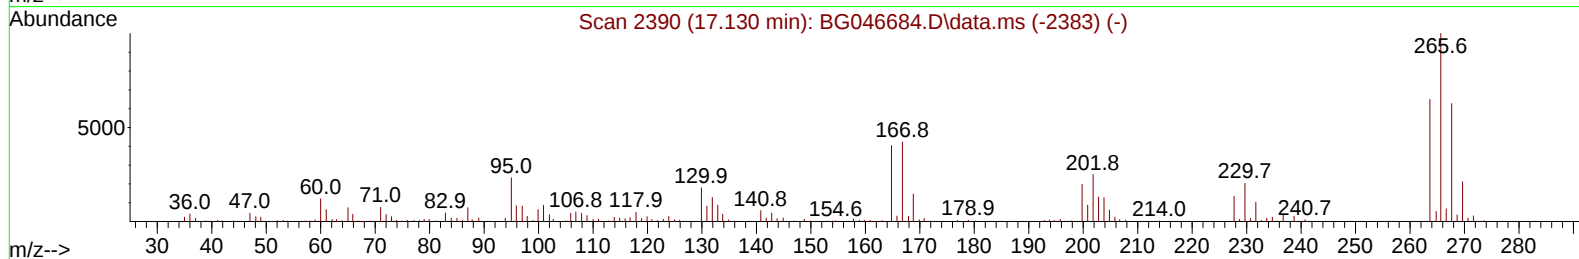
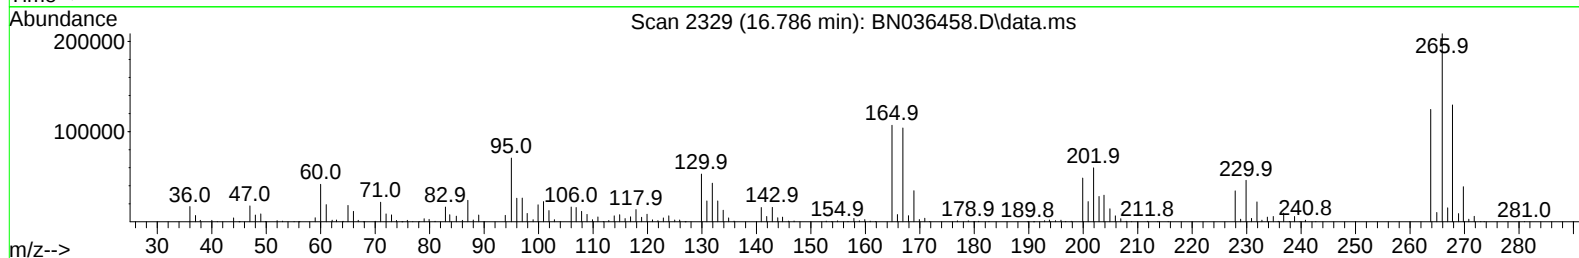


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021325\
Data File : BN036458.D
Acq On : 13 Feb 2025 09:09
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 13 11:56:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 23 16:55:25 2022
Response via : Initial Calibration

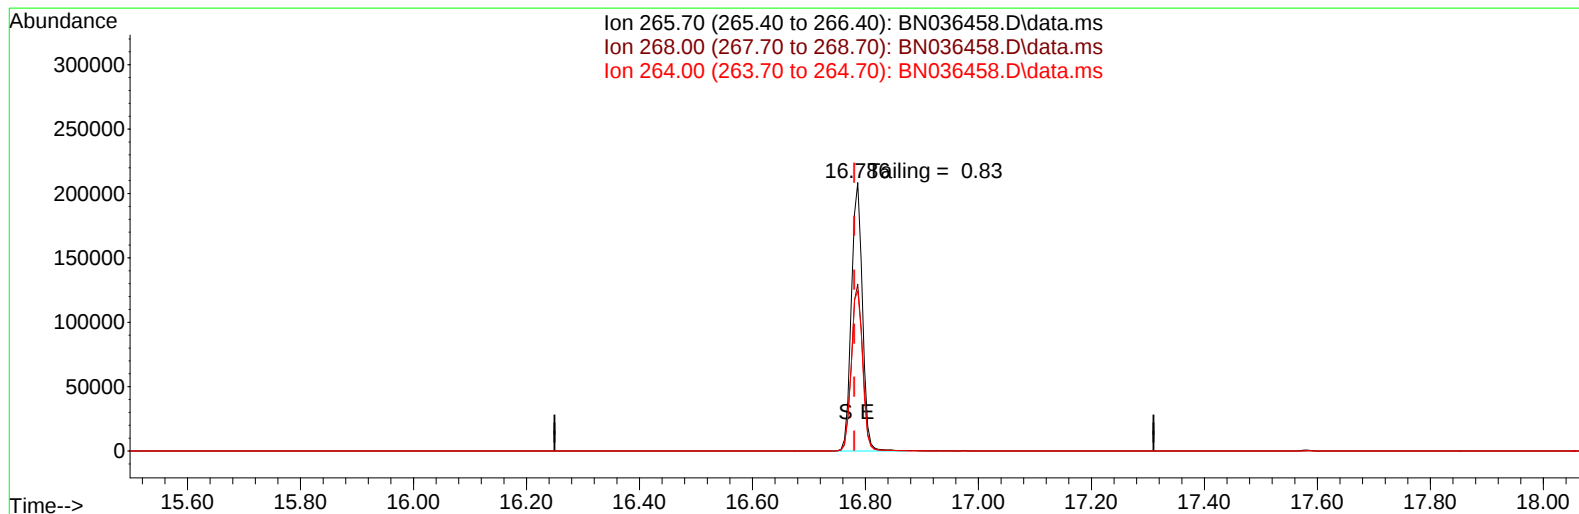

TIC: BN036458.D\data.ms

(70) Pentachlorophenol (C)




16.786min (+ 0.006) 658143.62 ng m

response 284072

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.17
264.00	61.60	59.74
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021325\
Data File : BN036458.D
Acq On : 13 Feb 2025 09:09
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 13 11:56:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 23 16:55:25 2022
Response via : Initial Calibration

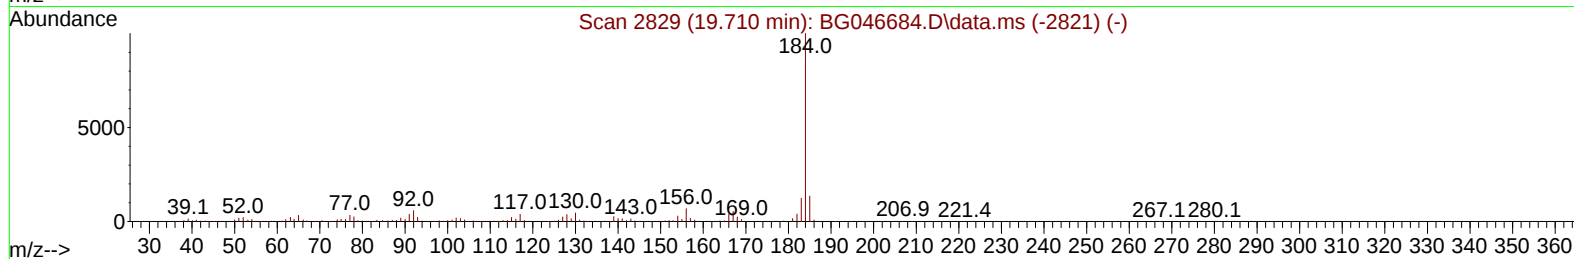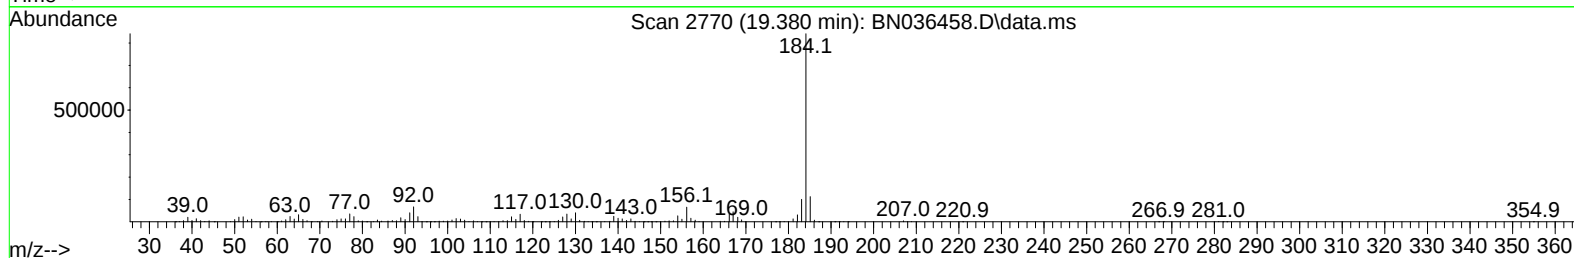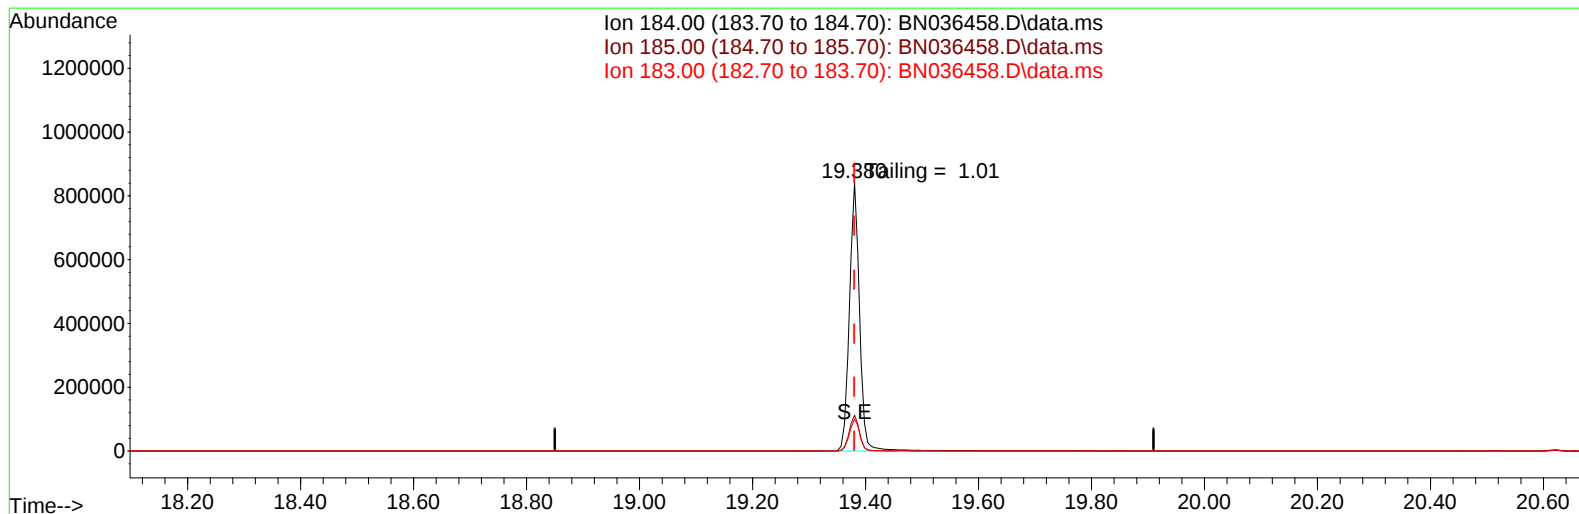

TIC: BN036458.D\data.ms

(77) Benzidine

19.380min (+ 0.000) 2563.43 ng m

response 1053317

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.38
183.00	13.20	11.96
0.00	0.00	0.00