


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021325\
Data File : BN036458.D
Acq On : 13 Feb 2025 09:09
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN021025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Feb 11 01:17:14 2025

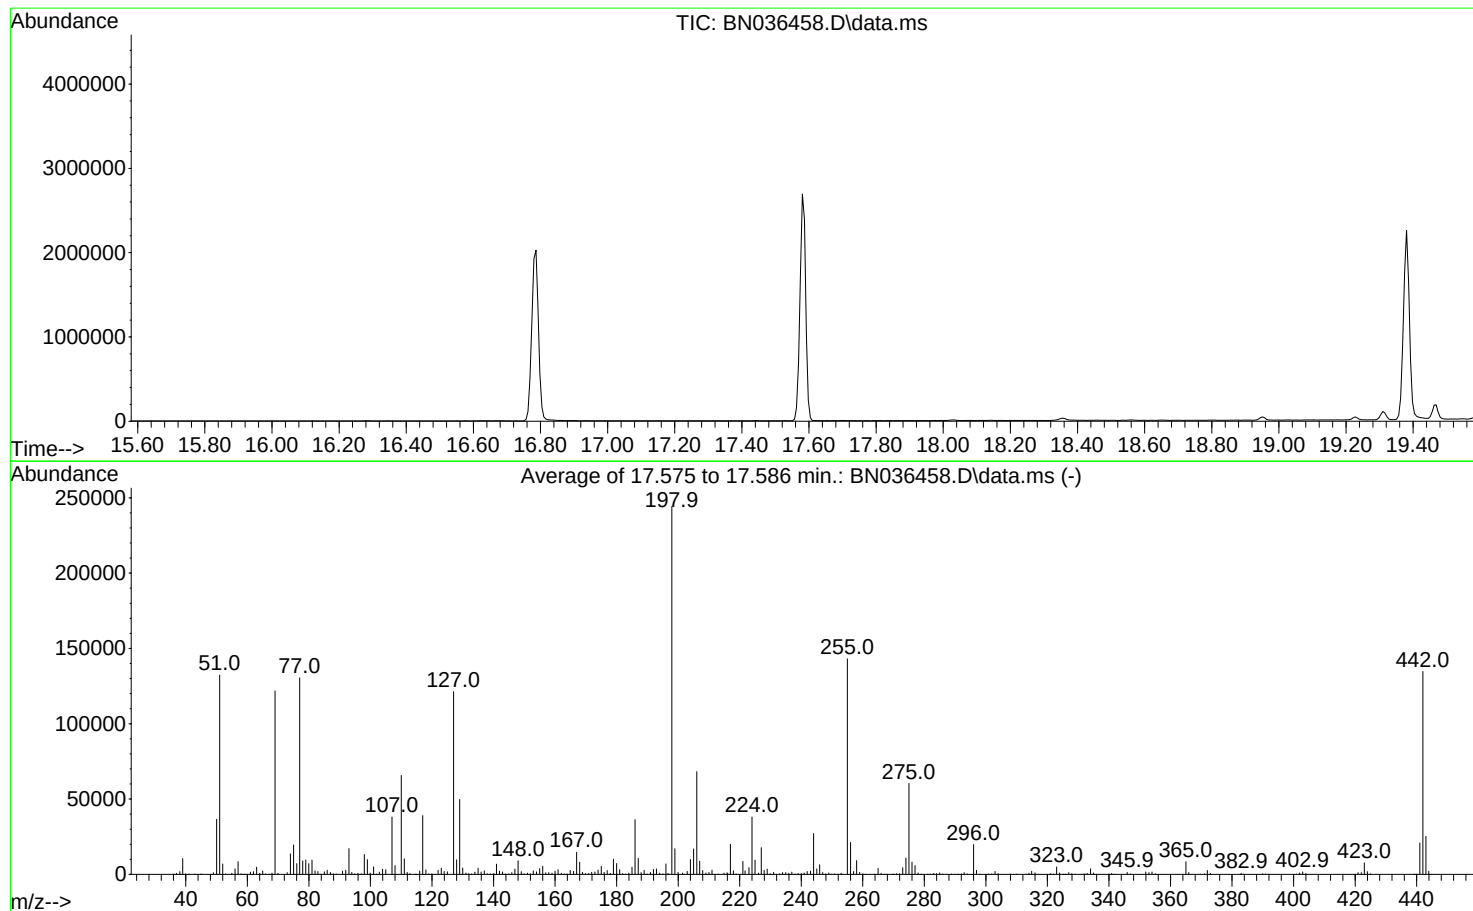




AutoFind: Scans 2463, 2464, 2465; Background Corrected with Scan 2456

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.1	132211	PASS
68	69	0.00	2	0.7	808	PASS
69	198	0.00	100	49.9	121872	PASS
70	69	0.00	2	0.5	594	PASS
127	198	10	80	49.7	121365	PASS
197	198	0.00	2	0.3	688	PASS
198	198	100	100	100.0	244224	PASS
199	198	5	9	7.0	17053	PASS
275	198	10	60	24.7	60405	PASS
365	198	1	100	3.5	8451	PASS
441	198	0.01	100	8.5	20871	PASS
442	442	50	100	100.0	134749	PASS
443	442	15	24	18.8	25291	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021325\
Data File : BN036458.D
Acq On : 13 Feb 2025 09:09
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Feb 13 11:56:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 23 16:55:25 2022
Response via : Initial Calibration

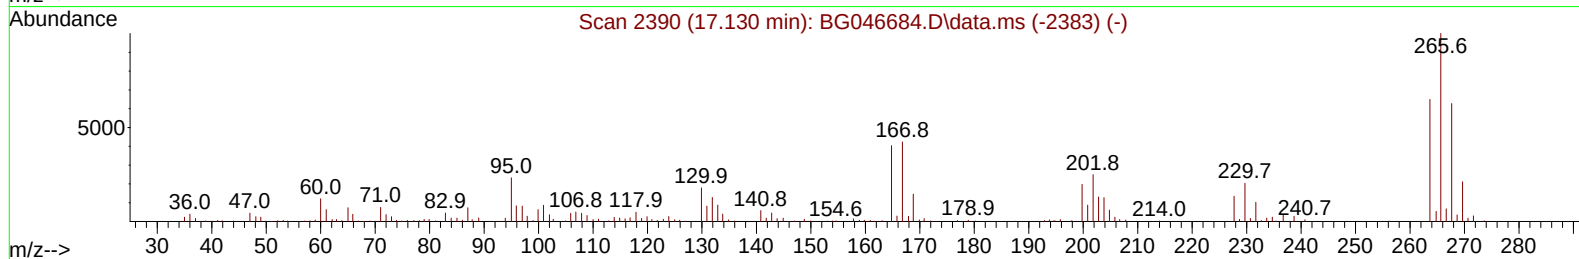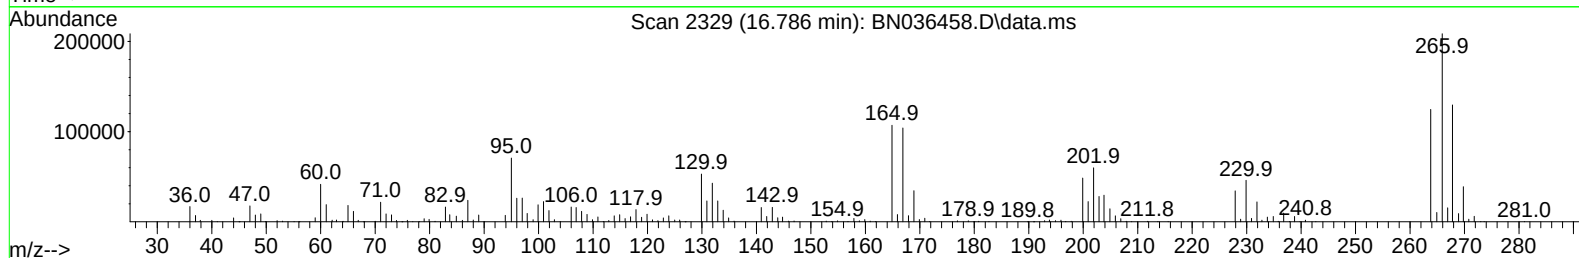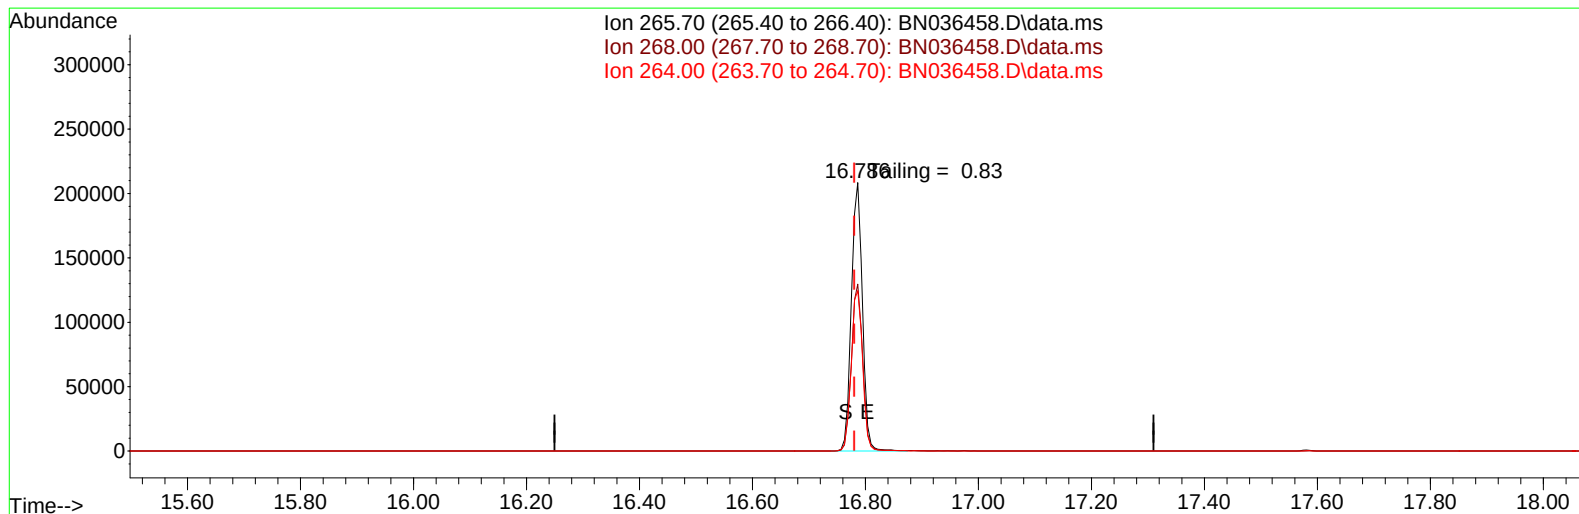

TIC: BN036458.D\data.ms

(70) Pentachlorophenol (C)

16.786min (+ 0.006) 658143.62 ng m




response 284072

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.17
264.00	61.60	59.74
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021325\
Data File : BN036458.D
Acq On : 13 Feb 2025 09:09
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Feb 13 11:56:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 23 16:55:25 2022
Response via : Initial Calibration

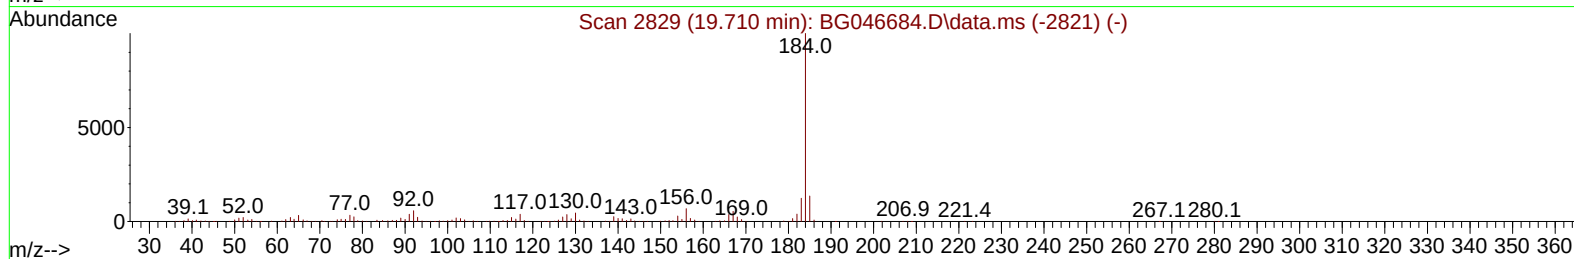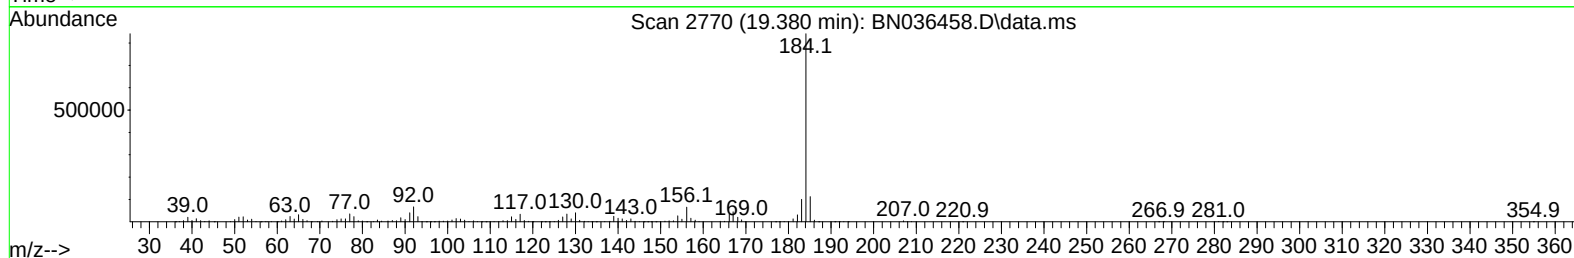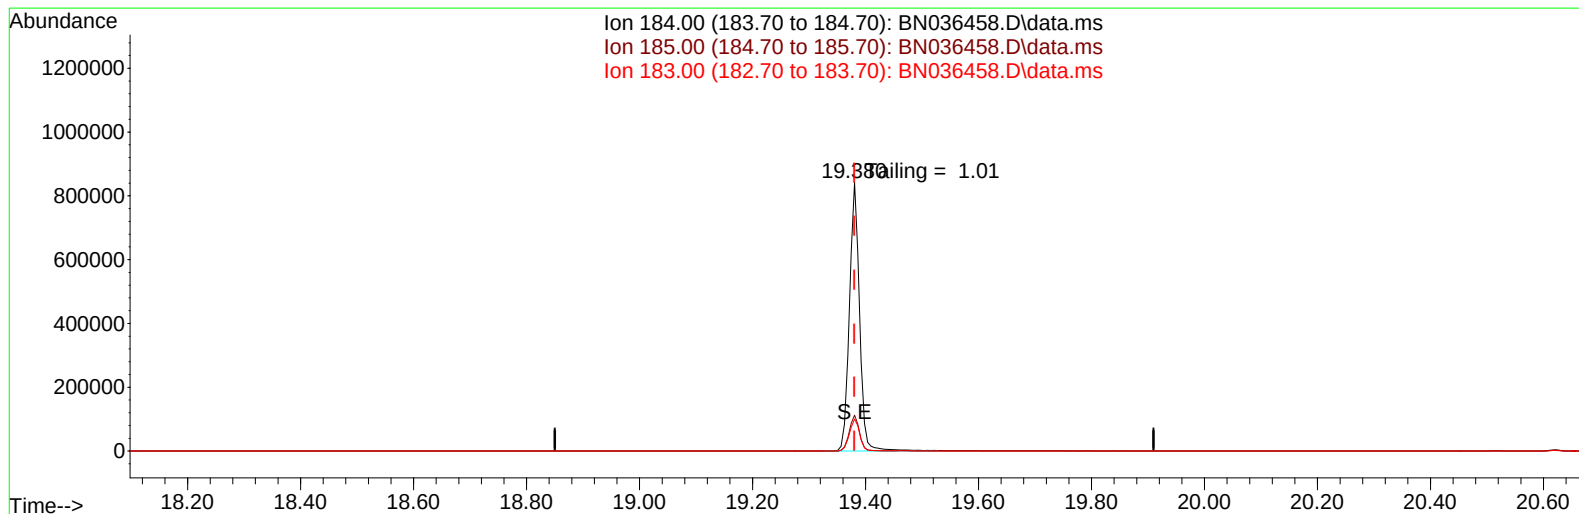

TIC: BN036458.D\data.ms

(77) Benzidine

19.380min (+ 0.000) 2563.43 ng m

response 1053317

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.38
183.00	13.20	11.96
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/13/2025	BNA_N	<u>BN036458.D</u>
Compound Name	Response	Retention Time
DDT	917216	20.621
DDD	11860	20.233
DDE	151	19.669
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12011	929227	1.29

Instrument :
BNA_N
ClientSampleId :
DFTPP