

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021424\
 Data File : BN029776.D
 Acq On : 14 Feb 2024 19:04
 Operator : MA/JU
 Sample : P1289-16
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AG5

Quant Time: Feb 14 22:25:48 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 13 22:50:45 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.869	152	173545	20.000	ng/ul	0.00
20) Naphthalene-d8	10.663	136	714479	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.510	164	375561	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.263	188	769145	20.000	ng/ul	0.00
79) Chrysene-d12	21.463	240	689610	20.000	ng/ul	0.00
88) Perylene-d12	23.833	264	783976	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.322	96	16818	3.187	ng/uL	0.00
4) Pyridine-d5	3.734	84	133724	9.504	ng/ul	0.00
7) Phenol-d5	7.040	99	101964	6.281	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.210	67	346165	31.953	ng/ul	0.00
11) 2-Chlorophenol-d4	7.399	132	315529	26.824	ng/ul	0.00
15) 4-Methylphenol-d8	8.581	113	194809	16.092	ng/ul	0.00
21) Nitrobenzene-d5	9.034	128	201768	36.386	ng/ul	0.00
24) 2-Nitrophenol-d4	9.751	143	188356	39.001	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.287	165	312469	32.779	ng/ul	0.00
31) 4-Chloroaniline-d4	10.810	131	485674	29.864	ng/ul	0.00
46) Dimethylphthalate-d6	13.934	166	1039346	37.171	ng/ul	0.00
49) Acenaphthylene-d8	14.204	160	1198975	36.108	ng/ul	0.00
54) 4-Nitrophenol-d4	14.722	143	25895	4.879	ng/ul	0.00
60) Fluorene-d10	15.510	176	867550	36.472	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.633	200	117025	31.226	ng/ul	0.00
73) Anthracene-d10	17.363	188	1364047	37.841	ng/ul	0.00
81) Pyrene-d10	19.663	212	1579144	38.158	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.680	264	1613699	41.135	ng/ul	0.00
Target Compounds						
					Qvalue	
16) Acetophenone	8.699	105	21675	1.125	ng/ul	97
59) Diethylphthalate	15.345	149	59363	2.019	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021424\
Data File : BN029776.D
Acq On : 14 Feb 2024 19:04
Operator : MA/JU
Sample : P1289-16
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AG5

Quant Time: Feb 14 22:25:48 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 13 22:50:45 2024
Response via : Initial Calibration




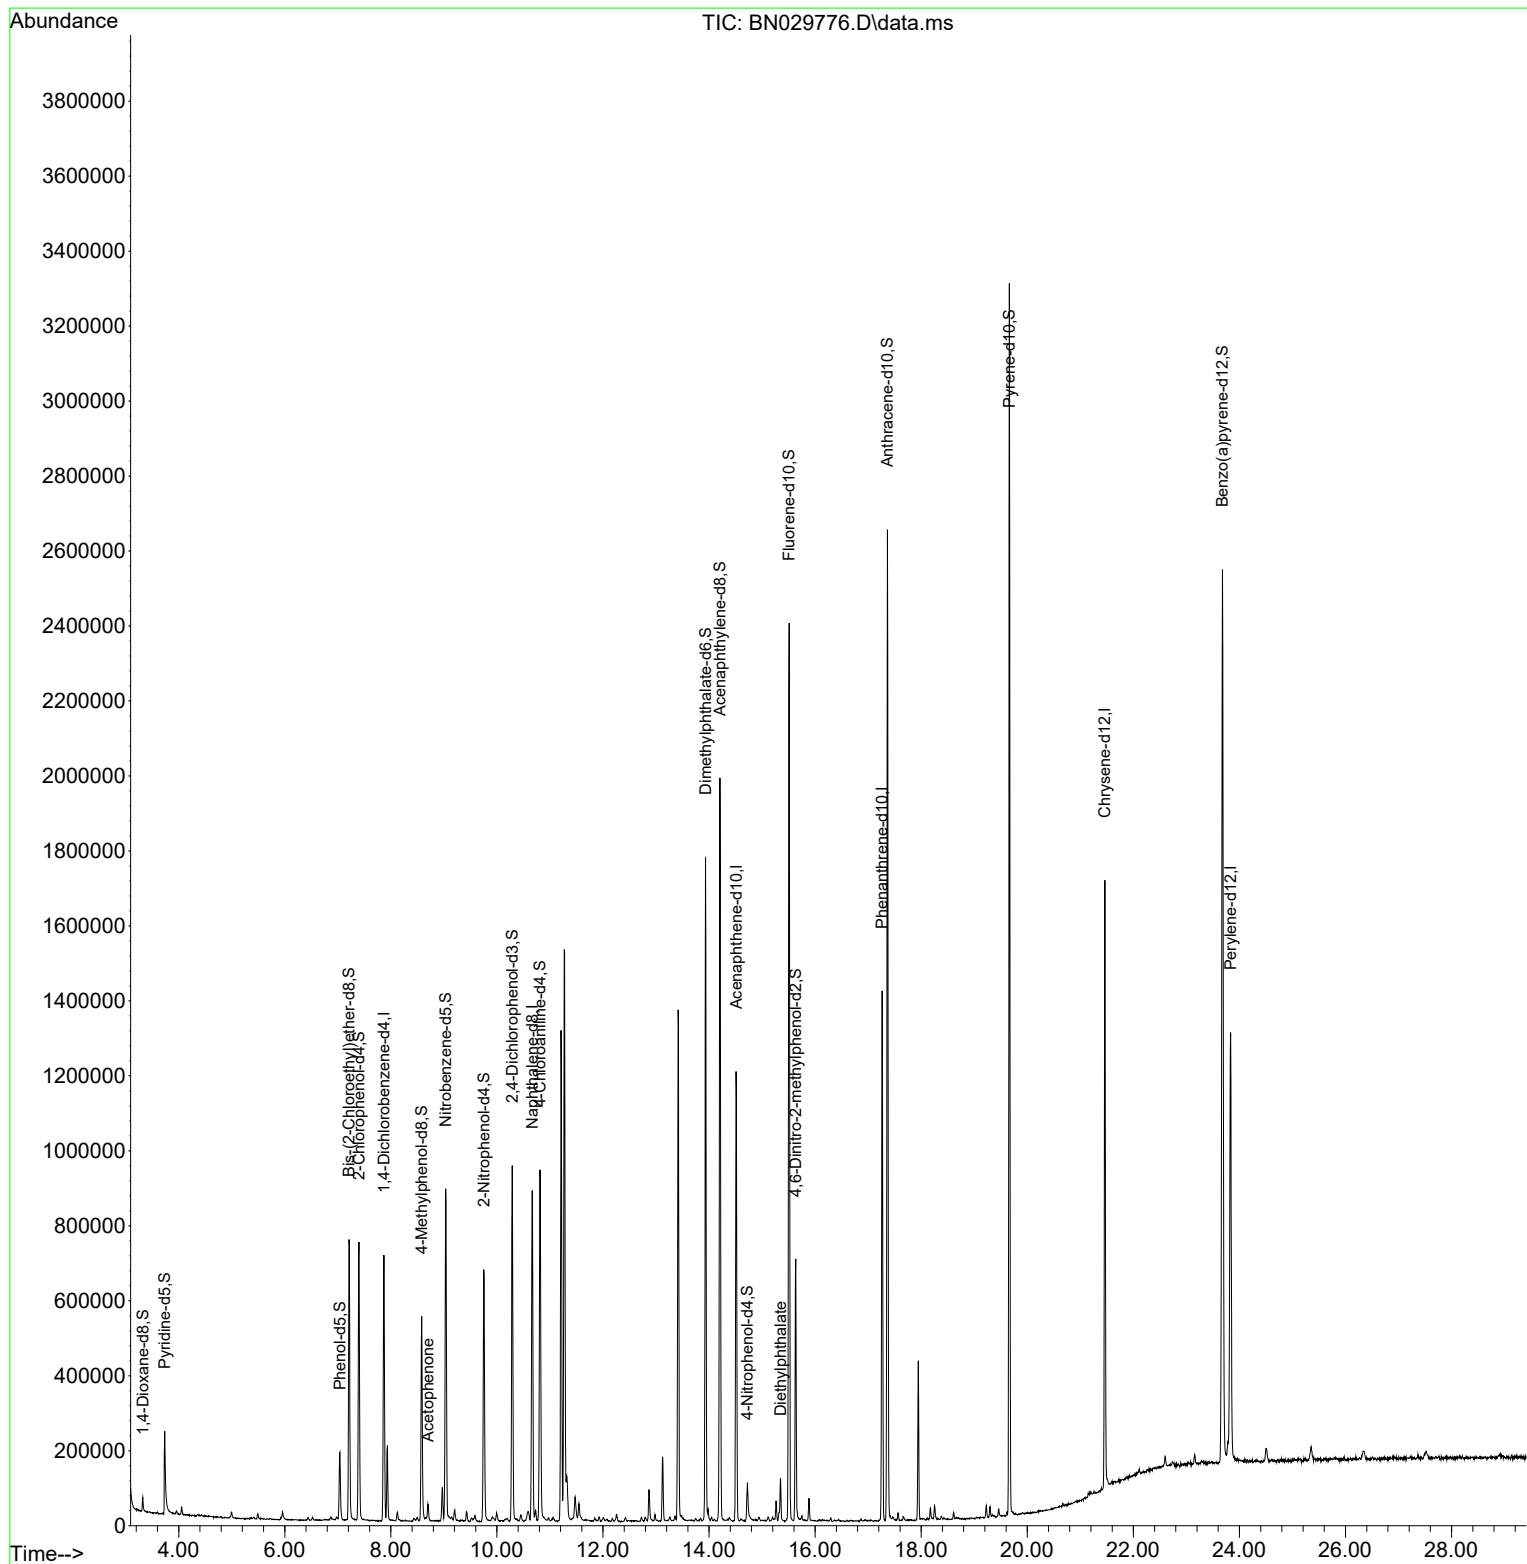


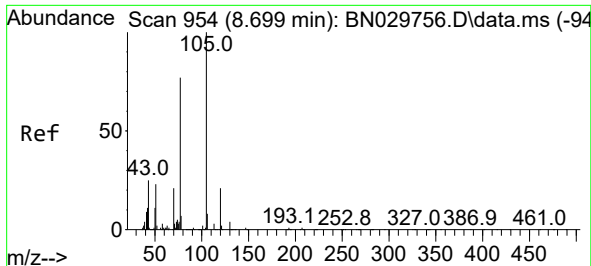

#16
Acetophenone
Concen: 1.125 ng/ul
RT: 8.699 min Scan# 91
Delta R.T. -0.000 min
Lab File: BN029776.D
Acq: 14 Feb 2024 19:04

Instrument :
BNA_N
ClientSampleId :
C0AG5

Tgt Ion:105 Resp: 21675
Ion Ratio Lower Upper
105 100
77 86.8 67.4 101.0
51 26.6 20.7 31.1

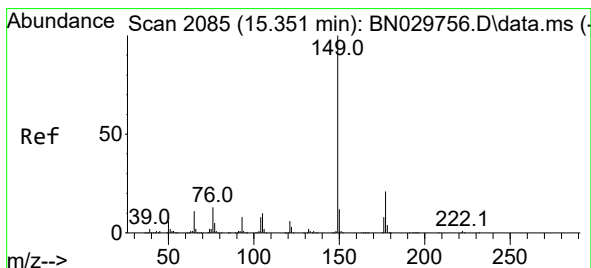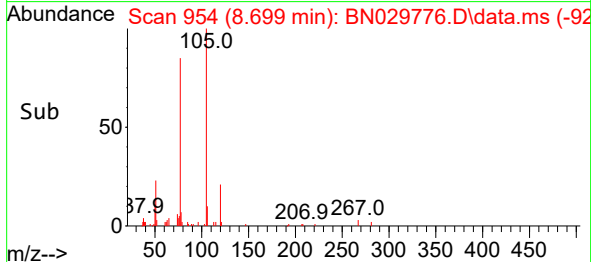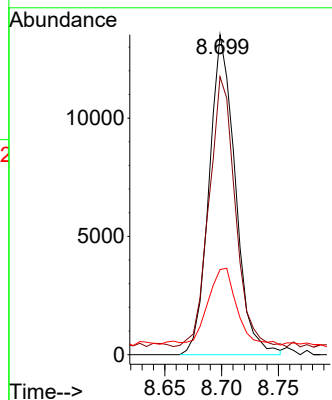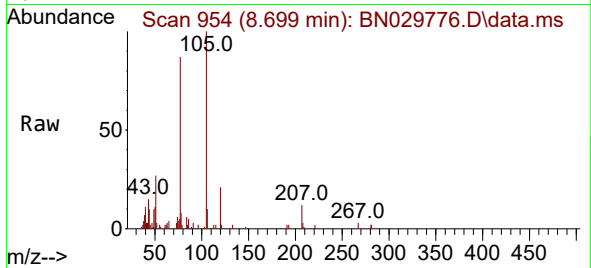

#59
Diethylphthalate
Concen: 2.019 ng/ul
RT: 15.345 min Scan# 2084
Delta R.T. -0.006 min
Lab File: BN029776.D
Acq: 14 Feb 2024 19:04

Tgt Ion:149 Resp: 59363
Ion Ratio Lower Upper
149 100
177 19.6 15.8 23.6
150 11.7 9.6 14.4

