

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021424\
 Data File : BN029778.D
 Acq On : 14 Feb 2024 20:16
 Operator : MA/JU
 Sample : P1299-02
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH6Z6

Quant Time: Feb 14 22:26:12 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 13 22:50:45 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.869	152	154760	20.000	ng/ul	0.00
20) Naphthalene-d8	10.663	136	630882	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.510	164	333362	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.263	188	686345	20.000	ng/ul	0.00
79) Chrysene-d12	21.463	240	634124	20.000	ng/ul	0.00
88) Perylene-d12	23.833	264	725916	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.317	96	27566	5.859	ng/uL	0.00
4) Pyridine-d5	3.734	84	169433	13.503	ng/ul	0.00
7) Phenol-d5	7.034	99	202823	14.011	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.210	67	387461	40.106	ng/ul	0.00
11) 2-Chlorophenol-d4	7.399	132	394179	37.578	ng/ul	0.00
15) 4-Methylphenol-d8	8.581	113	295817	27.402	ng/ul	0.00
21) Nitrobenzene-d5	9.034	128	222281	45.396	ng/ul	0.00
24) 2-Nitrophenol-d4	9.751	143	211716	49.647	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.287	165	358597	42.602	ng/ul	0.00
31) 4-Chloroaniline-d4	10.810	131	462733	32.223	ng/ul	0.00
46) Dimethylphthalate-d6	13.934	166	1146710	46.203	ng/ul	0.00
49) Acenaphthylene-d8	14.204	160	1288489	43.715	ng/ul	0.00
54) 4-Nitrophenol-d4	14.722	143	53148	11.283	ng/ul	0.00
60) Fluorene-d10	15.510	176	943516	44.687	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.634	200	134197	40.127	ng/ul	0.00
73) Anthracene-d10	17.363	188	1432604	44.538	ng/ul	0.00
81) Pyrene-d10	19.663	212	1683119	44.229	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.680	264	1740172	47.907	ng/ul	0.00
Target Compounds						
48) 2,6-Dinitrotoluene	13.940	165	7996	1.759	ng/ul#	Qvalue 36


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021424\
Data File : BN029778.D
Acq On : 14 Feb 2024 20:16
Operator : MA/JU
Sample : P1299-02
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH6Z6

Quant Time: Feb 14 22:26:12 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 13 22:50:45 2024
Response via : Initial Calibration

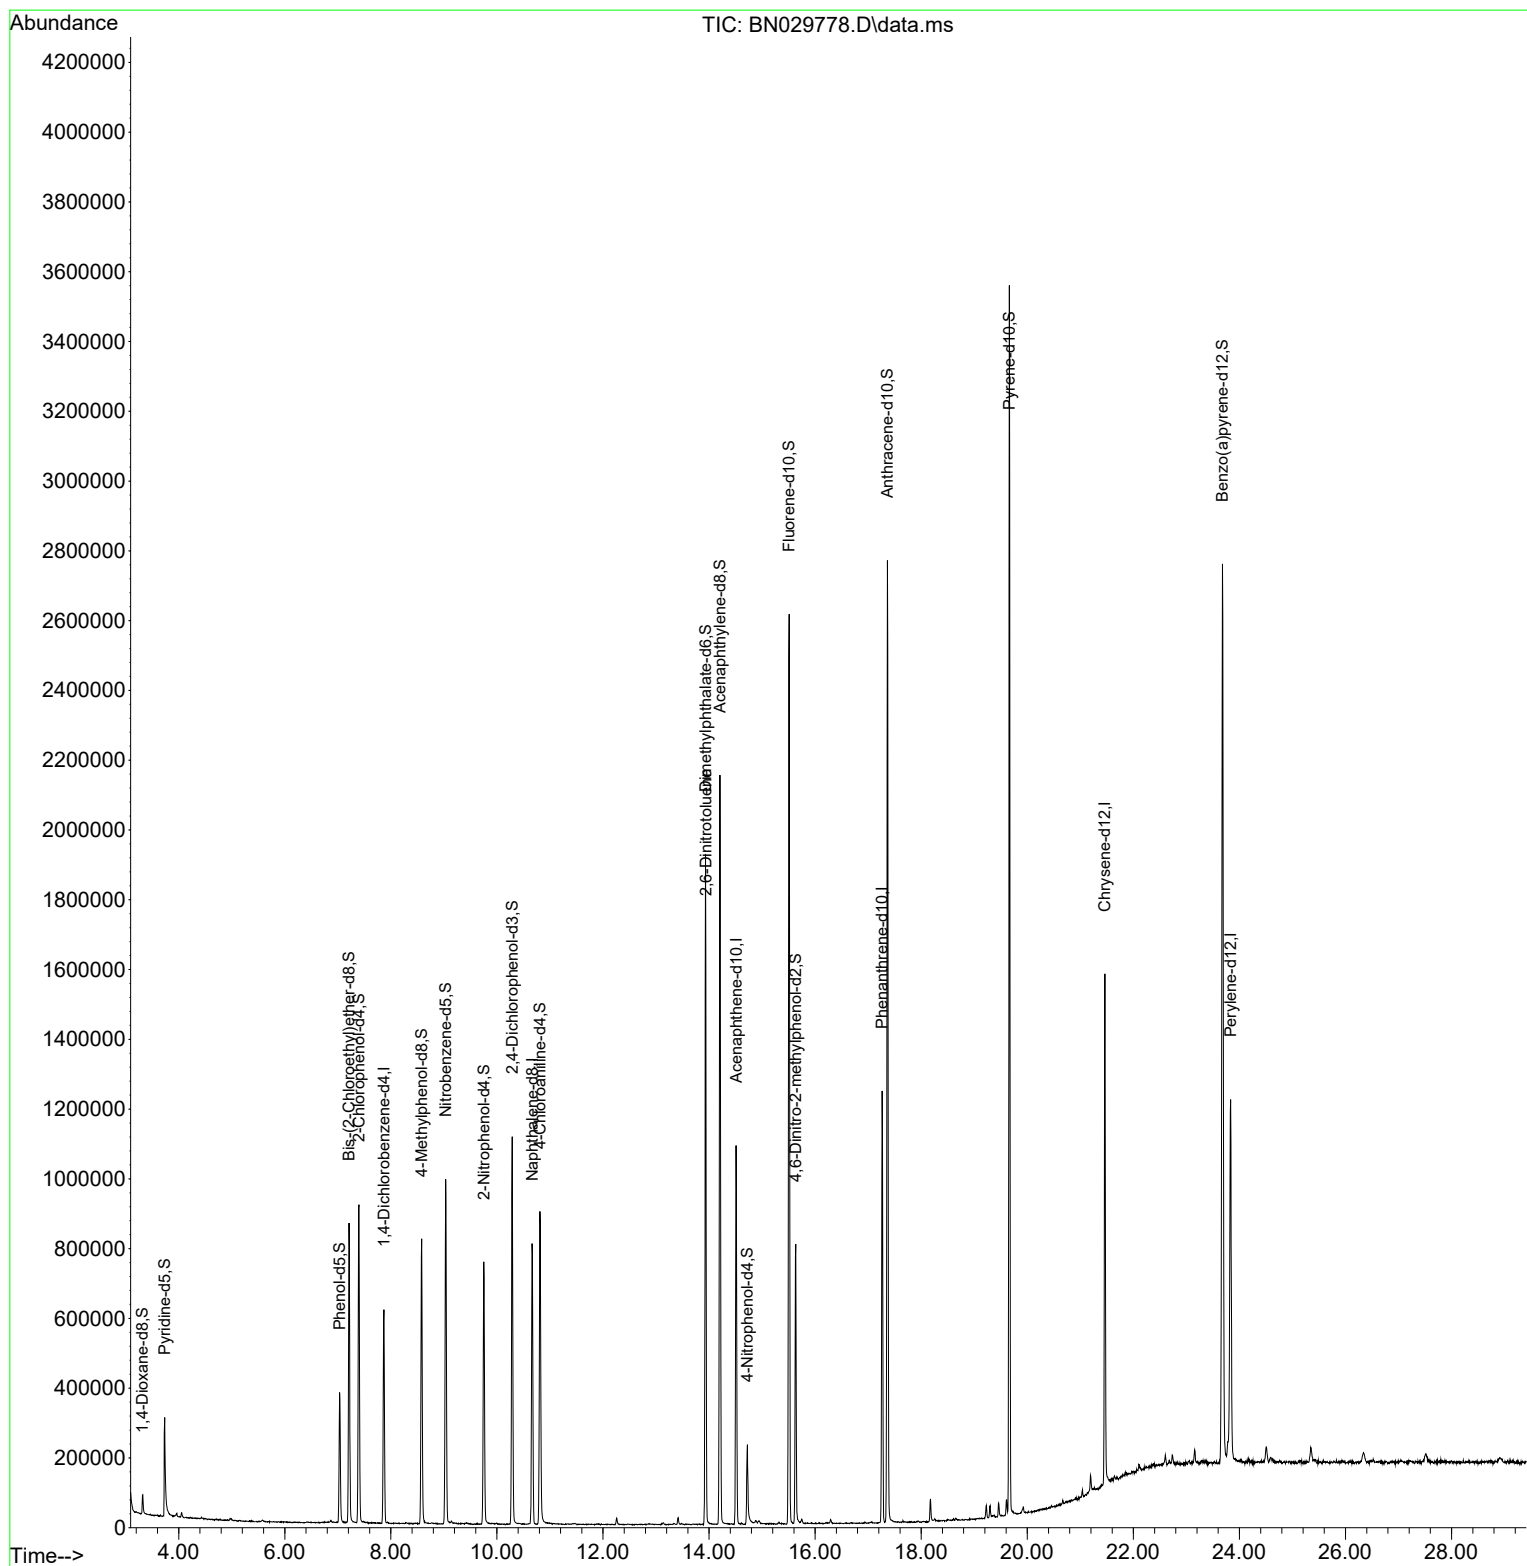

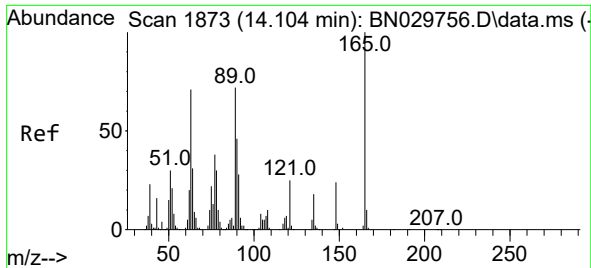

#48
 2,6-Dinitrotoluene
 Concen: 1.759 ng/ul
 RT: 13.940 min Scan# 11
 Delta R.T. -0.171 min
 Lab File: BN029778.D
 Acq: 14 Feb 2024 20:16

Instrument :
 BNA_N
 ClientSampleId :
 BH6Z6

Tgt Ion	Ratio	Lower	Upper
165	100		
89	0.0	55.8	83.8#
121	27.5	19.8	29.6

