

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021424\
 Data File : BN029779.D
 Acq On : 14 Feb 2024 20:52
 Operator : MA/JU
 Sample : P1299-03
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH6Z7

Quant Time: Feb 14 22:26:24 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 13 22:50:45 2024
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.869	152	166694	20.000	ng/ul	0.00
20) Naphthalene-d8	10.663	136	688656	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.510	164	359183	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.263	188	727622	20.000	ng/ul	0.00
79) Chrysene-d12	21.463	240	664989	20.000	ng/ul	0.00
88) Perylene-d12	23.833	264	754073	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.322	96	24699	4.874	ng/uL	0.00
4) Pyridine-d5	3.734	84	179874	13.309	ng/ul	0.00
7) Phenol-d5	7.034	99	182888	11.730	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.211	67	376725	36.203	ng/ul	0.00
11) 2-Chlorophenol-d4	7.393	132	374424	33.139	ng/ul	0.00
15) 4-Methylphenol-d8	8.581	113	277704	23.882	ng/ul	0.00
21) Nitrobenzene-d5	9.034	128	215067	40.238	ng/ul	0.00
24) 2-Nitrophenol-d4	9.752	143	205262	44.095	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.287	165	344798	37.526	ng/ul	0.00
31) 4-Chloroaniline-d4	10.810	131	427464	27.270	ng/ul	0.00
46) Dimethylphthalate-d6	13.934	166	1085689	40.599	ng/ul	0.00
49) Acenaphthylene-d8	14.204	160	1282108	40.372	ng/ul	0.00
54) 4-Nitrophenol-d4	14.722	143	43438	8.558	ng/ul	0.00
60) Fluorene-d10	15.510	176	933910	41.052	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.634	200	120110	33.878	ng/ul	0.00
73) Anthracene-d10	17.363	188	1385980	40.644	ng/ul	0.00
81) Pyrene-d10	19.663	212	1545610	38.731	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.680	264	1539852	40.809	ng/ul	0.00
Target Compounds						
48) 2,6-Dinitrotoluene	13.940	165	8105	1.655	ng/ul#	39


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021424\
Data File : BN029779.D
Acq On : 14 Feb 2024 20:52
Operator : MA/JU
Sample : P1299-03
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH6Z7

Quant Time: Feb 14 22:26:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 13 22:50:45 2024
Response via : Initial Calibration

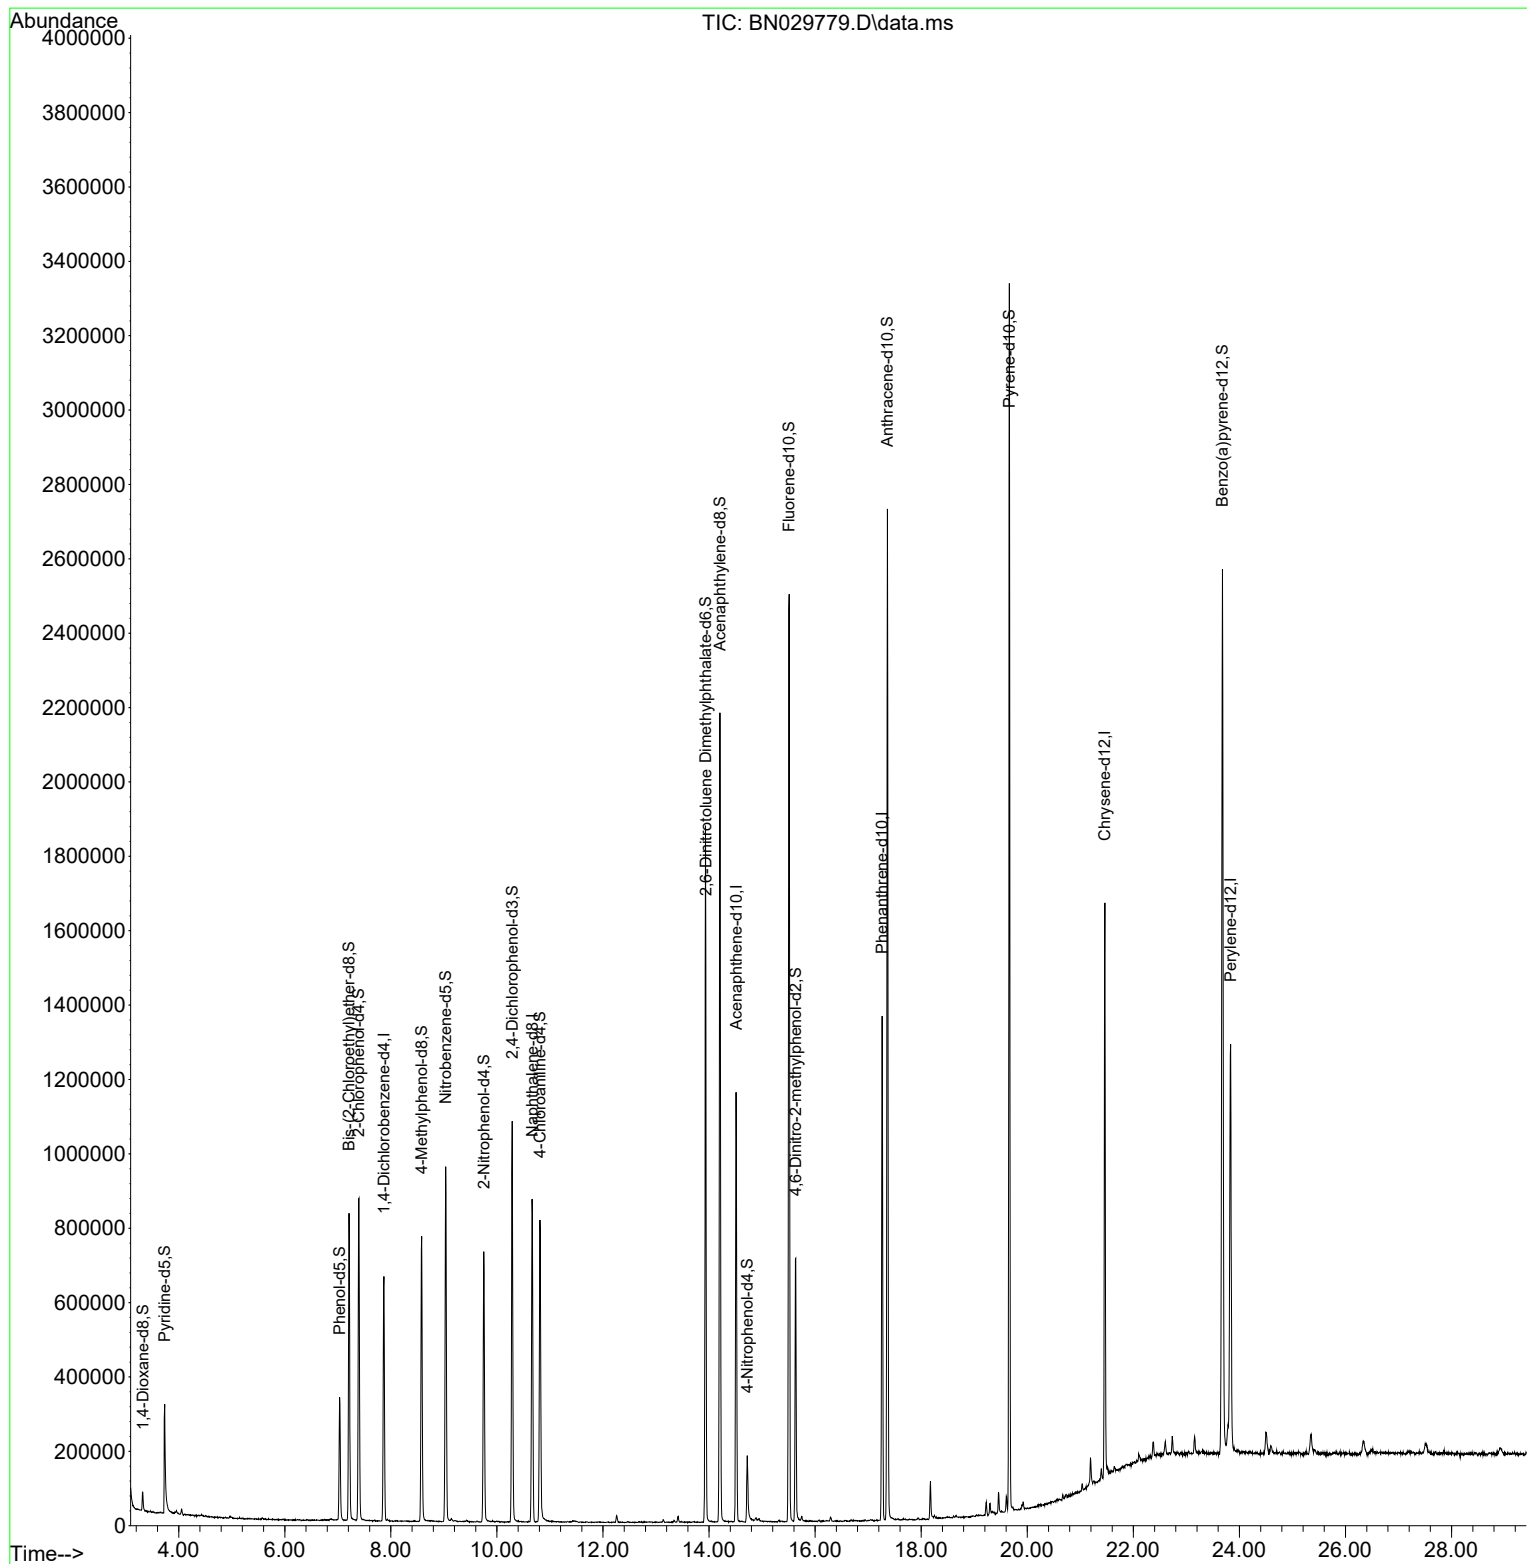

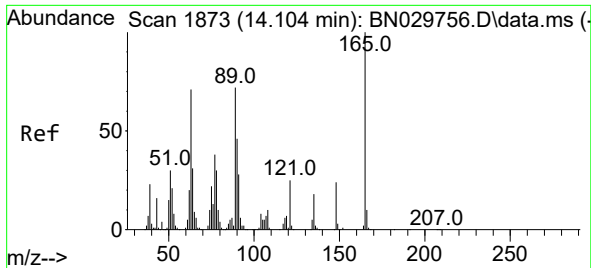

#48
 2,6-Dinitrotoluene
 Concen: 1.655 ng/ul
 RT: 13.940 min Scan# 11
 Delta R.T. -0.171 min
 Lab File: BN029779.D
 Acq: 14 Feb 2024 20:52

Instrument :
 BNA_N
 ClientSampleId :
 BH6Z7

Tgt Ion:165 Resp: 8105
 Ion Ratio Lower Upper
 165 100
 89 2.8 55.8 83.8#
 121 26.6 19.8 29.6

