

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021424\
 Data File : BN029821.D
 Acq On : 16 Feb 2024 10:21
 Operator : MA/JU
 Sample : PB158885TB 10X
 Misc :
 ALS Vial : 102 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SLEB885

Quant Time: Feb 17 04:45:27 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 13 22:50:45 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.864	152	178120	20.000	ng/ul	0.00
20) Naphthalene-d8	10.663	136	733733	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.510	164	396357	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.263	188	826243	20.000	ng/ul	0.00
79) Chrysene-d12	21.463	240	772738	20.000	ng/ul	0.00
88) Perylene-d12	23.833	264	866951	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.317	96	42594	7.865	ng/uL	0.00
4) Pyridine-d5	3.728	84	555656	38.475	ng/ul	0.00
7) Phenol-d5	7.034	99	710933	42.672	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.211	67	450879	40.550	ng/ul	0.00
11) 2-Chlorophenol-d4	7.393	132	559781	46.366	ng/ul	0.00
15) 4-Methylphenol-d8	8.575	113	550628	44.316	ng/ul	-0.01
21) Nitrobenzene-d5	9.034	128	276826	48.611	ng/ul	0.00
24) 2-Nitrophenol-d4	9.752	143	286671	57.800	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.287	165	474340	48.454	ng/ul	0.00
31) 4-Chloroaniline-d4	10.810	131	692312	41.453	ng/ul	0.00
46) Dimethylphthalate-d6	13.934	166	1428521	48.409	ng/ul	0.00
49) Acenaphthylene-d8	14.204	160	1660542	47.384	ng/ul	0.00
54) 4-Nitrophenol-d4	14.722	143	245973	43.918	ng/ul	0.00
60) Fluorene-d10	15.504	176	1188656	47.349	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.634	200	176188	43.763	ng/ul	0.00
73) Anthracene-d10	17.363	188	1839333	47.500	ng/ul	0.00
81) Pyrene-d10	19.663	212	2103097	45.352	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.680	264	2131582	49.136	ng/ul	0.00


Target Compounds					Qvalue
17) N-Nitroso-di-n-propyla...	8.575	70	15517	1.520 ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021424\
Data File : BN029821.D
Acq On : 16 Feb 2024 10:21
Operator : MA/JU
Sample : PB158885TB 10X
Misc :
ALS Vial : 102 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SLEB885


Quant Time: Feb 17 04:45:27 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 13 22:50:45 2024
Response via : Initial Calibration

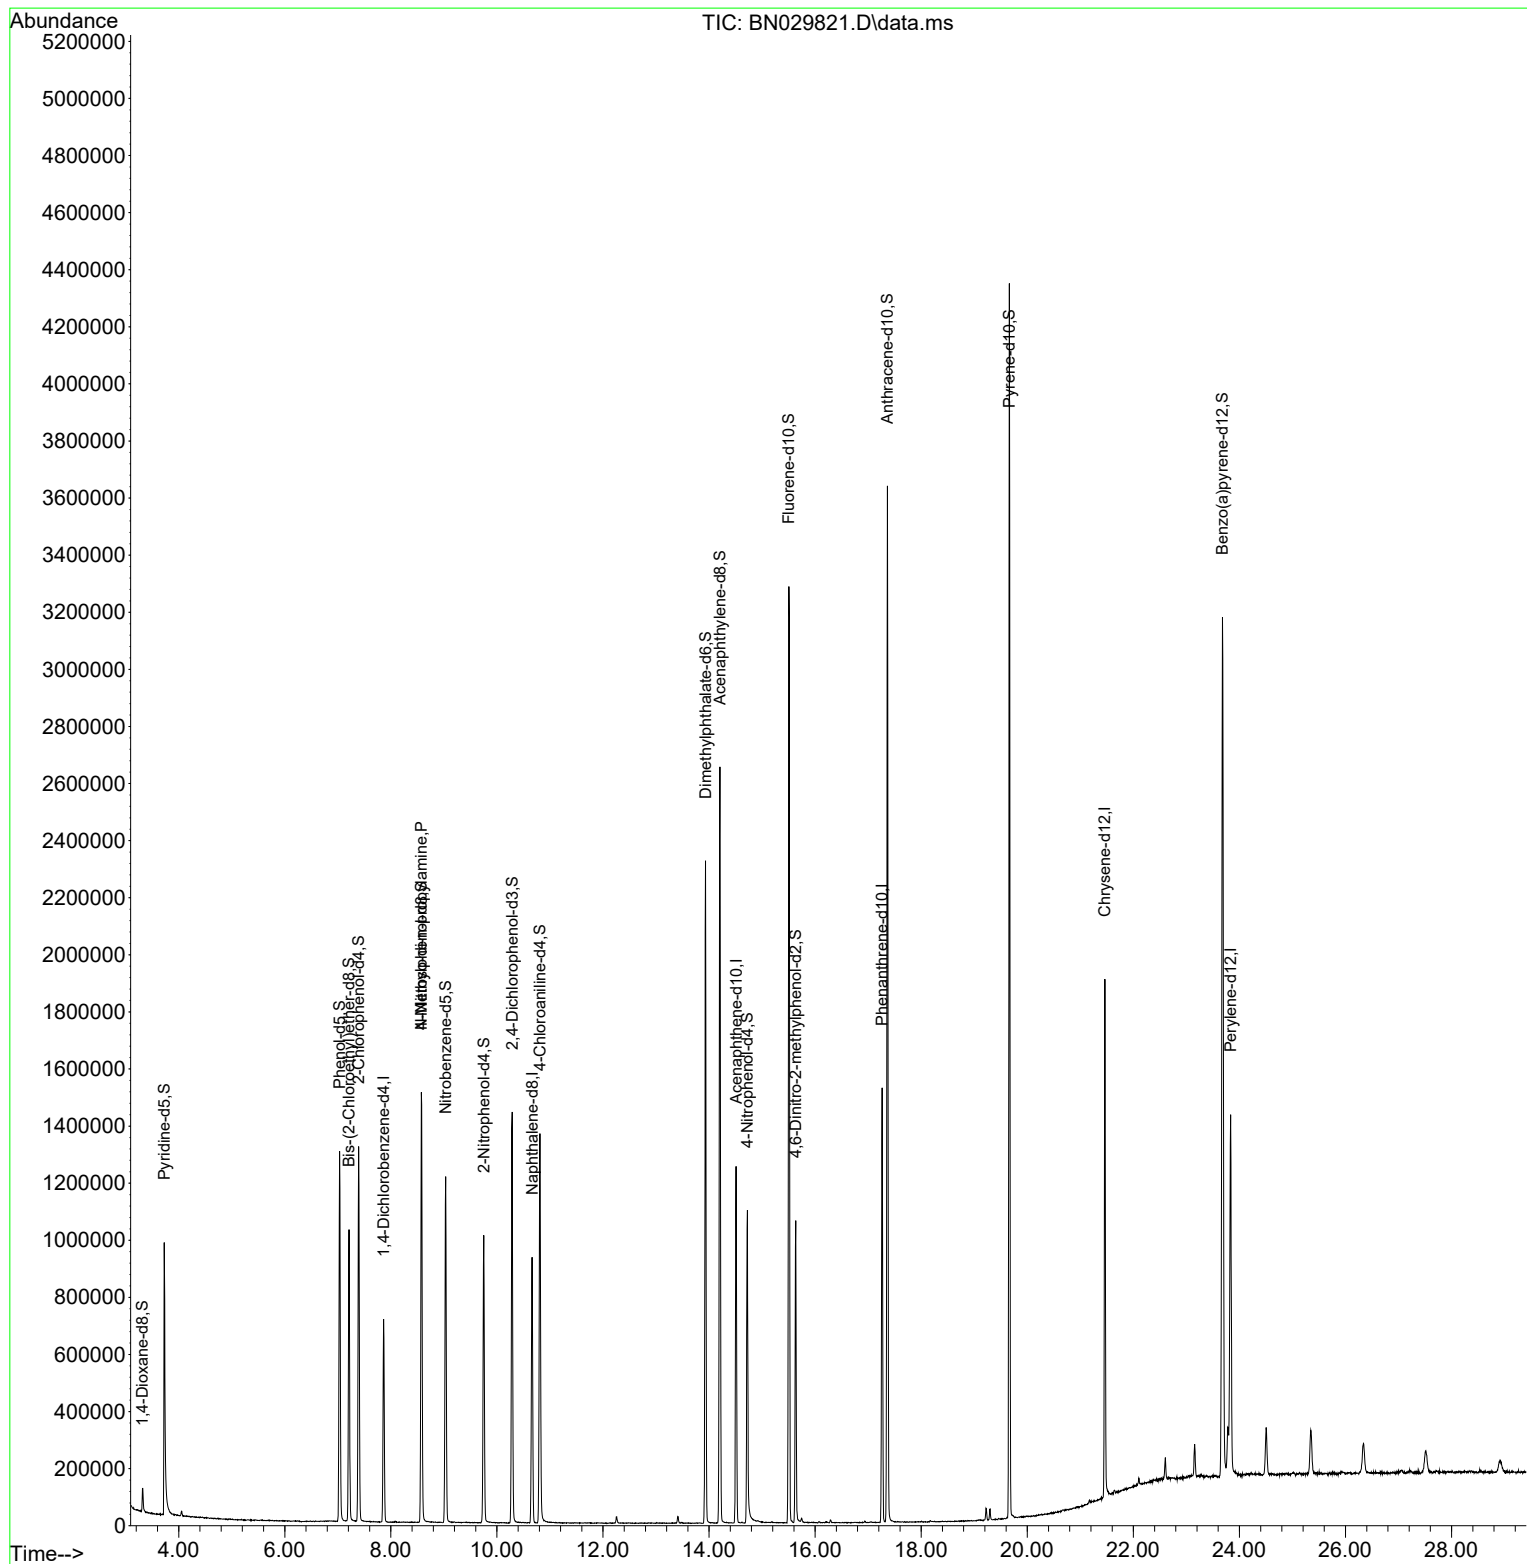

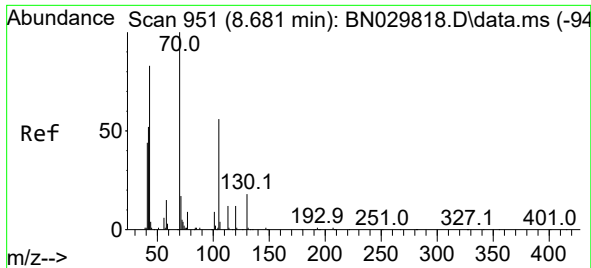

#17
N-Nitroso-di-n-propylamine
Concen: 1.520 ng/ul
RT: 8.575 min Scan# 91
Delta R.T. -0.112 min
Lab File: BN029821.D
Acq: 16 Feb 2024 10:21

Instrument :
BNA_N
ClientSampleId :
SLEB885

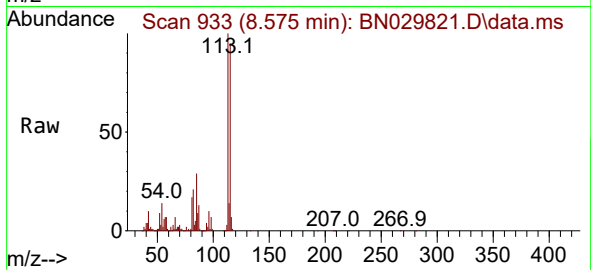

Tgt Ion:	70	Resp:	15517
Ion	Ratio	Lower	Upper
70	100		
42	352.9	43.0	64.4#
101	0.0	7.4	11.2#
130	0.0	15.1	22.7#

