




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021424\
Data File : BN029820.D
Acq On : 16 Feb 2024 09:45
Operator : MA/JU
Sample : SSTDCCC020
Misc :
ALS Vial : 101 Sample Multiplier: 1

Instrument :
BNA_N
LabSampleId :
SSTDCCC020

Manual IntegrationsAPPROVED

Quant Time: Feb 17 04:44:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 13 22:50:45 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 02/19/2024
Supervised By :mohammad ahmed 02/19/2024

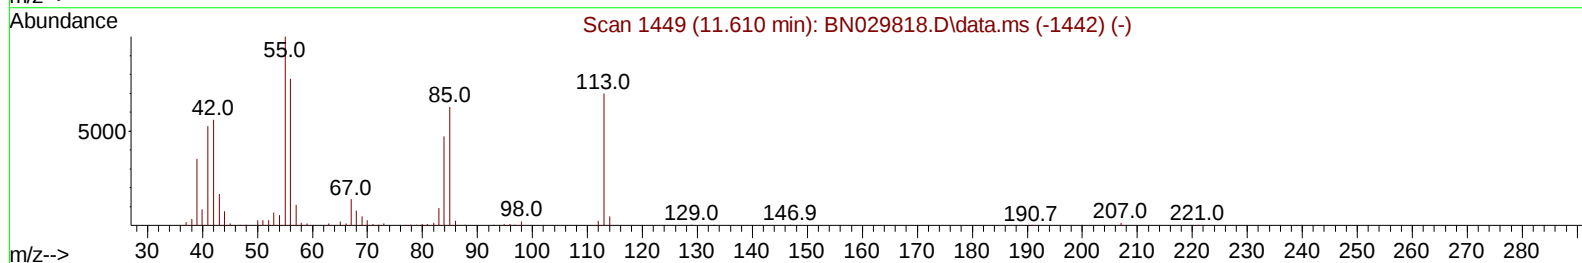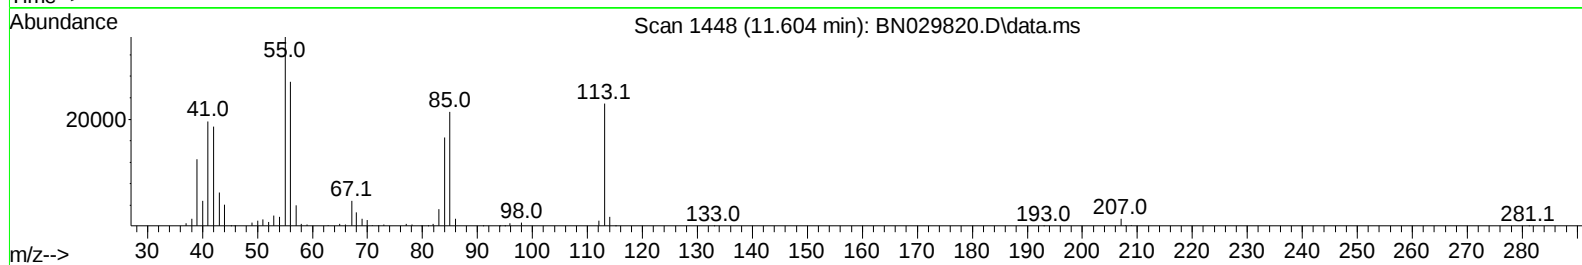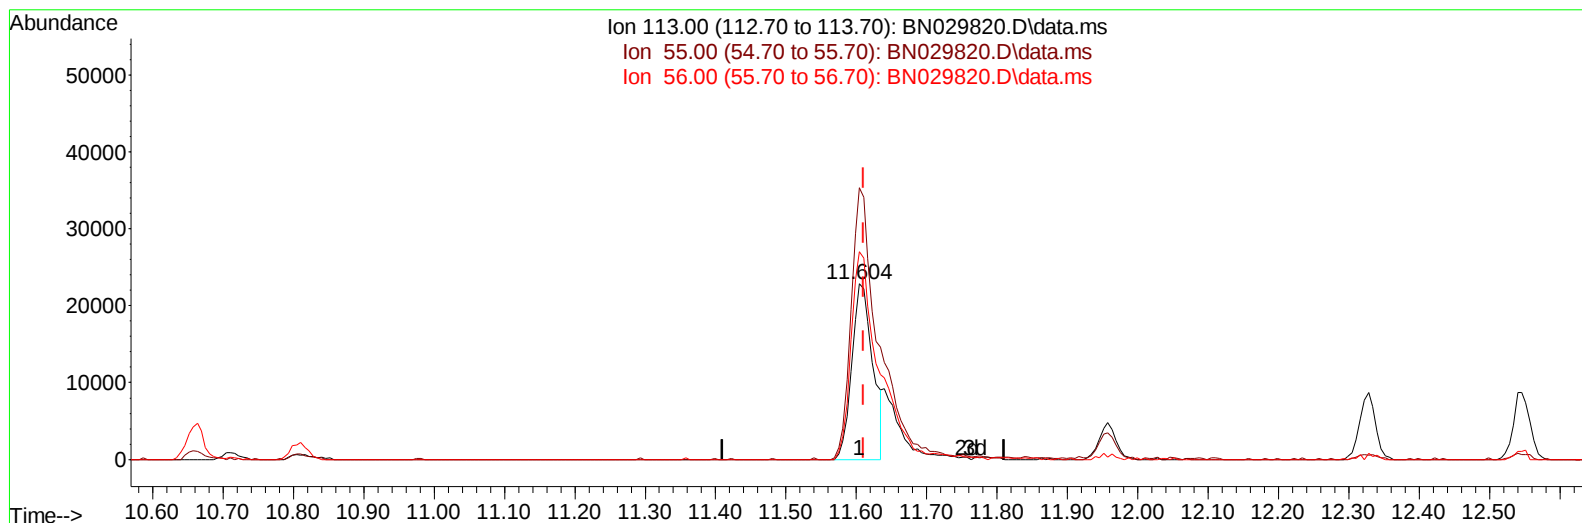

TIC: BN029820.D\data.ms

(34) Caprolactam

11.604min (-0.006) 14.74 ng/ul

response 46831

Ion	Exp%	Act%
113.00	100.00	100.00
55.00	156.60	154.39
56.00	129.20	118.08
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021424\
Data File : BN029820.D
Acq On : 16 Feb 2024 09:45
Operator : MA/JU
Sample : SSTDCCC020
Misc :
ALS Vial : 101 Sample Multiplier: 1

Instrument :
BNA_N
LabSampleId :
SSTDCCC020

Manual IntegrationsAPPROVED

Quant Time: Feb 17 04:44:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 13 22:50:45 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 02/19/2024
Supervised By :mohammad ahmed 02/19/2024

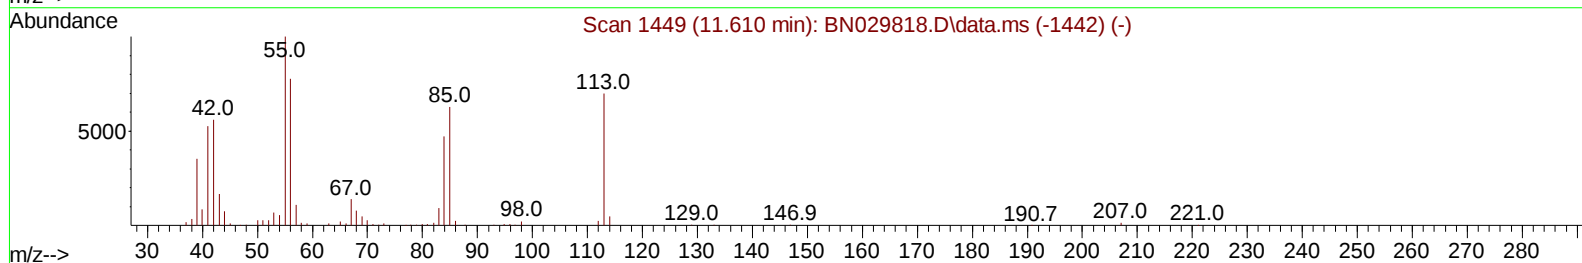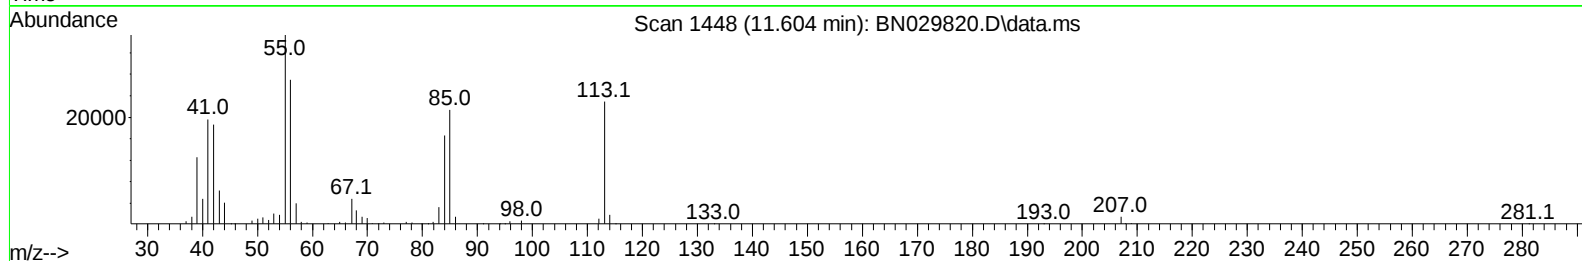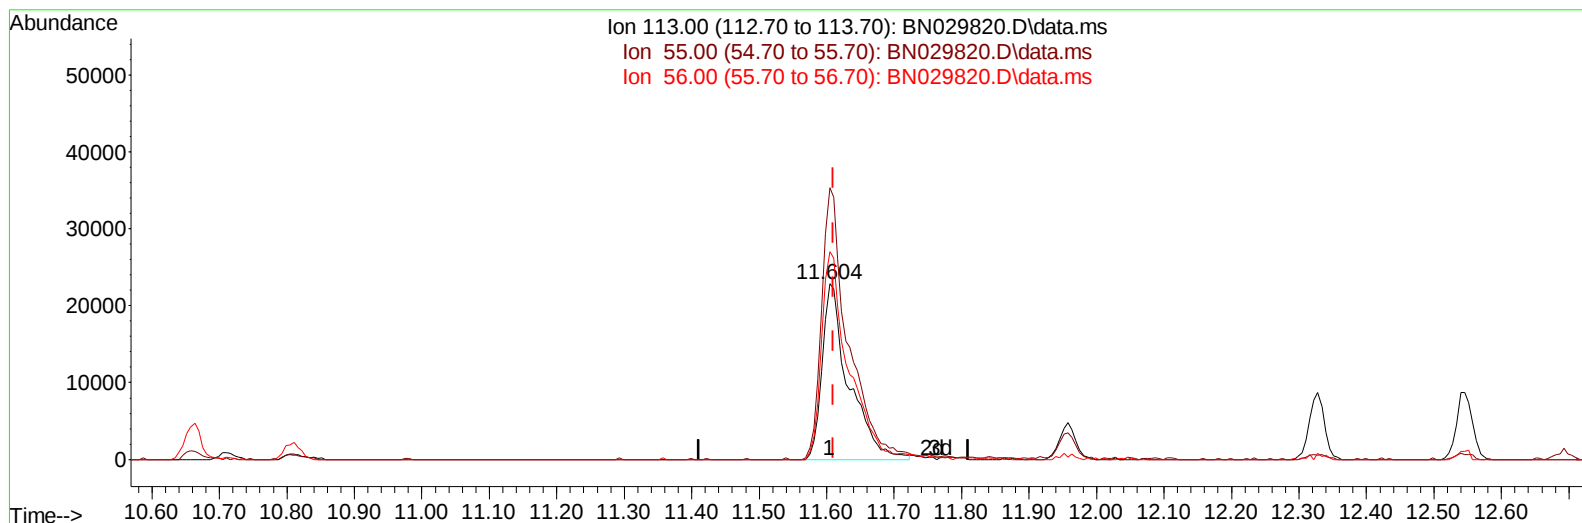

TIC: BN029820.D\data.ms

(34) Caprolactam

11.604min (-0.006) 19.63 ng/ul m

response 62376

Ion	Exp%	Act%
113.00	100.00	100.00
55.00	156.60	154.39
56.00	129.20	118.08
0.00	0.00	0.00

Instrument :
BNA_N
LabSampleId :
SSTDCCC020

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 02/19/2024
Supervised By :mohammad ahmed 02/19/2024

