

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021424\
 Data File : BN029752.D
 Acq On : 14 Feb 2024 03:28
 Operator : MA/JU
 Sample : P1286-05
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH6T4

Quant Time: Feb 14 03:55:06 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 13 22:50:45 2024
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.863	152	209732	20.000	ng/u1	0.00
20) Naphthalene-d8	10.663	136	837663	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.510	164	411331	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.263	188	790500	20.000	ng/u1	0.00
79) Chrysene-d12	21.463	240	704285	20.000	ng/u1	0.00
88) Perylene-d12	23.833	264	805803	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.317	96	26419	4.143	ng/uL	0.00
4) Pyridine-d5	3.728	84	225673	13.271	ng/u1	0.00
7) Phenol-d5	7.028	99	481439	24.541	ng/u1	-0.01
9) Bis-(2-Chloroethyl)eth...	7.205	67	331968	25.356	ng/u1	-0.01
11) 2-Chlorophenol-d4	7.393	132	379392	26.688	ng/u1	0.00
15) 4-Methylphenol-d8	8.575	113	244037	16.680	ng/u1	-0.01
21) Nitrobenzene-d5	9.028	128	181693	27.947	ng/u1	-0.01
24) 2-Nitrophenol-d4	9.752	143	169538	29.942	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.281	165	297010	26.575	ng/u1	-0.01
31) 4-Chloroaniline-d4	10.810	131	375457	19.692	ng/u1	0.00
46) Dimethylphthalate-d6	13.934	166	880364	28.748	ng/u1	0.00
49) Acenaphthylene-d8	14.204	160	1036527	28.501	ng/u1	0.00
54) 4-Nitrophenol-d4	14.716	143	120648	20.757	ng/u1	0.00
60) Fluorene-d10	15.504	176	759074	29.137	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.628	200	82684	21.466	ng/u1	0.00
73) Anthracene-d10	17.363	188	1043559	28.168	ng/u1	0.00
81) Pyrene-d10	19.663	212	1308286	30.955	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.686	264	1217814	30.203	ng/u1	0.00
Target Compounds						
16) Acetophenone	8.693	105	39189	1.683	ng/u1	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021424\
Data File : BN029752.D
Acq On : 14 Feb 2024 03:28
Operator : MA/JU
Sample : P1286-05
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH6T4

Quant Time: Feb 14 03:55:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 13 22:50:45 2024
Response via : Initial Calibration

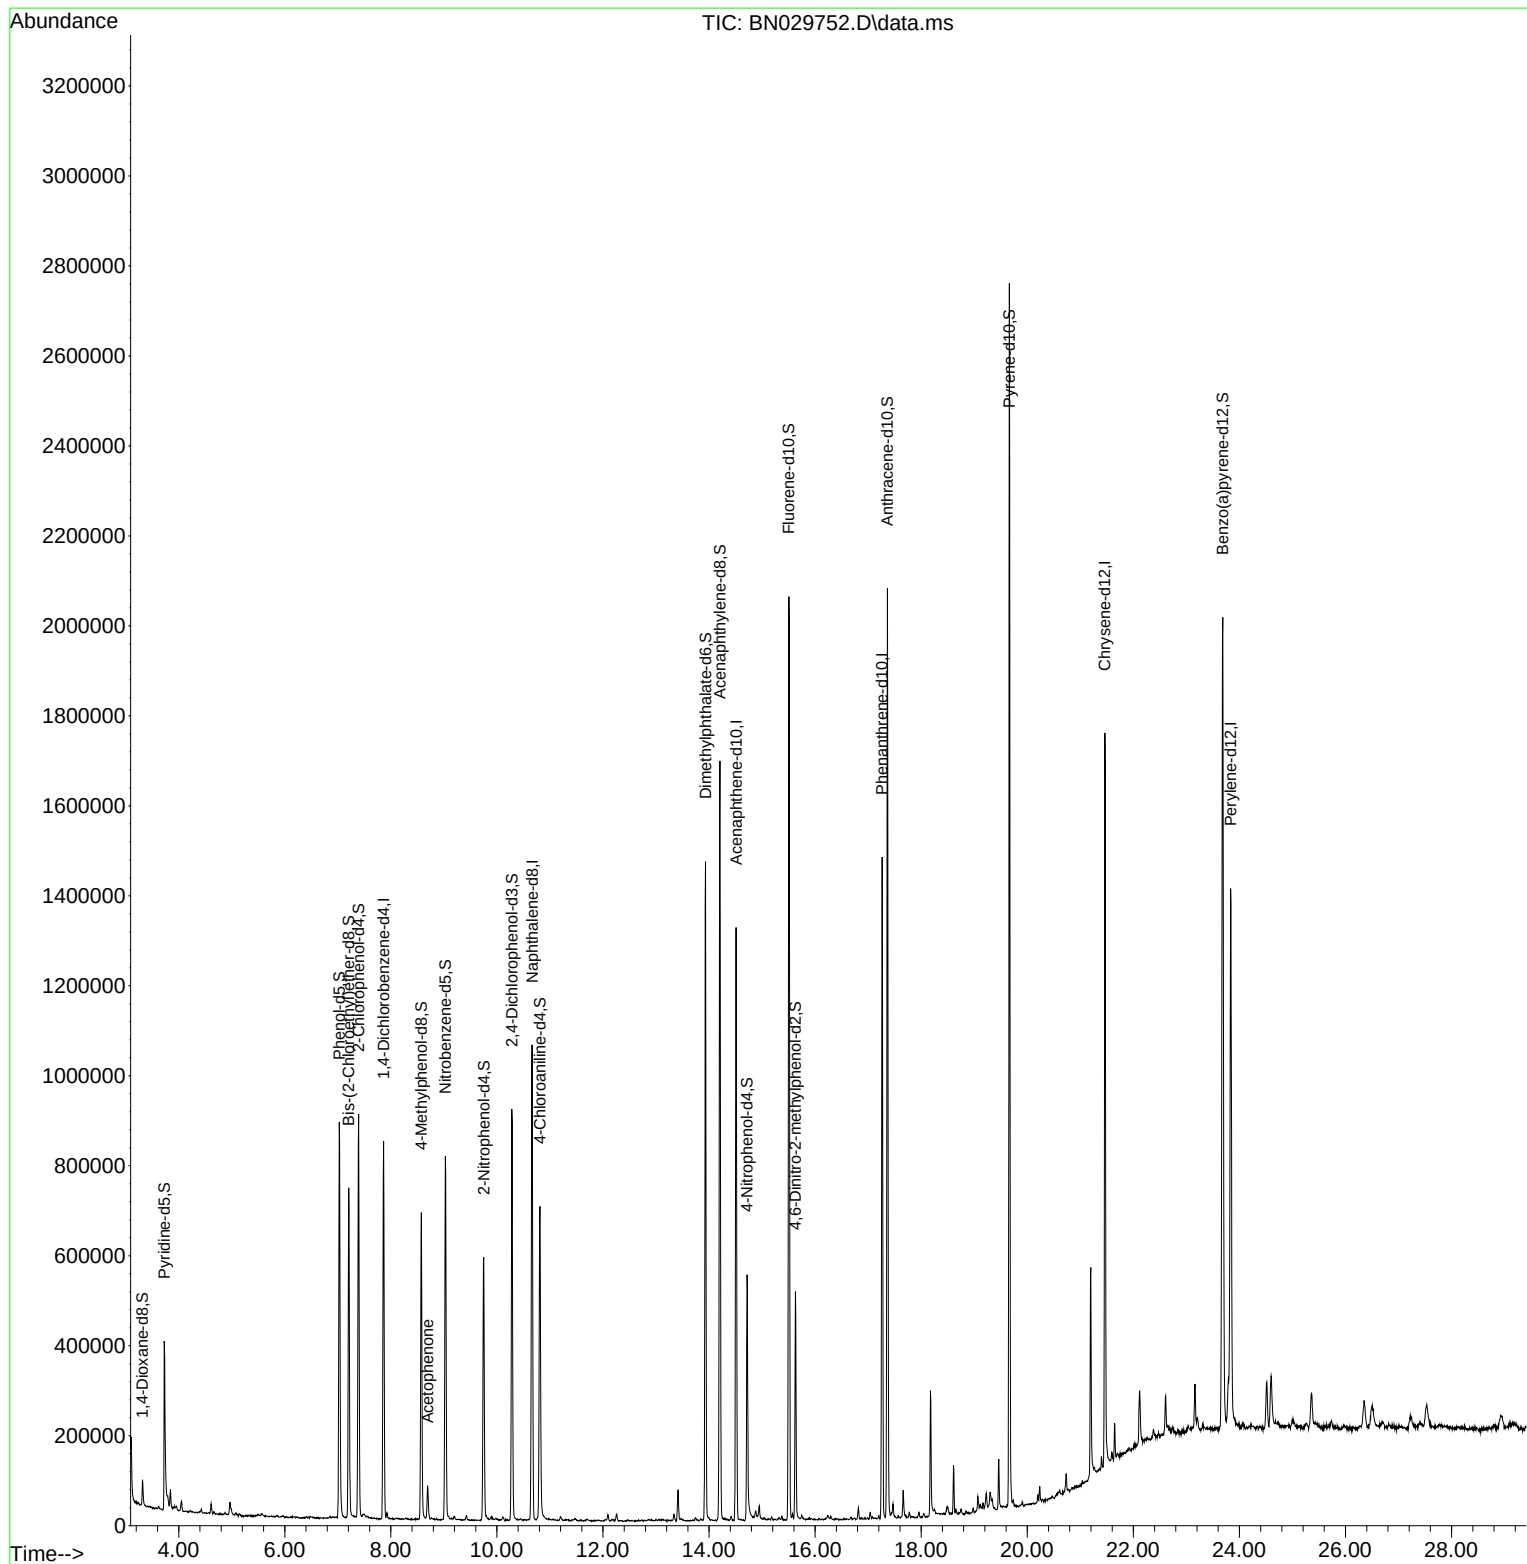

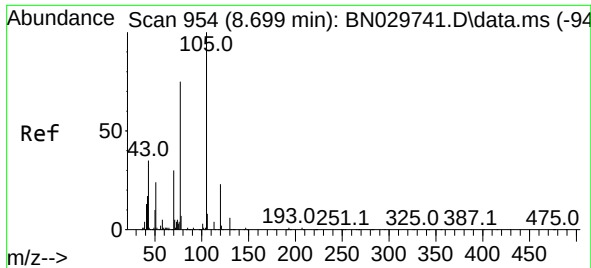

#16
 Acetophenone
 Concen: 1.683 ng/ul
 RT: 8.693 min Scan# 91
 Delta R.T. -0.006 min
 Lab File: BN029752.D
 Acq: 14 Feb 2024 03:28

Instrument :
 BNA_N
 ClientSampleId :
 BH6T4

Tgt Ion:105 Resp: 39189
 Ion Ratio Lower Upper
 105 100
 77 91.3 67.4 101.0
 51 29.5 20.7 31.1

