

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021424\
 Data File : BN029753.D
 Acq On : 14 Feb 2024 04:04
 Operator : MA/JU
 Sample : P1286-06
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH6T5

Quant Time: Feb 14 04:43:02 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 13 22:50:45 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.869	152	199071	20.000	ng/u1	0.00
20) Naphthalene-d8	10.663	136	821425	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.510	164	439175	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.263	188	872643	20.000	ng/u1	0.00
79) Chrysene-d12	21.463	240	749951	20.000	ng/u1	0.00
88) Perylene-d12	23.833	264	856082	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.322	96	24804	4.098	ng/uL	0.00
4) Pyridine-d5	3.734	84	200141	12.400	ng/u1	0.00
7) Phenol-d5	7.034	99	431309	23.163	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.211	67	299228	24.079	ng/u1	0.00
11) 2-Chlorophenol-d4	7.399	132	336946	24.972	ng/u1	0.00
15) 4-Methylphenol-d8	8.581	113	231177	16.647	ng/u1	0.00
21) Nitrobenzene-d5	9.034	128	164014	25.726	ng/u1	0.00
24) 2-Nitrophenol-d4	9.752	143	158228	28.497	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.287	165	280603	25.603	ng/u1	0.00
31) 4-Chloroaniline-d4	10.816	131	295016	15.779	ng/u1	0.00
46) Dimethylphthalate-d6	13.934	166	891846	27.276	ng/u1	0.00
49) Acenaphthylene-d8	14.204	160	1014293	26.121	ng/u1	0.00
54) 4-Nitrophenol-d4	14.722	143	95093	15.323	ng/u1	0.00
60) Fluorene-d10	15.510	176	780460	28.058	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.634	200	71472	16.809	ng/u1	0.00
73) Anthracene-d10	17.363	188	1039059	25.407	ng/u1	0.00
81) Pyrene-d10	19.663	212	1273042	28.287	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.680	264	1180533	27.559	ng/u1	0.00
Target Compounds						
					Qvalue	
16) Acetophenone	8.699	105	68252	3.088	ng/u1	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021424\
Data File : BN029753.D
Acq On : 14 Feb 2024 04:04
Operator : MA/JU
Sample : P1286-06
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH6T5

Quant Time: Feb 14 04:43:02 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 13 22:50:45 2024
Response via : Initial Calibration

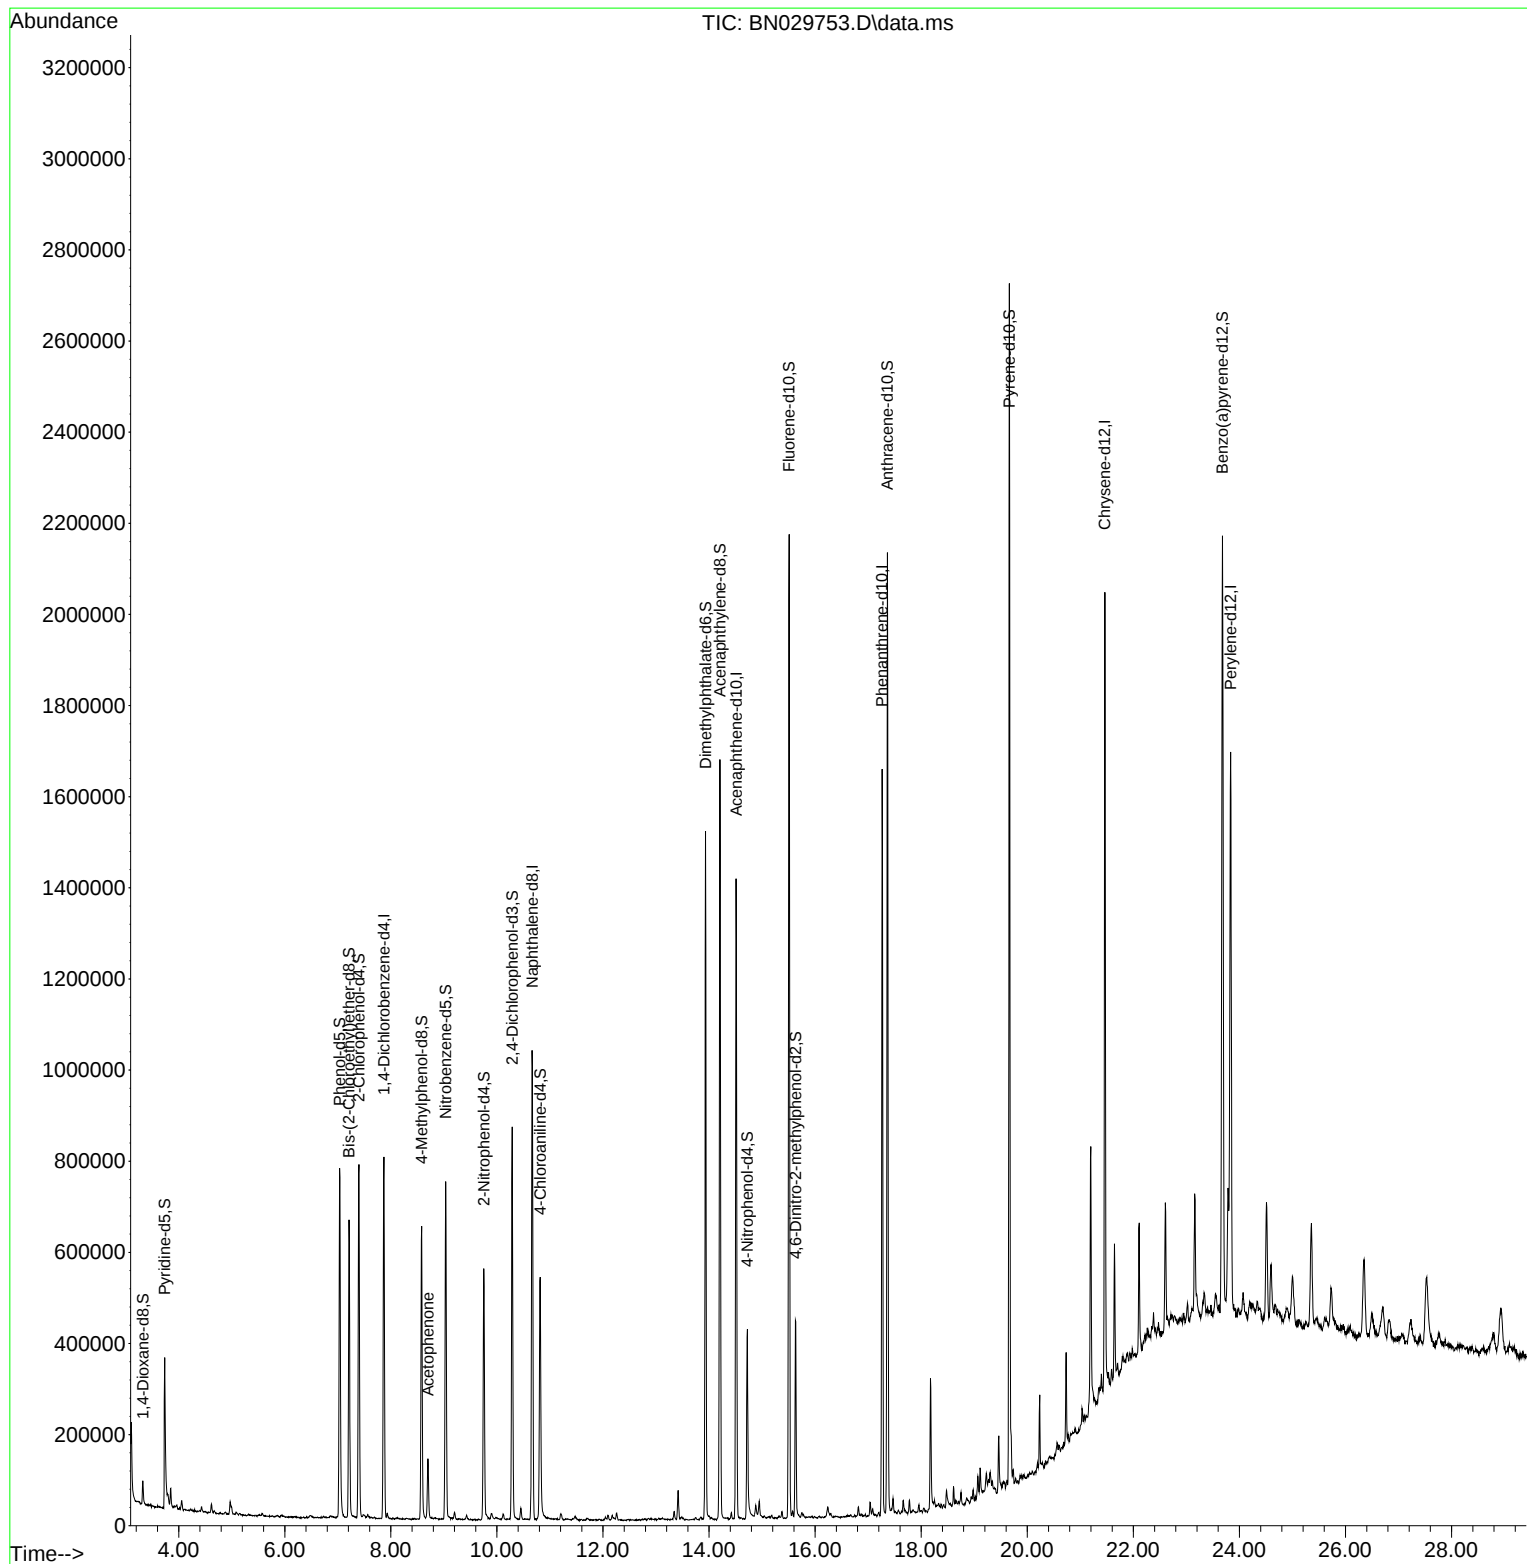

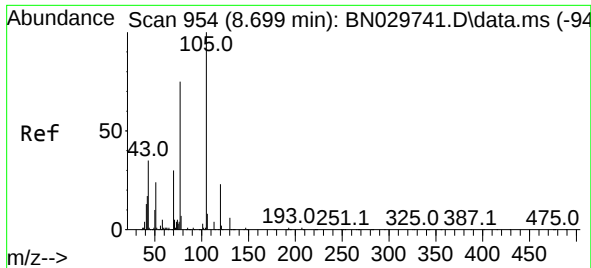

#16
 Acetophenone
 Concen: 3.088 ng/ul
 RT: 8.699 min Scan# 91
 Delta R.T. -0.000 min
 Lab File: BN029753.D
 Acq: 14 Feb 2024 04:04

Instrument :
 BNA_N
 ClientSampleId :
 BH6T5

Tgt Ion:105 Resp: 68252
 Ion Ratio Lower Upper
 105 100
 77 82.4 67.4 101.0
 51 28.4 20.7 31.1

