

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021424\
 Data File : BN029763.D
 Acq On : 14 Feb 2024 10:39
 Operator : MA/JU
 Sample : P1286-15
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH6S6

Quant Time: Feb 14 11:49:29 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 13 22:50:45 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.869	152	207788	20.000	ng/u1	0.00
20) Naphthalene-d8	10.669	136	816936	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.510	164	425854	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.263	188	816276	20.000	ng/u1	0.00
79) Chrysene-d12	21.463	240	705056	20.000	ng/u1	0.00
88) Perylene-d12	23.833	264	789946	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.323	96	26532	4.200	ng/uL	0.00
4) Pyridine-d5	3.734	84	212078	12.588	ng/u1	0.00
7) Phenol-d5	7.040	99	473517	24.363	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.211	67	320909	24.740	ng/u1	0.00
11) 2-Chlorophenol-d4	7.399	132	372070	26.418	ng/u1	0.00
15) 4-Methylphenol-d8	8.581	113	253893	17.516	ng/u1	0.00
21) Nitrobenzene-d5	9.034	128	179196	28.262	ng/u1	0.00
24) 2-Nitrophenol-d4	9.758	143	176101	31.890	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.287	165	300674	27.586	ng/u1	0.00
31) 4-Chloroaniline-d4	10.816	131	376120	20.227	ng/u1	0.00
46) Dimethylphthalate-d6	13.934	166	894825	28.223	ng/u1	0.00
49) Acenaphthylene-d8	14.204	160	1060206	28.158	ng/u1	0.00
54) 4-Nitrophenol-d4	14.722	143	123823	20.577	ng/u1	0.00
60) Fluorene-d10	15.510	176	771317	28.597	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.634	200	87838	22.084	ng/u1	0.00
73) Anthracene-d10	17.363	188	1062305	27.769	ng/u1	0.00
81) Pyrene-d10	19.663	212	1255795	29.680	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.680	264	1204144	30.463	ng/u1	0.00
Target Compounds						
					Qvalue	
16) Acetophenone	8.699	105	44854	1.944	ng/u1	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021424\
Data File : BN029763.D
Acq On : 14 Feb 2024 10:39
Operator : MA/JU
Sample : P1286-15
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH6S6

Quant Time: Feb 14 11:49:29 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 13 22:50:45 2024
Response via : Initial Calibration

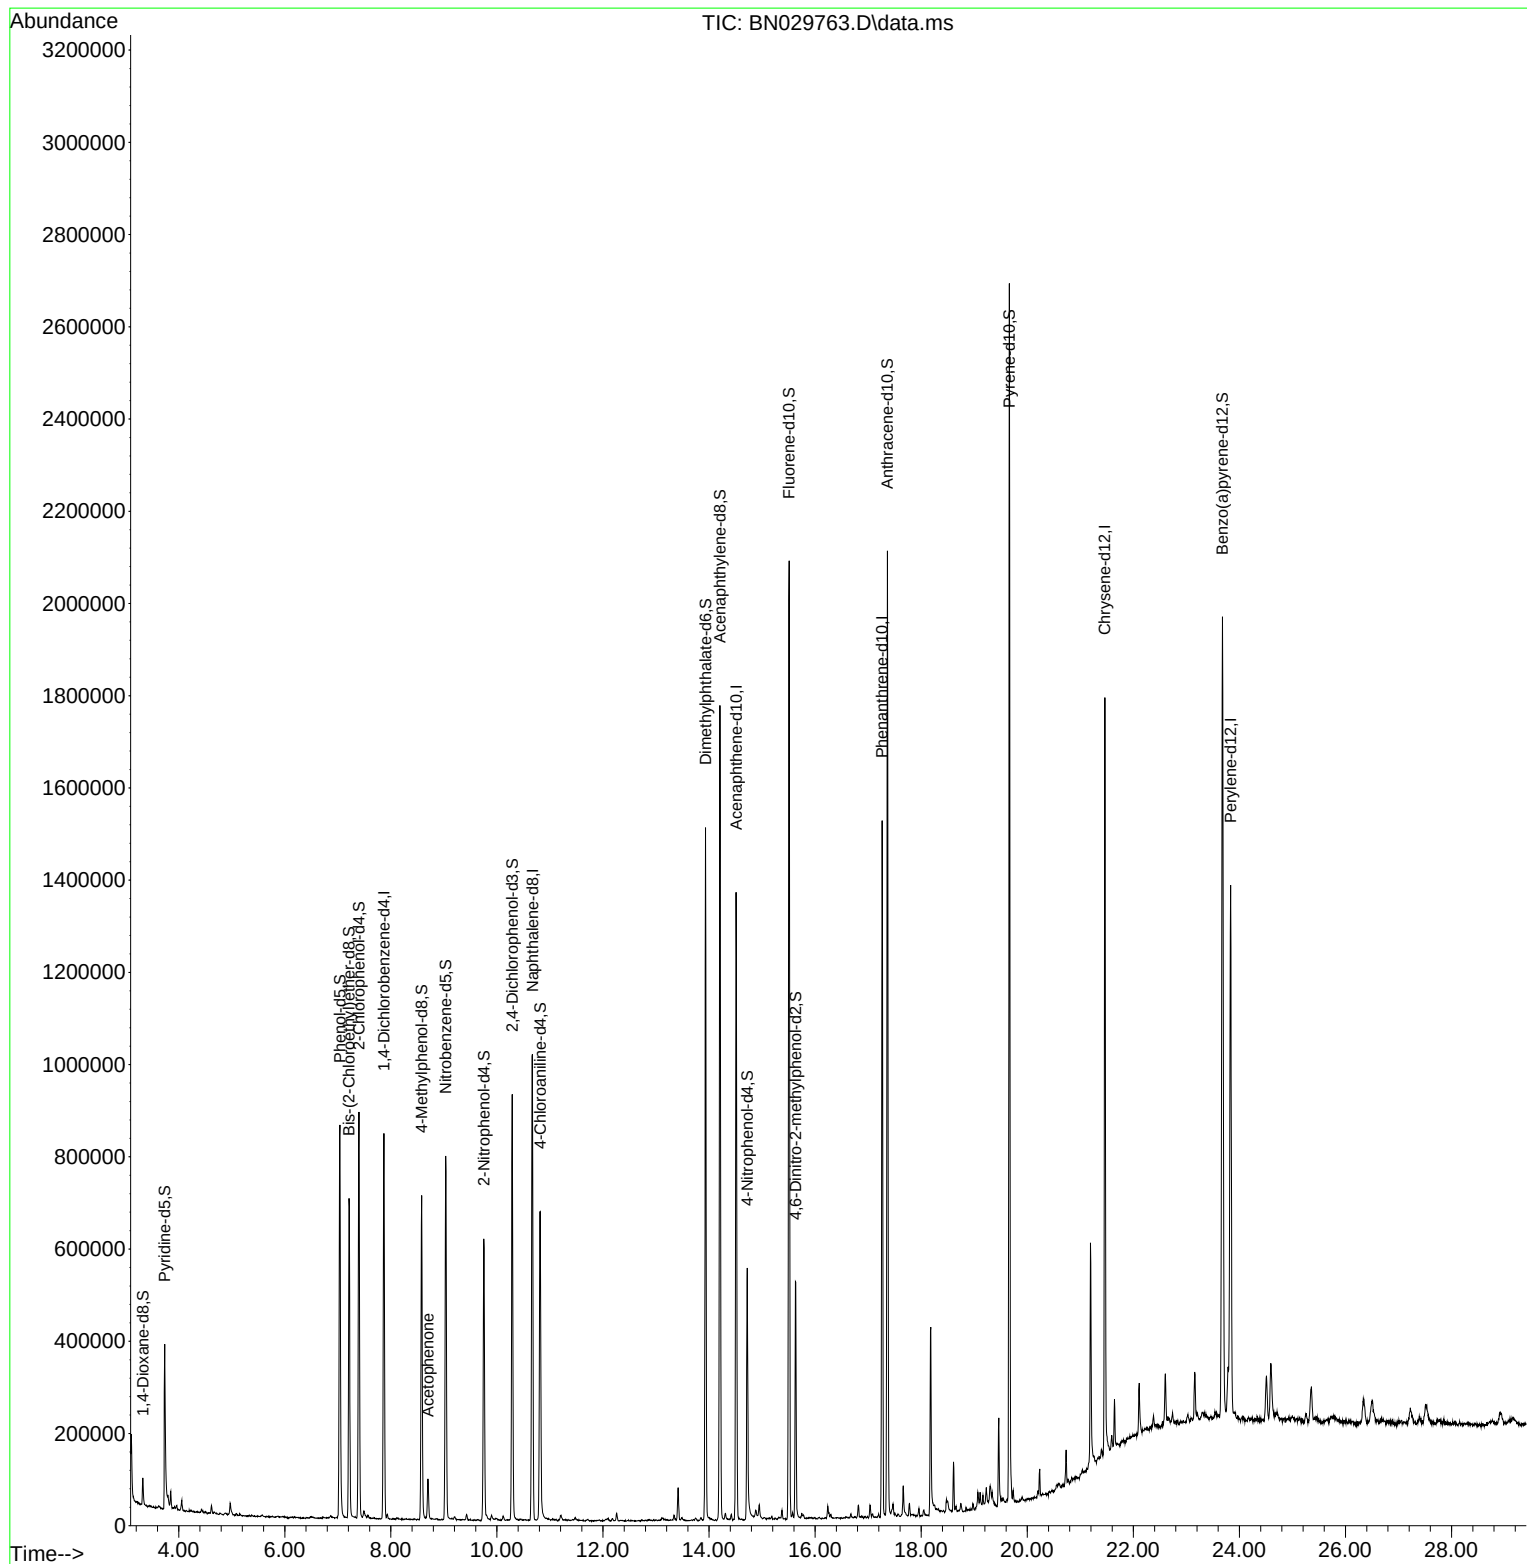

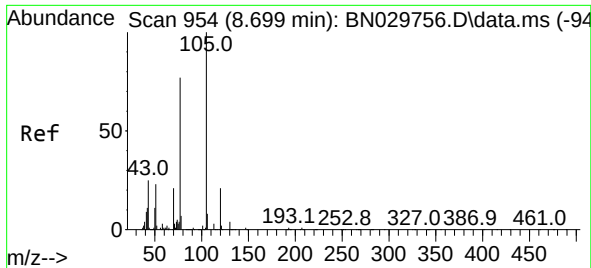

#16
Acetophenone
Concen: 1.944 ng/ul
RT: 8.699 min Scan# 91
Delta R.T. 0.000 min
Lab File: BN029763.D
Acq: 14 Feb 2024 10:39

Instrument :
BNA_N
ClientSampleId :
BH6S6

Tgt Ion:105 Resp: 44854
Ion Ratio Lower Upper
105 100
77 83.4 67.4 101.0
51 26.5 20.7 31.1

