

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021424\
 Data File : BN029765.D
 Acq On : 14 Feb 2024 11:51
 Operator : MA/JU
 Sample : P1289-20DL 10X
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AF1DL

Quant Time: Feb 14 22:49:54 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 13 22:50:45 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.869	152	177772	20.000	ng/u1	0.00
20) Naphthalene-d8	10.663	136	691013	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.510	164	358478	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.263	188	710822	20.000	ng/u1	0.00
79) Chrysene-d12	21.463	240	624293	20.000	ng/u1	0.00
88) Perylene-d12	23.833	264	722455	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.328	96	3157	0.584	ng/uL	0.00
4) Pyridine-d5	3.746	84	31412	2.179	ng/u1	0.02
7) Phenol-d5	7.040	99	46883	2.820	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.216	67	33747	3.041	ng/u1	0.00
11) 2-Chlorophenol-d4	7.399	132	38746	3.216	ng/u1	0.00
15) 4-Methylphenol-d8	8.581	113	36779	2.966	ng/u1	0.00
21) Nitrobenzene-d5	9.040	128	16956	3.162	ng/u1	0.00
24) 2-Nitrophenol-d4	9.757	143	14953	3.201	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.293	165	28047	3.042	ng/u1	0.00
31) 4-Chloroaniline-d4	10.816	131	43707	2.779	ng/u1	0.00
46) Dimethylphthalate-d6	13.934	166	96580	3.619	ng/u1	0.00
49) Acenaphthylene-d8	14.204	160	103589	3.268	ng/u1	0.00
54) 4-Nitrophenol-d4	0.000	143	0d	0.000	ng/u1	0.00
60) Fluorene-d10	15.504	176	82122	3.617	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	0.000	200	0d	0.000	ng/u1	0.00
73) Anthracene-d10	17.363	188	123727	3.714	ng/u1	0.00
81) Pyrene-d10	19.663	212	139171	3.715	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.680	264	132664	3.670	ng/u1	0.00
Target Compounds						
2) 1,4-Dioxane	3.358	88	76987	13.753	ng/uL	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021424\
Data File : BN029765.D
Acq On : 14 Feb 2024 11:51
Operator : MA/JU
Sample : P1289-20DL 10X
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AF1DL

Quant Time: Feb 14 22:49:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 13 22:50:45 2024
Response via : Initial Calibration

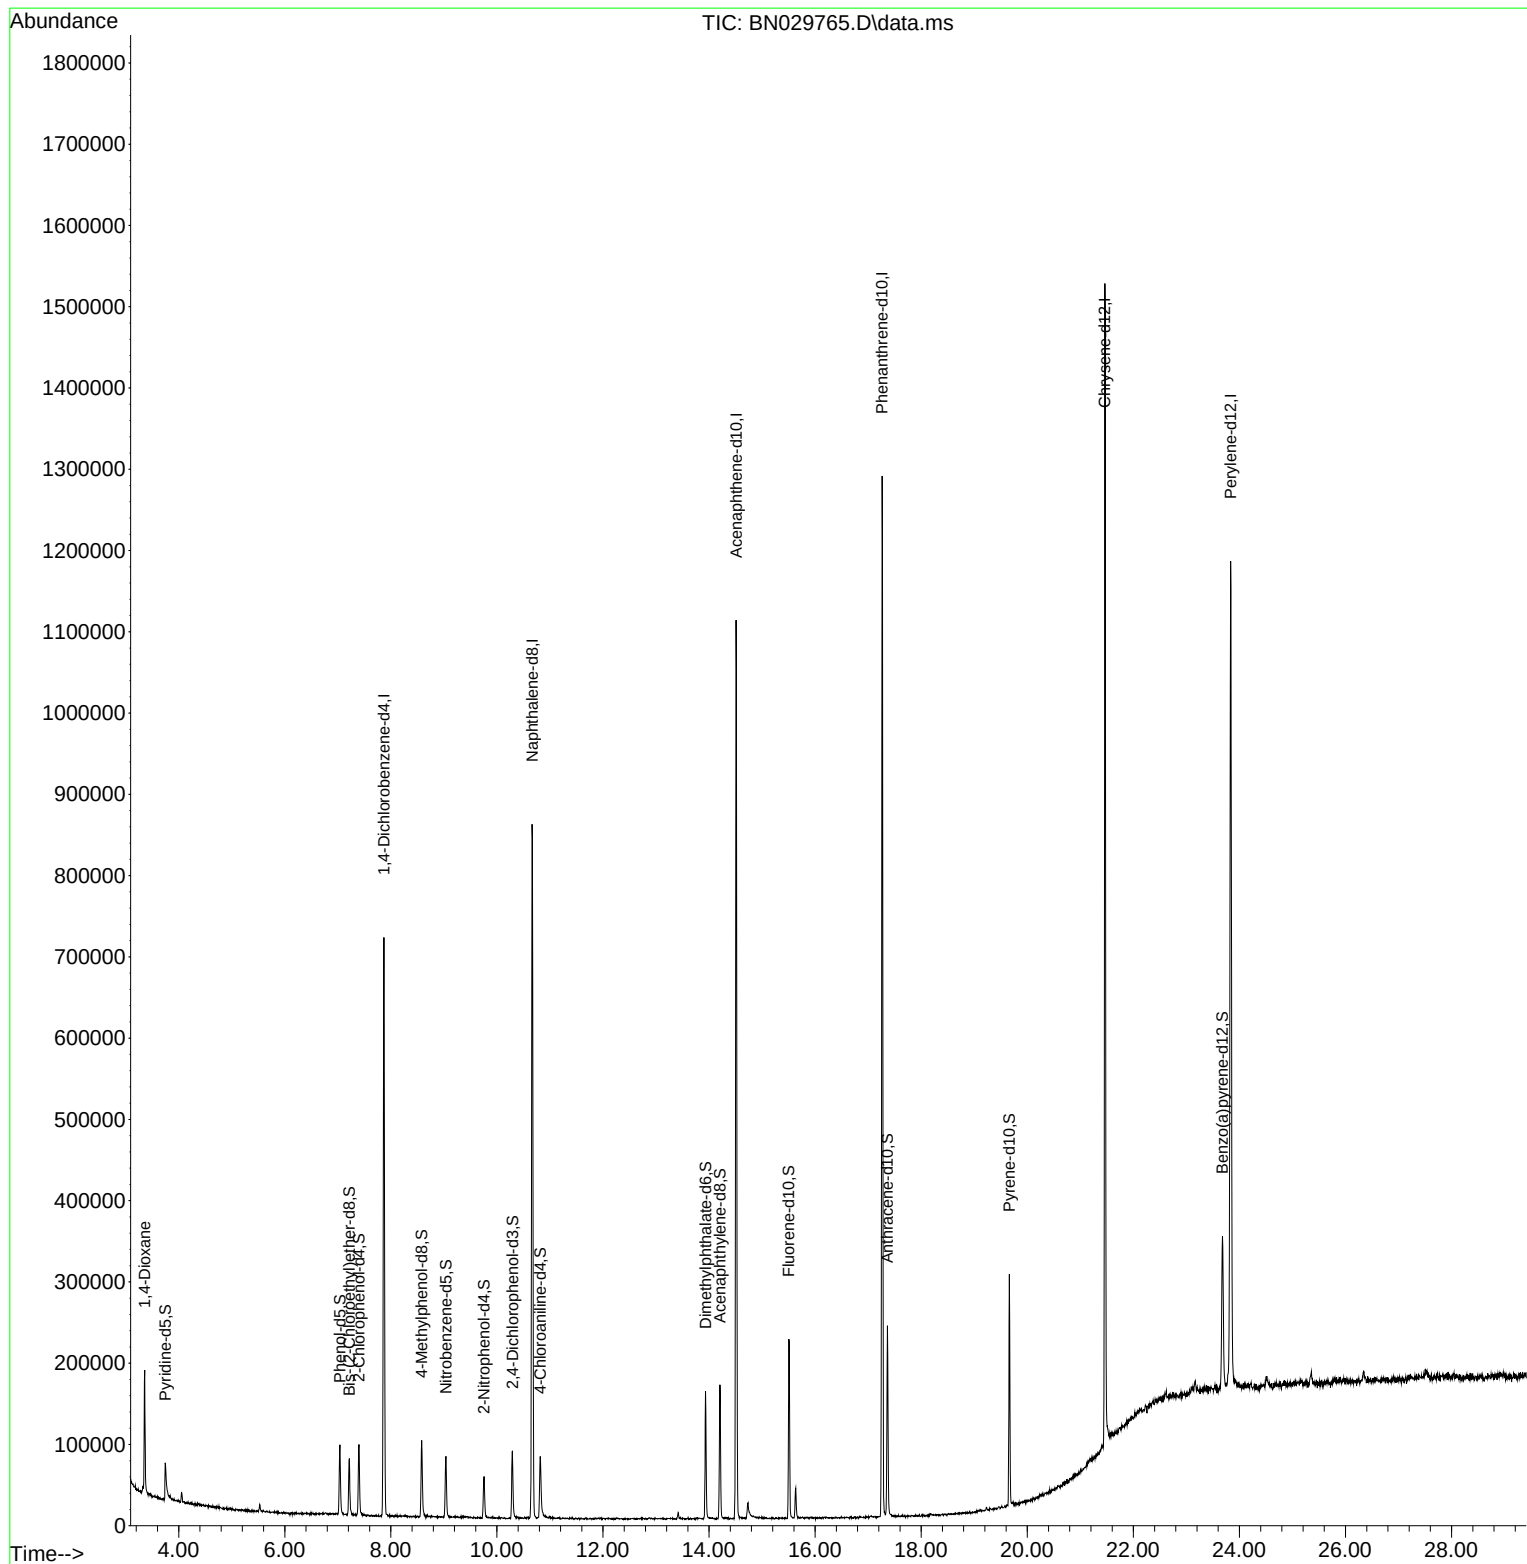

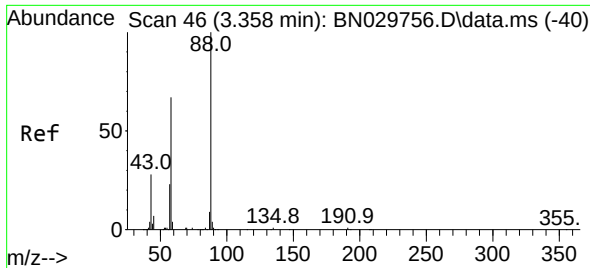

#2
 1,4-Dioxane
 Concen: 13.753 ng/uL
 RT: 3.358 min Scan# 40
 Delta R.T. -0.000 min
 Lab File: BN029765.D
 Acq: 14 Feb 2024 11:51

Instrument :
 BNA_N
 ClientSampleId :
 C0AF1DL

Tgt Ion: 88 Resp: 76987
 Ion Ratio Lower Upper
 88 100
 43 27.7 22.1 33.1
 58 66.3 56.5 84.7

