

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021424\
 Data File : BN029781.D
 Acq On : 14 Feb 2024 22:04
 Operator : MA/JU
 Sample : P1286-02
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH6S3

Quant Time: Feb 14 23:02:29 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 13 22:50:45 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.869	152	186530	20.000	ng/u1	0.00
20) Naphthalene-d8	10.663	136	760523	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.510	164	410062	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.263	188	822365	20.000	ng/u1	0.00
79) Chrysene-d12	21.463	240	723215	20.000	ng/u1	0.00
88) Perylene-d12	23.833	264	827017	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.323	96	18949	3.341	ng/uL	0.00
4) Pyridine-d5	3.734	84	148624	9.827	ng/u1	0.00
7) Phenol-d5	7.034	99	344192	19.728	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.211	67	235283	20.206	ng/u1	0.00
11) 2-Chlorophenol-d4	7.393	132	273343	21.620	ng/u1	0.00
15) 4-Methylphenol-d8	8.581	113	172098	13.226	ng/u1	0.00
21) Nitrobenzene-d5	9.034	128	130340	22.082	ng/u1	0.00
24) 2-Nitrophenol-d4	9.752	143	132748	25.823	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.287	165	221386	21.818	ng/u1	0.00
31) 4-Chloroaniline-d4	10.810	131	282305	16.308	ng/u1	0.00
46) Dimethylphthalate-d6	13.934	166	713849	23.382	ng/u1	0.00
49) Acenaphthylene-d8	14.204	160	820539	22.632	ng/u1	0.00
54) 4-Nitrophenol-d4	14.722	143	93897	16.205	ng/u1	0.00
60) Fluorene-d10	15.504	176	609136	23.454	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.634	200	64006	15.973	ng/u1	0.00
73) Anthracene-d10	17.363	188	899944	23.350	ng/u1	0.00
81) Pyrene-d10	19.663	212	1138748	26.238	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.680	264	1079492	26.085	ng/u1	0.00
Target Compounds						
					Qvalue	
16) Acetophenone	8.699	105	33711	1.628	ng/u1	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021424\
Data File : BN029781.D
Acq On : 14 Feb 2024 22:04
Operator : MA/JU
Sample : P1286-02
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH6S3

Quant Time: Feb 14 23:02:29 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 13 22:50:45 2024
Response via : Initial Calibration

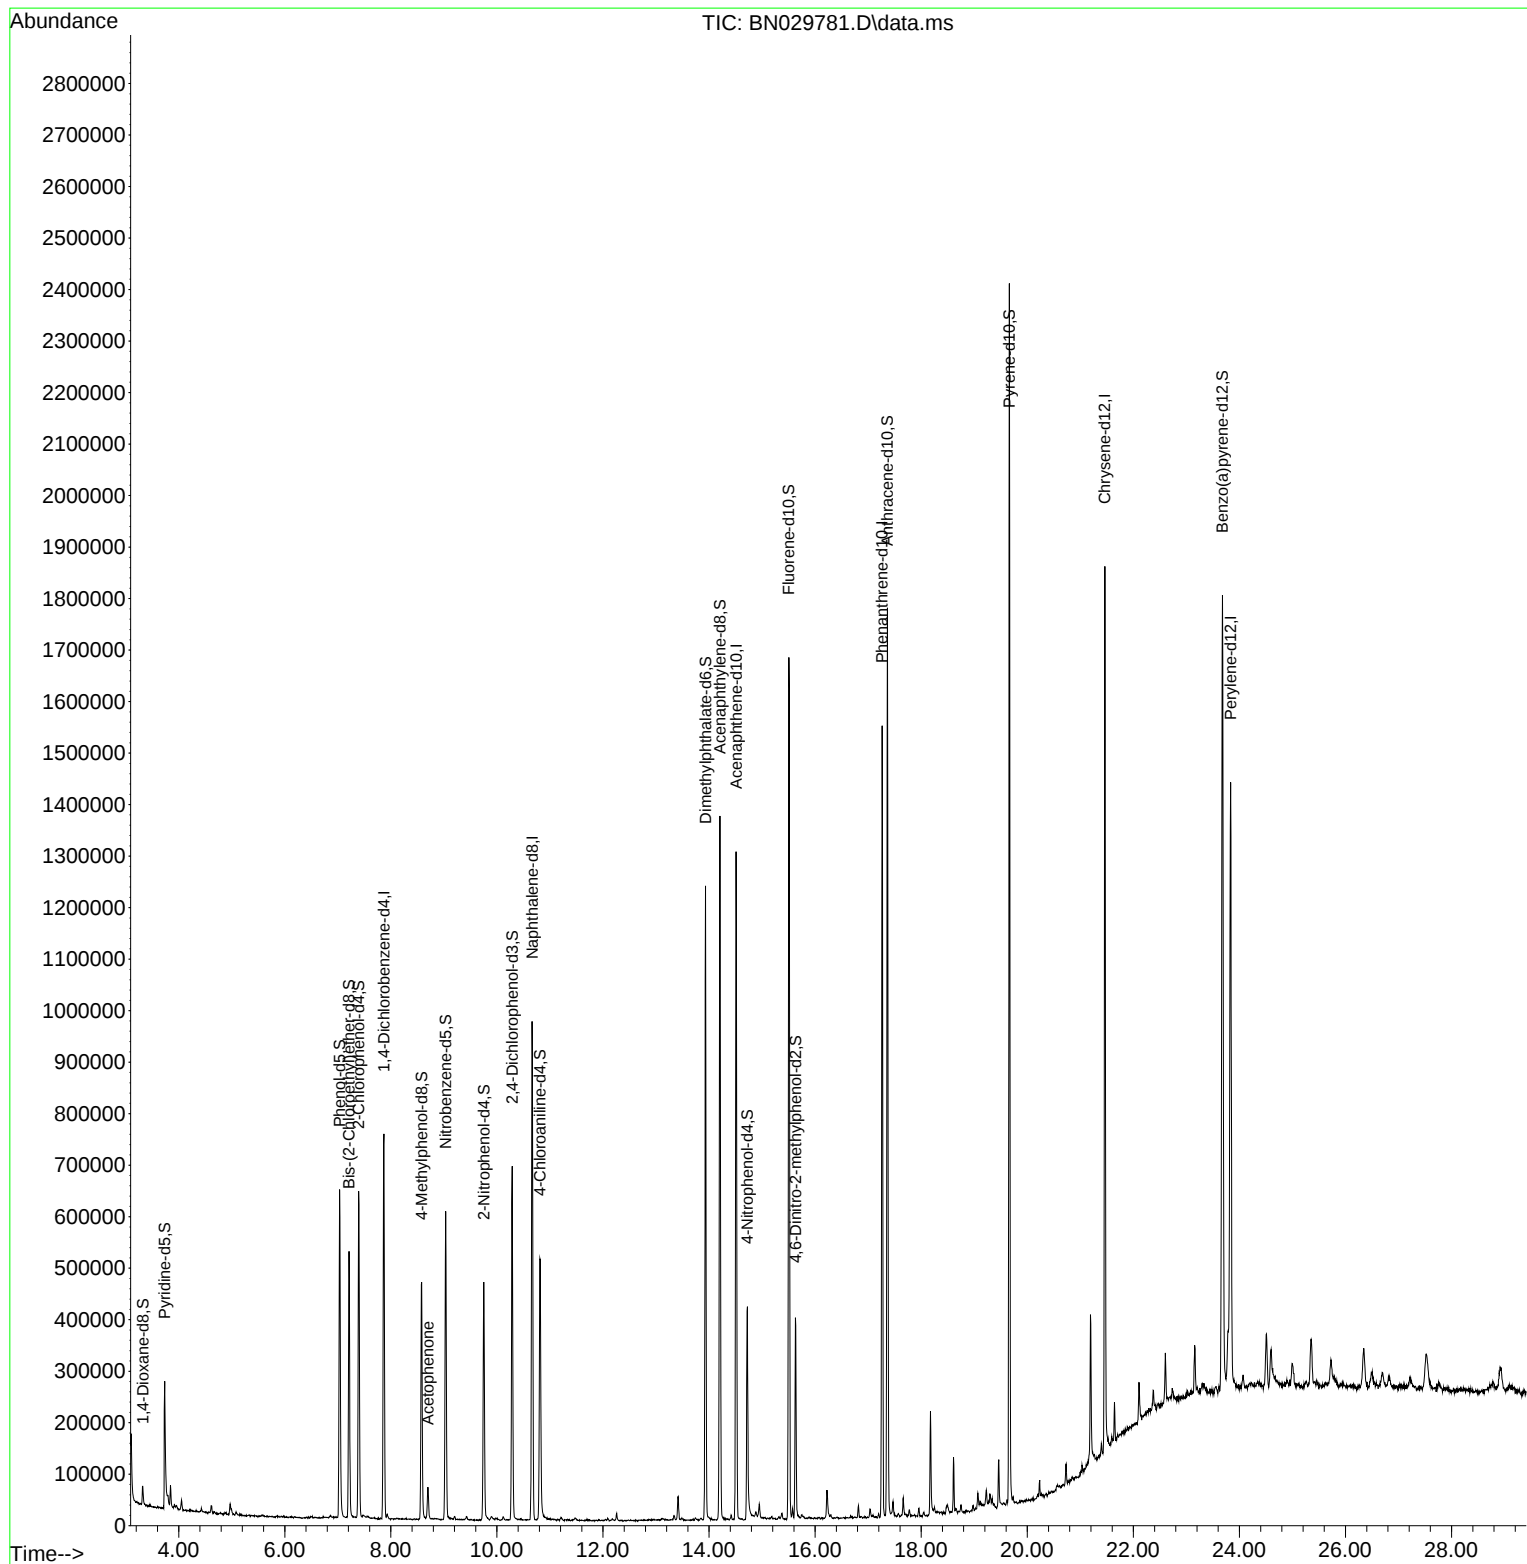

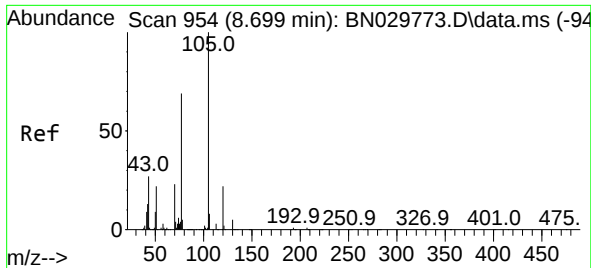

#16
 Acetophenone
 Concen: 1.628 ng/ul
 RT: 8.699 min Scan# 91
 Delta R.T. 0.000 min
 Lab File: BN029781.D
 Acq: 14 Feb 2024 22:04

Instrument :
 BNA_N
 ClientSampleId :
 BH6S3

Tgt Ion:105 Resp: 33711
 Ion Ratio Lower Upper
 105 100
 77 83.4 67.4 101.0
 51 28.6 20.7 31.1

