

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021424\
 Data File : BN029770.D
 Acq On : 14 Feb 2024 14:52
 Operator : MA/JU
 Sample : PB158805BL
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK805

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029770.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.322	37	40	46	rVB	50181	63134	2.26%	0.182%
2	3.734	107	110	134	rBV	518079	856099	30.65%	2.470%
3	4.058	162	165	171	rVB3	14856	19216	0.69%	0.055%
4	5.828	465	466	471	rBV5	2262	3001	0.11%	0.009%
5	7.040	665	672	689	rBV	679171	1081022	38.71%	3.119%
6	7.216	694	702	714	rBV	523186	847400	30.34%	2.445%
7	7.399	725	733	743	rBV	702685	1112906	39.85%	3.211%
8	7.869	806	813	820	rBV	671148	1051985	37.67%	3.035%
9	8.469	912	915	919	rBV5	2083	3152	0.11%	0.009%
10	8.581	927	934	946	rBV	786747	1278346	45.77%	3.689%
11	9.034	1004	1011	1023	rBV	597205	1011583	36.22%	2.919%
12	9.399	1069	1073	1076	rBV5	2195	3343	0.12%	0.010%
13	9.752	1127	1133	1144	rBV	467173	807541	28.92%	2.330%
14	10.287	1217	1224	1237	rBV	730120	1238826	44.36%	3.574%
15	10.669	1281	1289	1298	rBV	836817	1410932	50.52%	4.071%
16	10.816	1305	1314	1329	rBV	705182	1277911	45.76%	3.687%
17	12.263	1554	1560	1564	rBV3	11429	18902	0.68%	0.055%
18	13.416	1749	1756	1760	rBV2	12466	21006	0.75%	0.061%
19	13.487	1764	1768	1772	rBV5	2415	3983	0.14%	0.011%
20	13.934	1837	1844	1853	rBV	1151081	1589486	56.91%	4.586%
21	14.204	1883	1890	1900	rBV2	1318697	1948662	69.77%	5.623%
22	14.269	1900	1901	1905	rVB3	3854	3165	0.11%	0.009%
23	14.510	1936	1942	1952	rBV	1048077	1596525	57.17%	4.607%
24	14.722	1971	1978	1991	rBV	442626	752046	26.93%	2.170%
25	15.369	2086	2088	2093	rVB5	2323	2932	0.10%	0.008%
26	15.510	2105	2112	2119	rBV	1568475	2261193	80.97%	6.524%
27	15.634	2125	2133	2141	rBV	398378	573784	20.55%	1.656%
28	15.692	2141	2143	2145	rVV3	5428	4637	0.17%	0.013%
29	15.745	2149	2152	2156	rVB6	7409	9785	0.35%	0.028%
30	15.922	2180	2182	2185	rBV4	2385	2996	0.11%	0.009%
31	16.298	2242	2246	2249	rBV5	6423	9124	0.33%	0.026%
32	17.263	2404	2410	2418	rBV	1219779	1795420	64.29%	5.180%
33	17.363	2421	2427	2438	rBV	1678444	2435003	87.19%	7.026%
34	17.904	2516	2519	2520	rBV3	2732	2877	0.10%	0.008%
35	18.175	2559	2565	2568	rBV7	7339	12053	0.43%	0.035%
36	18.827	2674	2676	2679	rBV3	1988	2828	0.10%	0.008%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021424\
Data File : BN029770.D
Acq On : 14 Feb 2024 14:52
Operator : MA/JU
Sample : PB158805BL
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK805

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Title : SVOA CALIBRATION

37	19.227	2740	2744	2749	rBV3	21956	29611	1.06%	0.085%
38	19.298	2752	2756	2760	rBV	18672	24265	0.87%	0.070%
39	19.463	2782	2784	2788	rVB5	6902	6636	0.24%	0.019%
40	19.616	2809	2810	2812	rBV2	5741	3694	0.13%	0.011%
41	19.663	2812	2818	2825	rBV	1973685	2736453	97.98%	7.896%
42	21.469	3119	3125	3130	rBV	1419279	1892978	67.78%	5.462%
43	23.680	3494	3501	3511	rBV2	1355554	2792796	100.00%	8.058%
44	23.839	3521	3528	3541	rVB	1011936	2058185	73.70%	5.939%




Sum of corrected areas: 34657422

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021424\
Data File : BN029770.D
Acq On : 14 Feb 2024 14:52
Operator : MA/JU
Sample : PB158805BL
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK805

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

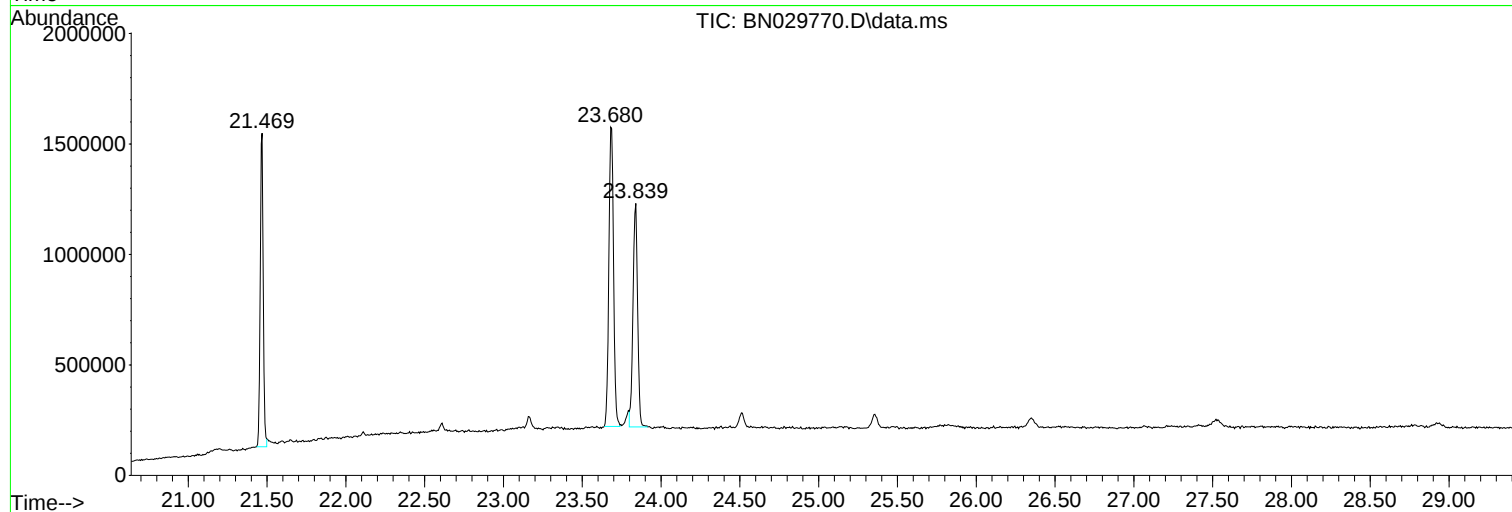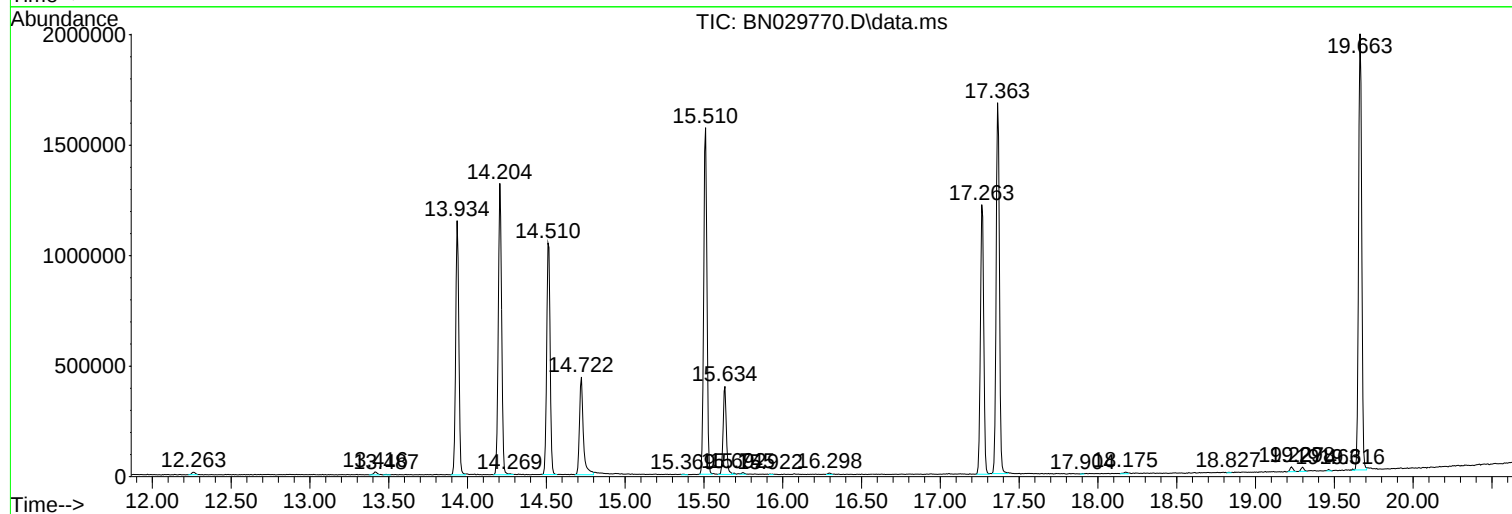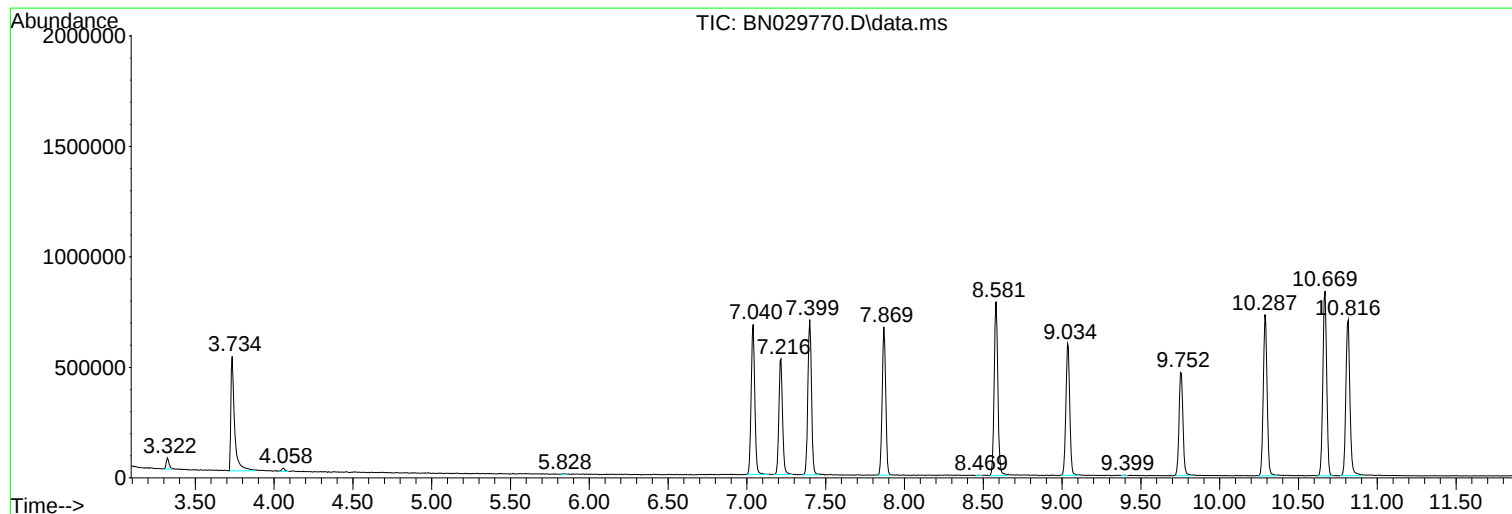

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021424\
Data File : BN029770.D
Acq On : 14 Feb 2024 14:52
Operator : MA/JU
Sample : PB158805BL
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK805

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021424\
Data File : BN029770.D
Acq On : 14 Feb 2024 14:52
Operator : MA/JU
Sample : PB158805BL
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK805

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------