

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021424\
 Data File : BN029777.D
 Acq On : 14 Feb 2024 19:40
 Operator : MA/JU
 Sample : P1289-18
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AG8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029777.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.323	36	40	46	rBV	28964	39058	0.92%	0.102%
2	3.740	108	111	132	rBV	87757	174109	4.11%	0.453%
3	4.052	161	164	171	rVB	17729	27418	0.65%	0.071%
4	4.381	218	220	225	rBV5	3322	4897	0.12%	0.013%
5	7.034	665	671	679	rBV	158917	260814	6.15%	0.678%
6	7.211	695	701	714	rBV	667475	1052965	24.85%	2.737%
7	7.393	726	732	746	rVB	625895	1010057	23.84%	2.626%
8	7.869	805	813	821	rBV	606248	975476	23.02%	2.536%
9	7.981	829	832	838	rVB6	6909	7872	0.19%	0.020%
10	8.581	927	934	946	rBV	442540	749268	17.68%	1.948%
11	9.034	1003	1011	1022	rBV	773970	1269679	29.96%	3.300%
12	9.140	1027	1029	1036	rVB5	6795	10799	0.25%	0.028%
13	9.428	1071	1078	1084	rBV4	7478	13459	0.32%	0.035%
14	9.622	1106	1111	1115	rVB7	4757	6827	0.16%	0.018%
15	9.752	1126	1133	1141	rBV	564891	947745	22.37%	2.464%
16	10.287	1216	1224	1236	rBV	829877	1382565	32.63%	3.594%
17	10.663	1281	1288	1299	rVB	801217	1347334	31.80%	3.502%
18	10.810	1301	1313	1324	rBV	660047	1176207	27.76%	3.057%
19	11.434	1414	1419	1422	rBV6	5291	9457	0.22%	0.025%
20	11.928	1500	1503	1508	rVB5	6304	9507	0.22%	0.025%
21	12.104	1525	1533	1536	rBV6	4249	7072	0.17%	0.018%
22	12.257	1554	1559	1565	rBV4	14938	26731	0.63%	0.069%
23	13.346	1739	1744	1747	rBV4	6362	10160	0.24%	0.026%
24	13.410	1751	1755	1760	rBV6	11470	19126	0.45%	0.050%
25	13.934	1837	1844	1855	rVV	1502173	2080264	49.09%	5.407%
26	14.204	1883	1890	1904	rBV2	1706205	2526482	59.62%	6.567%
27	14.510	1936	1942	1950	rBV	1054694	1567047	36.98%	4.073%
28	14.722	1972	1978	1986	rBV2	79862	145657	3.44%	0.379%
29	14.793	1989	1990	1996	rVB6	3317	5487	0.13%	0.014%
30	14.945	2010	2016	2020	rVB5	5525	10550	0.25%	0.027%
31	15.510	2105	2112	2125	rVB	2030432	3021236	71.30%	7.853%
32	15.634	2125	2133	2144	rBV	596987	866344	20.44%	2.252%
33	15.745	2148	2152	2157	rVB4	7812	12874	0.30%	0.033%
34	16.292	2241	2245	2250	rBV8	6550	9406	0.22%	0.024%
35	16.939	2352	2355	2359	rBV6	3374	5617	0.13%	0.015%
36	17.263	2404	2410	2420	rBV	1301007	1783491	42.09%	4.636%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021424\
 Data File : BN029777.D
 Acq On : 14 Feb 2024 19:40
 Operator : MA/JU
 Sample : P1289-18
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AG8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

37	17.363	2420	2427	2440	rBV2	2421914	3367621	79.47%	8.754%
38	17.663	2475	2478	2481	rBV4	7394	8253	0.19%	0.021%
39	18.175	2559	2565	2575	rBV	57046	90431	2.13%	0.235%
40	18.469	2609	2615	2618	rBV7	3647	5628	0.13%	0.015%
41	18.610	2637	2639	2644	rVB6	9790	11374	0.27%	0.030%
42	19.228	2738	2744	2748	rBV3	29857	41580	0.98%	0.108%
43	19.298	2752	2756	2760	rVV	22838	30534	0.72%	0.079%
44	19.339	2760	2763	2766	rVV4	4813	6072	0.14%	0.016%
45	19.392	2767	2772	2778	rVB4	11902	21760	0.51%	0.057%
46	19.457	2778	2783	2788	rBV4	26260	39982	0.94%	0.104%
47	19.616	2808	2810	2812	rBV3	9450	7361	0.17%	0.019%
48	19.663	2812	2818	2826	rBV	2932485	3848102	90.81%	10.003%
49	20.510	2958	2962	2966	rBV2	19835	25408	0.60%	0.066%
50	20.669	2986	2989	2992	rBV5	10926	13014	0.31%	0.034%
51	21.192	3074	3078	3087	rBV2	73600	101931	2.41%	0.265%
52	21.339	3100	3103	3107	rBV5	18783	26611	0.63%	0.069%
53	21.463	3118	3124	3137	rBV	1474833	1964608	46.36%	5.107%
54	23.680	3493	3501	3513	rBV	2182167	4237504	100.00%	11.015%
55	23.833	3520	3527	3537	rVB	1023657	2049930	48.38%	5.329%




Sum of corrected areas: 38470761

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021424\
Data File : BN029777.D
Acq On : 14 Feb 2024 19:40
Operator : MA/JU
Sample : P1289-18
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AG8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

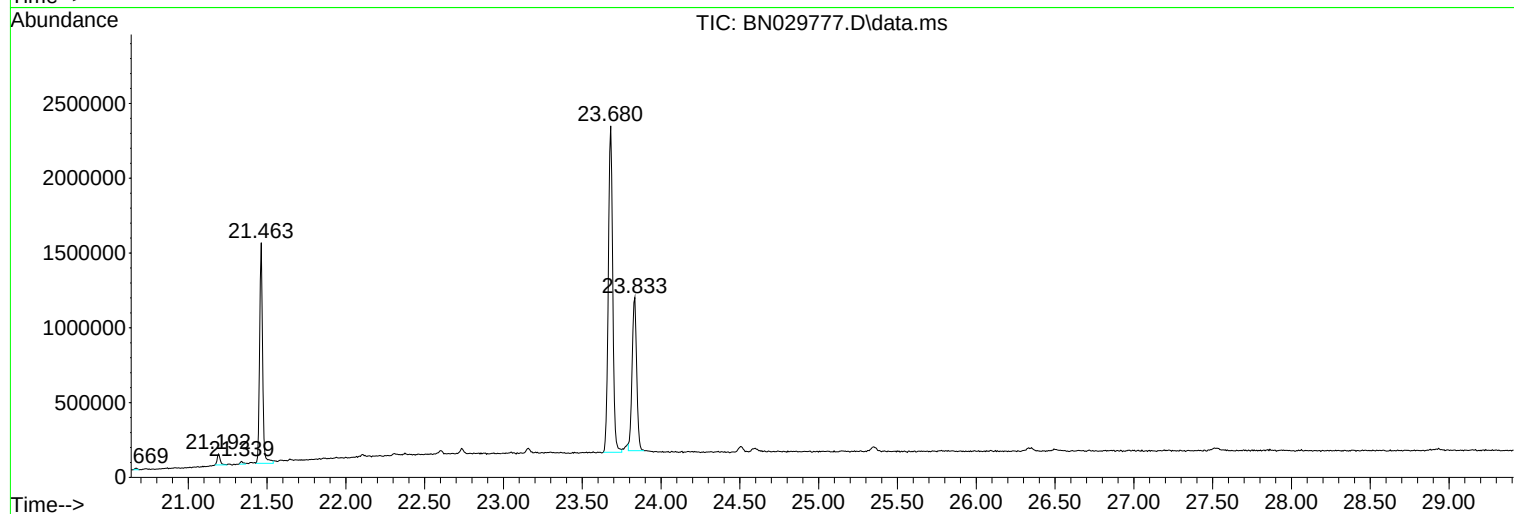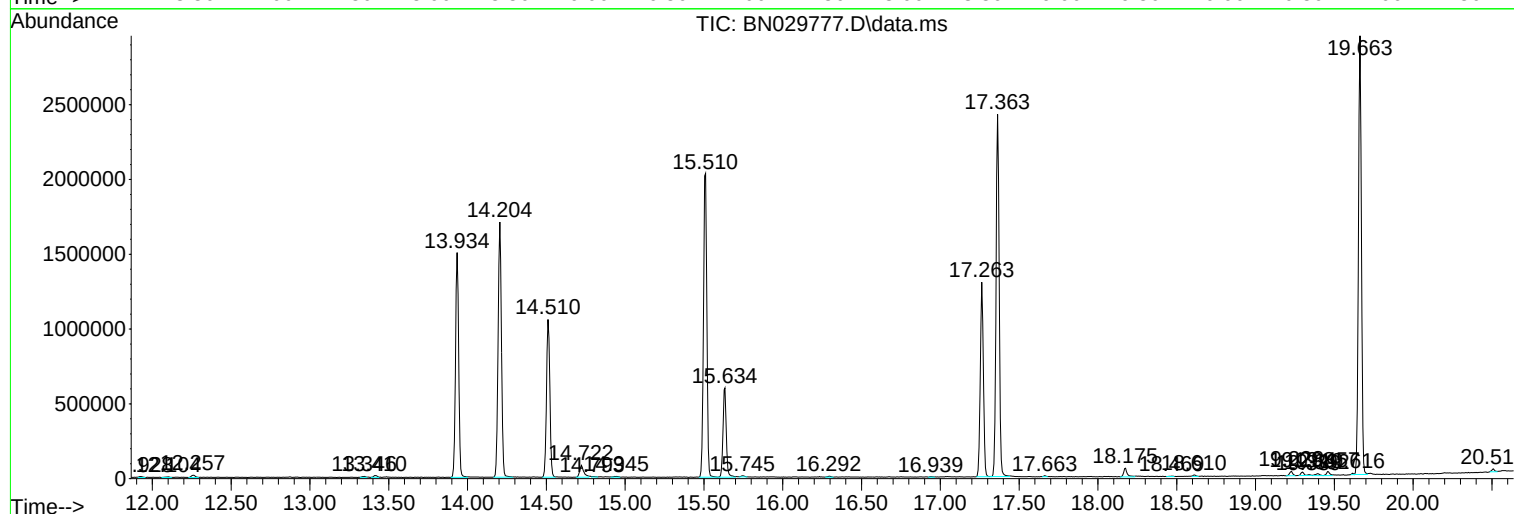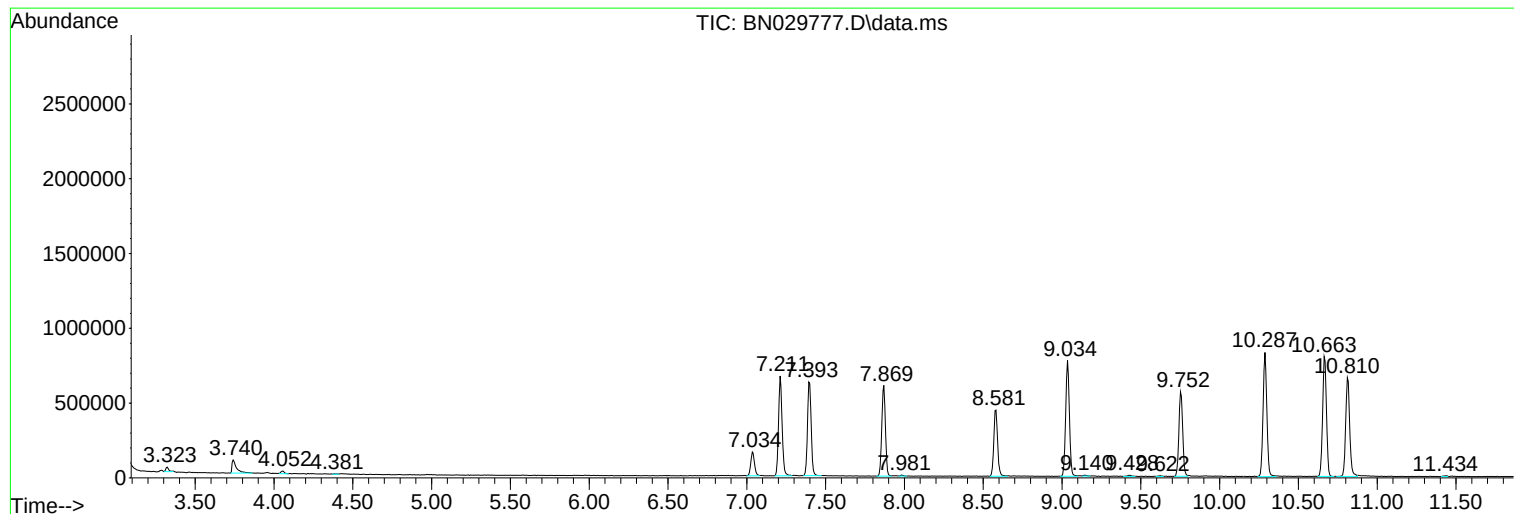

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021424\
Data File : BN029777.D
Acq On : 14 Feb 2024 19:40
Operator : MA/JU
Sample : P1289-18
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AG8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021424\
Data File : BN029777.D
Acq On : 14 Feb 2024 19:40
Operator : MA/JU
Sample : P1289-18
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AG8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc