

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021424\
 Data File : BN029778.D
 Acq On : 14 Feb 2024 20:16
 Operator : MA/JU
 Sample : P1299-02
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH6Z6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029778.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.322	36	40	53	rVB	56234	83759	1.67%	0.178%
2	3.734	107	110	127	rBV	282932	473120	9.41%	1.008%
3	4.052	161	164	172	rVB2	14511	23037	0.46%	0.049%
4	4.969	316	320	323	rBV4	7070	11074	0.22%	0.024%
5	5.575	418	423	428	rBV9	4583	9166	0.18%	0.020%
6	6.869	639	643	647	rBV5	4914	5994	0.12%	0.013%
7	7.034	665	671	682	rVB	372102	593968	11.82%	1.266%
8	7.210	695	701	714	rBV	856763	1337674	26.61%	2.850%
9	7.399	726	733	743	rBV	911607	1474835	29.34%	3.143%
10	7.869	806	813	820	rBV	612721	981560	19.53%	2.091%
11	8.281	877	883	885	rBV5	3490	5242	0.10%	0.011%
12	8.581	926	934	944	rBV	817366	1332914	26.52%	2.840%
13	9.034	1003	1011	1024	rBV	987467	1635559	32.54%	3.485%
14	9.146	1026	1030	1033	rVB6	6400	8597	0.17%	0.018%
15	9.234	1042	1045	1051	rVB7	3134	6334	0.13%	0.013%
16	9.422	1075	1077	1085	rVB6	4104	6952	0.14%	0.015%
17	9.751	1126	1133	1147	rBV	751966	1253774	24.94%	2.671%
18	10.287	1217	1224	1240	rBV	1110963	1852491	36.86%	3.947%
19	10.663	1281	1288	1296	rVB	803269	1346758	26.79%	2.870%
20	10.810	1305	1313	1329	rBV	896560	1598366	31.80%	3.406%
21	12.257	1554	1559	1566	rBV2	19043	32121	0.64%	0.068%
22	13.140	1704	1709	1715	rVB3	6026	11908	0.24%	0.025%
23	13.340	1739	1743	1750	rBV7	3782	7355	0.15%	0.016%
24	13.416	1752	1756	1763	rVB2	19532	30909	0.61%	0.066%
25	13.934	1837	1844	1857	rBV	1923410	2655718	52.84%	5.659%
26	14.204	1883	1890	1904	rBV	2146427	3145969	62.59%	6.703%
27	14.510	1935	1942	1951	rBV	1086487	1578076	31.40%	3.363%
28	14.722	1971	1978	1992	rBV	228782	415961	8.28%	0.886%
29	14.881	2003	2005	2010	rVB6	7358	10962	0.22%	0.023%
30	14.939	2010	2015	2022	rVB9	8855	21201	0.42%	0.045%
31	15.316	2076	2079	2083	rBV3	4575	6191	0.12%	0.013%
32	15.510	2103	2112	2124	rBV	2608831	3780786	75.22%	8.056%
33	15.634	2126	2133	2146	rVV	802112	1147995	22.84%	2.446%
34	15.745	2148	2152	2159	rVB3	12605	22560	0.45%	0.048%
35	16.292	2240	2245	2251	rVB7	11496	19164	0.38%	0.041%
36	16.675	2305	2310	2314	rBV8	3601	6373	0.13%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021424\
 Data File : BN029778.D
 Acq On : 14 Feb 2024 20:16
 Operator : MA/JU
 Sample : P1299-02
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH6Z6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

37	16.939	2351	2355	2359	rBV7	4142	6327	0.13%	0.013%
38	17.263	2404	2410	2418	rVB	1236644	1783165	35.48%	3.800%
39	17.363	2420	2427	2439	rBV2	2756184	4035953	80.29%	8.600%
40	17.939	2523	2525	2530	rVB5	4287	6043	0.12%	0.013%
41	18.175	2560	2565	2571	rBV	64983	92812	1.85%	0.198%
42	18.257	2577	2579	2582	rVB4	6538	6321	0.13%	0.013%
43	18.610	2637	2639	2643	rVB5	6283	6546	0.13%	0.014%
44	18.651	2643	2646	2652	rBV8	7005	12743	0.25%	0.027%
45	19.227	2739	2744	2751	rBV2	37163	56864	1.13%	0.121%
46	19.298	2751	2756	2760	rBV	34690	50989	1.01%	0.109%
47	19.457	2779	2783	2789	rBV3	40715	59696	1.19%	0.127%
48	19.610	2804	2809	2812	rBV2	44953	63901	1.27%	0.136%
49	19.663	2812	2818	2828	rVB	3518229	4694921	93.40%	10.004%
50	21.192	3075	3078	3083	rBV4	42943	55374	1.10%	0.118%
51	21.463	3119	3124	3131	rBV	1460358	1907674	37.95%	4.065%
52	23.680	3493	3501	3514	rBV2	2572960	5026416	100.00%	10.710%
53	23.833	3520	3527	3538	rVB	1030098	2131347	42.40%	4.541%




Sum of corrected areas: 46931515

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021424\
Data File : BN029778.D
Acq On : 14 Feb 2024 20:16
Operator : MA/JU
Sample : P1299-02
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH6Z6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

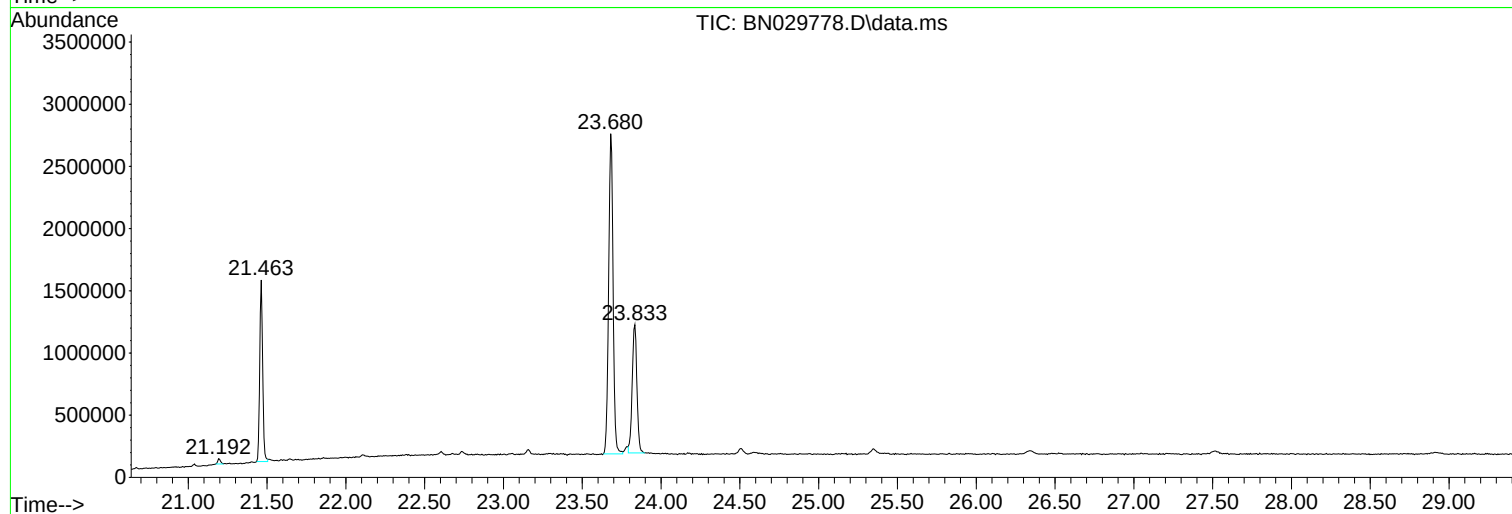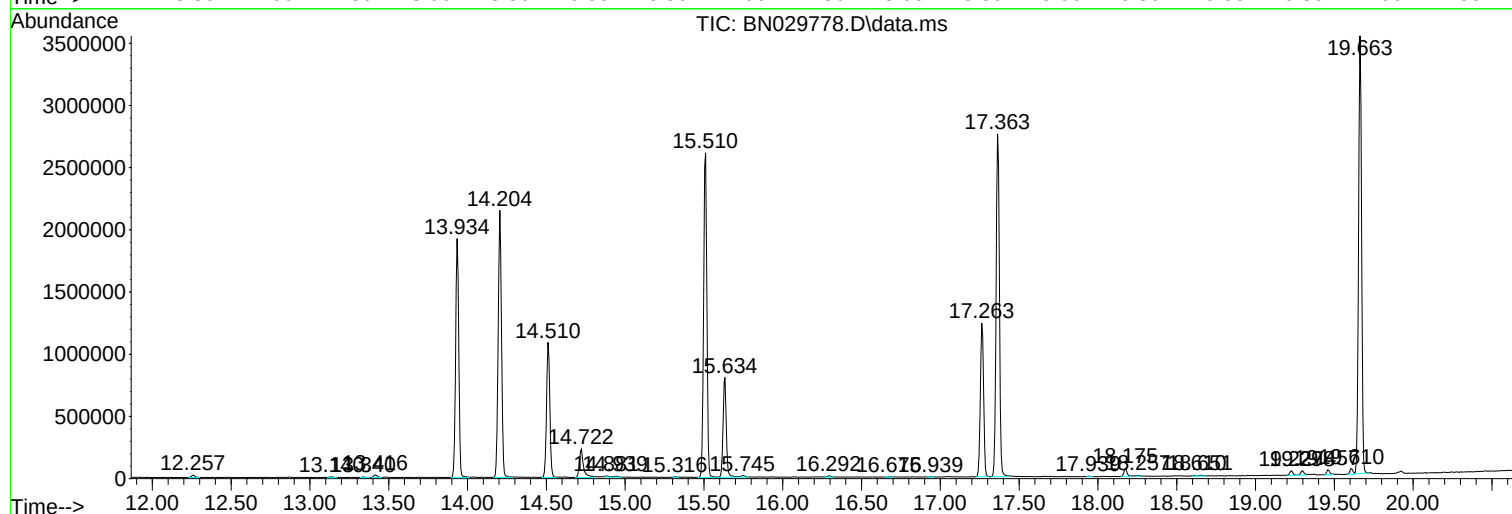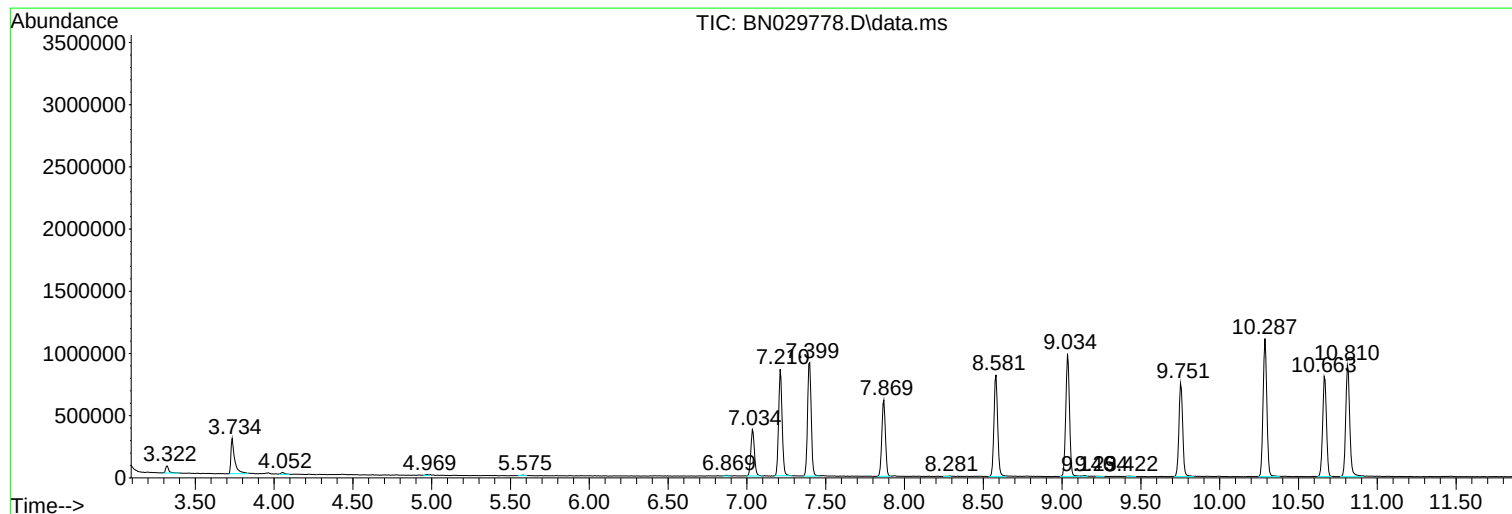

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021424\
Data File : BN029778.D
Acq On : 14 Feb 2024 20:16
Operator : MA/JU
Sample : P1299-02
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH6Z6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021424\
Data File : BN029778.D
Acq On : 14 Feb 2024 20:16
Operator : MA/JU
Sample : P1299-02
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH6Z6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc