

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021424\
 Data File : BN029779.D
 Acq On : 14 Feb 2024 20:52
 Operator : MA/JU
 Sample : P1299-03
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH6Z7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029779.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.317	36	39	47	rVB	51285	72404	1.61%	0.159%
2	3.734	107	110	125	rBV	292491	490095	10.92%	1.077%
3	4.052	161	164	170	rVB3	16765	25451	0.57%	0.056%
4	4.969	316	320	323	rBV3	6150	8692	0.19%	0.019%
5	5.575	420	423	427	rBV6	4236	5710	0.13%	0.013%
6	7.034	665	671	682	rVB	329115	527352	11.75%	1.158%
7	7.211	694	701	712	rBV	825370	1299182	28.96%	2.854%
8	7.399	726	733	742	rBV	864567	1393998	31.07%	3.062%
9	7.869	806	813	821	rBV	657175	1052266	23.45%	2.312%
10	7.934	821	824	829	rVB6	4506	5663	0.13%	0.012%
11	8.581	925	934	946	rBV	766989	1256866	28.01%	2.761%
12	9.034	1003	1011	1024	rBV	954168	1578038	35.17%	3.467%
13	9.140	1024	1029	1035	rVB8	7480	13497	0.30%	0.030%
14	9.428	1074	1078	1081	rBV5	3816	4863	0.11%	0.011%
15	9.622	1107	1111	1117	rVB8	2769	5133	0.11%	0.011%
16	9.752	1125	1133	1146	rBV	726783	1213980	27.06%	2.667%
17	10.287	1215	1224	1239	rBV	1078187	1807405	40.28%	3.970%
18	10.663	1281	1288	1298	rVB	868515	1465069	32.65%	3.218%
19	10.810	1304	1313	1333	rBV	811803	1466986	32.70%	3.223%
20	11.428	1415	1418	1420	rBV4	4050	4499	0.10%	0.010%
21	12.257	1555	1559	1564	rBV	17976	29470	0.66%	0.065%
22	13.134	1705	1708	1713	rVB3	7687	10508	0.23%	0.023%
23	13.340	1737	1743	1748	rBV8	5991	9911	0.22%	0.022%
24	13.416	1750	1756	1762	rVV2	16440	27111	0.60%	0.060%
25	13.934	1837	1844	1859	rBV	1872915	2532391	56.44%	5.563%
26	14.204	1883	1890	1904	rBV	2175539	3116640	69.46%	6.847%
27	14.510	1935	1942	1950	rBV	1154698	1678678	37.41%	3.688%
28	14.722	1972	1978	1991	rBV	178663	333762	7.44%	0.733%
29	14.887	1999	2006	2009	rBV9	7692	14045	0.31%	0.031%
30	14.940	2012	2015	2018	rVB4	5947	8344	0.19%	0.018%
31	15.322	2076	2080	2082	rVB4	4287	4943	0.11%	0.011%
32	15.510	2104	2112	2123	rBV	2494320	3688620	82.21%	8.103%
33	15.634	2126	2133	2143	rBV	707552	1040588	23.19%	2.286%
34	15.745	2148	2152	2157	rVB2	12098	17846	0.40%	0.039%
35	16.292	2241	2245	2250	rBV6	10914	16249	0.36%	0.036%
36	16.939	2353	2355	2360	rBV5	3818	5257	0.12%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021424\
Data File : BN029779.D
Acq On : 14 Feb 2024 20:52
Operator : MA/JU
Sample : P1299-03
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH6Z7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Title : SVOA CALIBRATION

37	17.263	2403	2410	2420	rBV	1356321	1895549	42.25%	4.164%
38	17.363	2420	2427	2439	rBV2	2718858	3821215	85.17%	8.394%
39	17.663	2474	2478	2480	rBV5	4797	5222	0.12%	0.011%
40	17.945	2524	2526	2530	rVB5	5514	6021	0.13%	0.013%
41	18.045	2541	2543	2549	rVB6	3607	5879	0.13%	0.013%
42	18.175	2559	2565	2575	rBV	103318	154226	3.44%	0.339%
43	18.251	2575	2578	2582	rVB3	7649	11848	0.26%	0.026%
44	18.610	2636	2639	2643	rBV6	5878	7054	0.16%	0.015%
45	18.657	2645	2647	2652	rVB6	4915	4741	0.11%	0.010%
46	19.228	2740	2744	2749	rVB3	36944	51698	1.15%	0.114%
47	19.298	2752	2756	2760	rVV	28796	40765	0.91%	0.090%
48	19.457	2779	2783	2790	rBV2	56988	76103	1.70%	0.167%
49	19.604	2805	2808	2812	rBV3	39300	49515	1.10%	0.109%
50	19.663	2812	2818	2827	rVV	3297030	4313861	96.15%	9.477%
51	19.922	2856	2862	2866	rVB5	18961	34823	0.78%	0.076%
52	21.192	3075	3078	3085	rVB4	69254	95344	2.13%	0.209%
53	21.463	3118	3124	3131	rBV	1547198	2023626	45.10%	4.445%
54	23.680	3493	3501	3511	rBV	2369820	4486755	100.00%	9.856%
55	23.833	3520	3527	3537	rVB	1089668	2205436	49.15%	4.845%




Sum of corrected areas: 45521193

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021424\
Data File : BN029779.D
Acq On : 14 Feb 2024 20:52
Operator : MA/JU
Sample : P1299-03
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH6Z7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

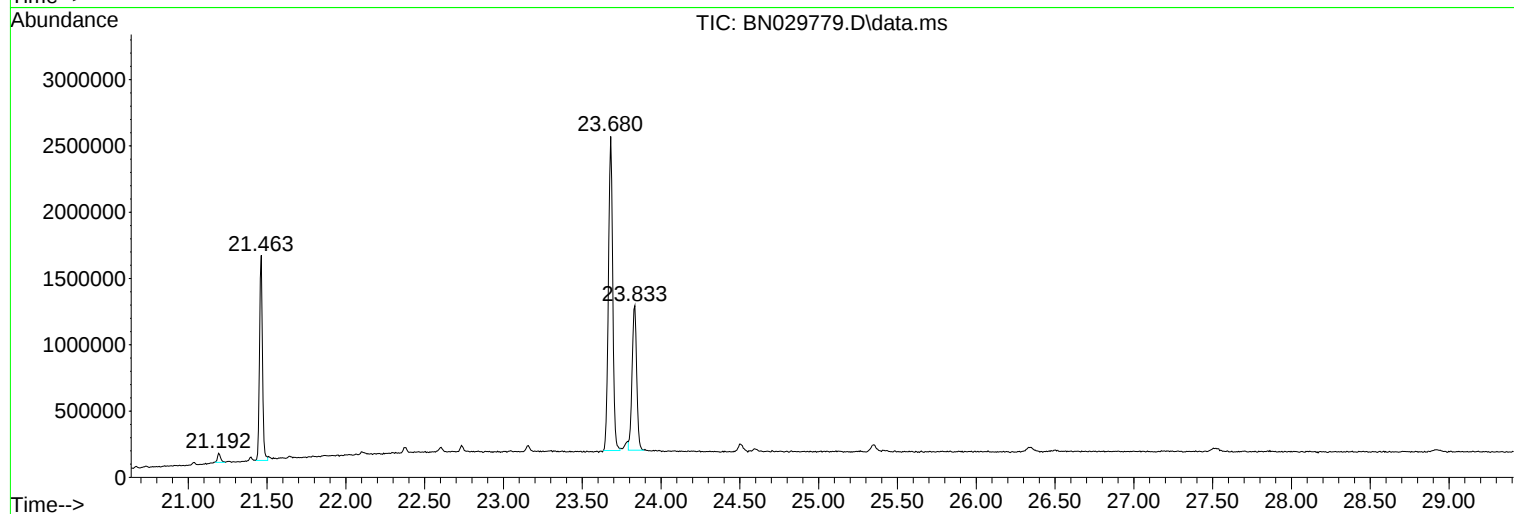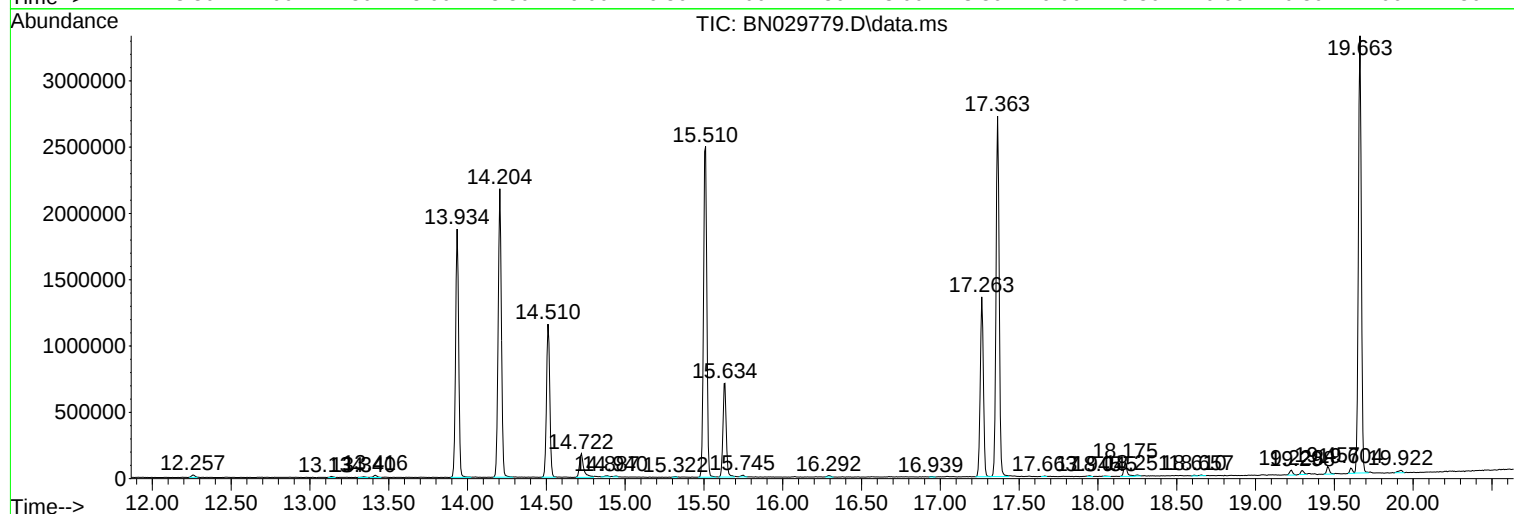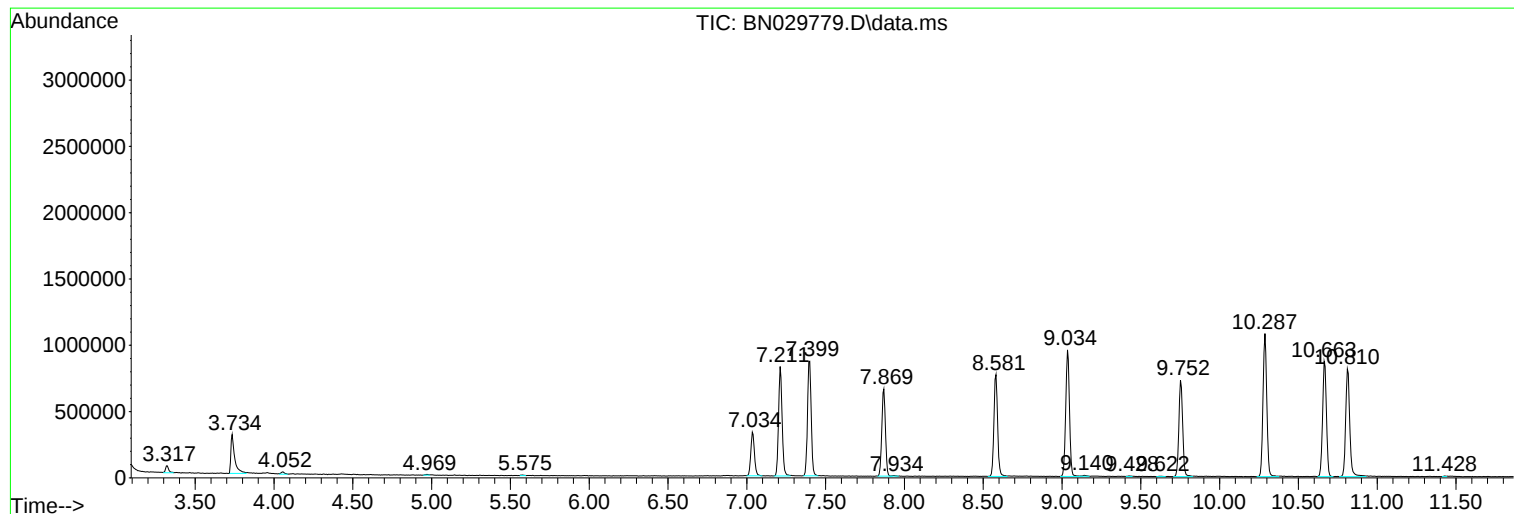

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021424\
Data File : BN029779.D
Acq On : 14 Feb 2024 20:52
Operator : MA/JU
Sample : P1299-03
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH6Z7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021424\
Data File : BN029779.D
Acq On : 14 Feb 2024 20:52
Operator : MA/JU
Sample : P1299-03
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH6Z7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------