

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021424\
 Data File : BN029791.D
 Acq On : 15 Feb 2024 04:40
 Operator : MA/JU
 Sample : PB158823BL
 Misc :
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK823

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029791.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.323	36	40	50	rVB	58038	84039	2.24%	0.191%
2	3.728	105	109	125	rBV	647073	1016621	27.15%	2.305%
3	4.058	161	165	170	rVB	19601	28471	0.76%	0.065%
4	6.093	509	511	516	rBV5	2185	3753	0.10%	0.009%
5	7.034	664	671	684	rBV	831984	1361907	36.37%	3.088%
6	7.211	695	701	711	rVV	674628	1042805	27.85%	2.364%
7	7.399	725	733	742	rBV	865525	1391102	37.15%	3.154%
8	7.869	806	813	823	rBV	718289	1139008	30.42%	2.582%
9	8.581	927	934	946	rBV	1000293	1626233	43.43%	3.687%
10	9.034	1004	1011	1022	rBV	793653	1307193	34.91%	2.964%
11	9.752	1125	1133	1145	rBV	630989	1065679	28.46%	2.416%
12	10.287	1216	1224	1235	rBV	955418	1593743	42.56%	3.613%
13	10.663	1280	1288	1297	rBV	917777	1561703	41.71%	3.541%
14	10.810	1305	1313	1326	rBV	916150	1648775	44.03%	3.738%
15	12.257	1554	1559	1565	rVB3	15026	24431	0.65%	0.055%
16	13.322	1737	1740	1743	rBV5	2376	3852	0.10%	0.009%
17	13.416	1750	1756	1761	rVB2	18819	29934	0.80%	0.068%
18	13.481	1764	1767	1771	rBV4	3852	4733	0.13%	0.011%
19	13.934	1837	1844	1857	rBV	1500702	2079990	55.55%	4.716%
20	14.204	1882	1890	1903	rBV	1740423	2582428	68.97%	5.855%
21	14.510	1936	1942	1951	rBV	1253793	1846952	49.33%	4.187%
22	14.722	1971	1978	2000	rBV	643888	1086112	29.01%	2.462%
23	15.510	2105	2112	2124	rBV	2101751	3033096	81.01%	6.876%
24	15.634	2127	2133	2143	rBV	597591	833393	22.26%	1.889%
25	15.745	2148	2152	2158	rVB3	9829	14620	0.39%	0.033%
26	16.292	2241	2245	2249	rBV5	6895	9855	0.26%	0.022%
27	17.051	2369	2374	2380	rVB5	3836	6246	0.17%	0.014%
28	17.263	2403	2410	2420	rBV	1513113	2144170	57.27%	4.861%
29	17.363	2420	2427	2442	rVV2	2296957	3294596	87.99%	7.469%
30	18.175	2561	2565	2570	rBV7	5626	9272	0.25%	0.021%
31	19.228	2739	2744	2749	rBV3	28941	41127	1.10%	0.093%
32	19.298	2752	2756	2761	rVV	24027	32350	0.86%	0.073%
33	19.463	2782	2784	2789	rVB6	5411	6038	0.16%	0.014%
34	19.663	2812	2818	2825	rBV	2792035	3744280	100.00%	8.489%
35	21.463	3119	3124	3135	rBV2	1698232	2278003	60.84%	5.164%
36	23.680	3494	3501	3513	rBV2	1853854	3702792	98.89%	8.395%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021424\
Data File : BN029791.D
Acq On : 15 Feb 2024 04:40
Operator : MA/JU
Sample : PB158823BL
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK823

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Title : SVOA CALIBRATION

37	23.833	3521	3527	3541	rVB	1164561	2429592	64.89%	5.508%
----	--------	------	------	------	-----	---------	---------	--------	--------




Sum of corrected areas: 44108894

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021424\
Data File : BN029791.D
Acq On : 15 Feb 2024 04:40
Operator : MA/JU
Sample : PB158823BL
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK823

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

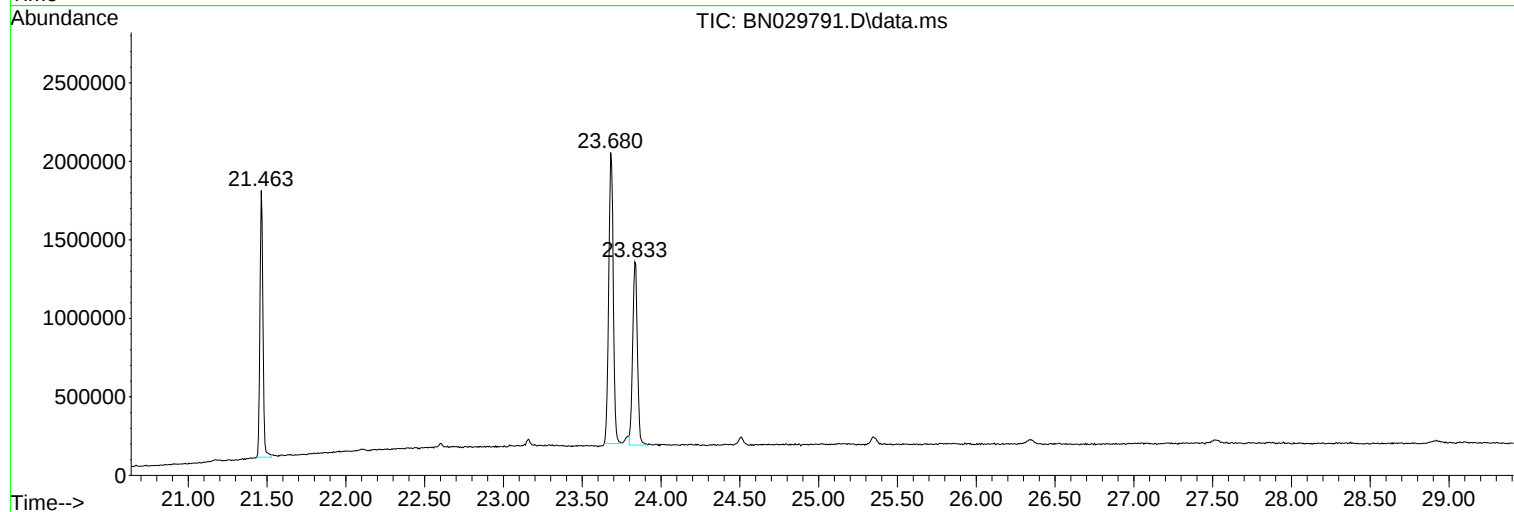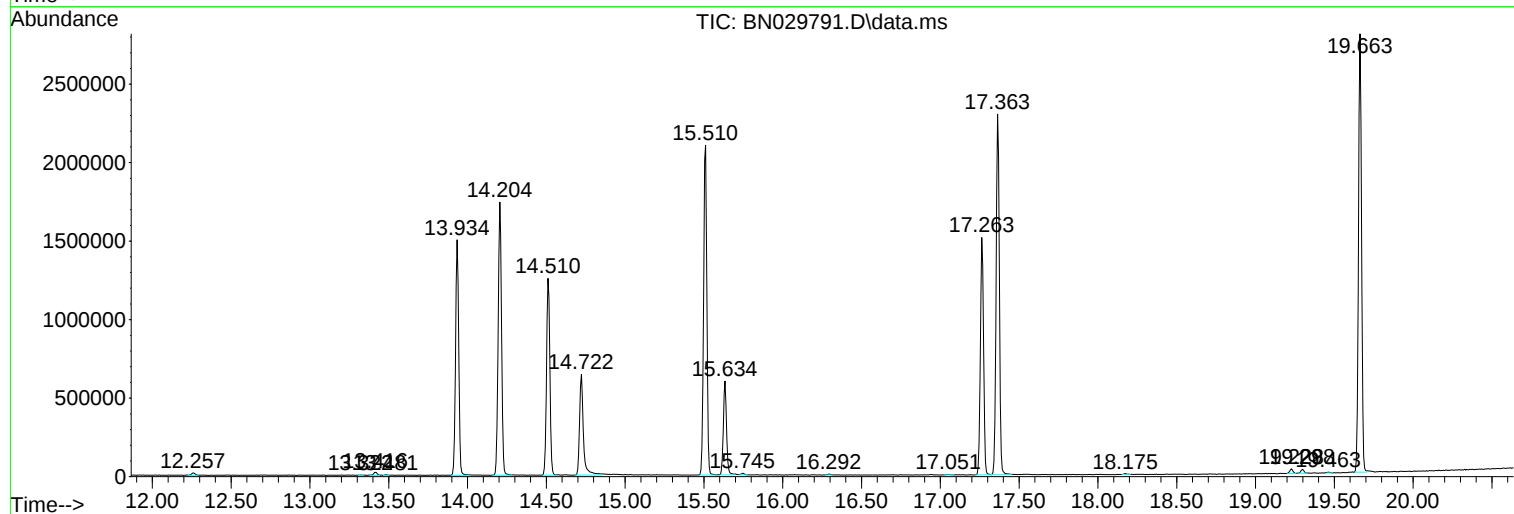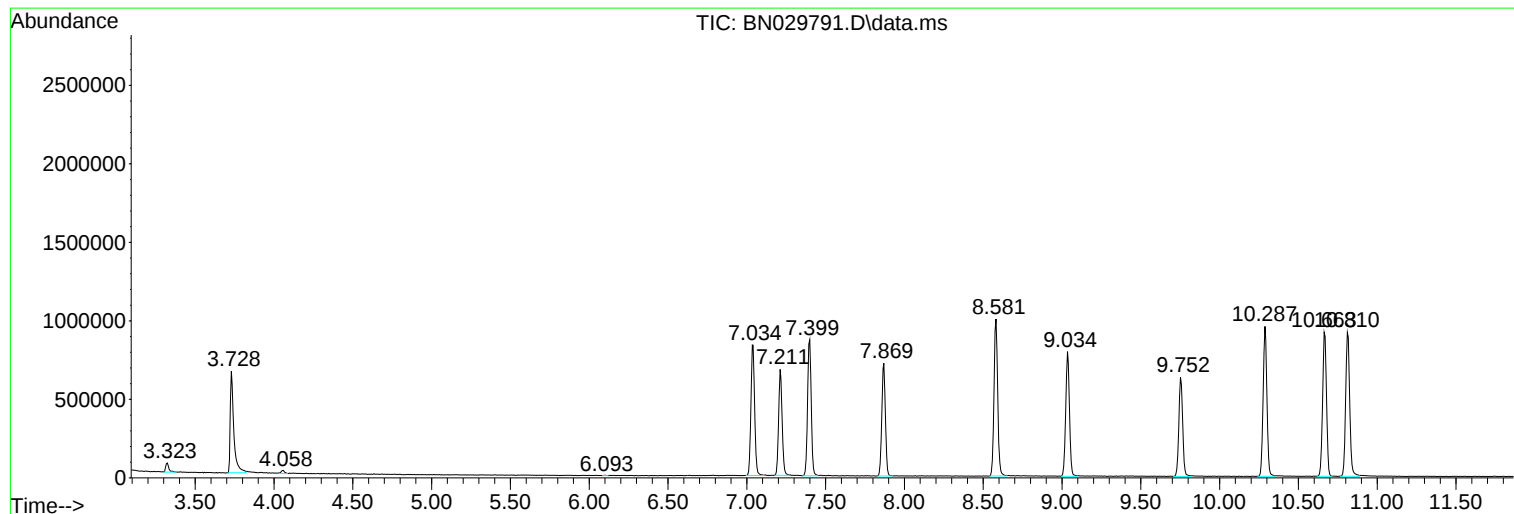

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021424\
Data File : BN029791.D
Acq On : 15 Feb 2024 04:40
Operator : MA/JU
Sample : PB158823BL
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK823

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021424\
Data File : BN029791.D
Acq On : 15 Feb 2024 04:40
Operator : MA/JU
Sample : PB158823BL
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK823

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------