

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021424\
 Data File : BN029805.D
 Acq On : 15 Feb 2024 13:05
 Operator : MA/JU
 Sample : PB158950BL
 Misc :
 ALS Vial : 84 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK950

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029805.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.317	36	39	46	rVB	43539	54428	1.87%	0.156%
2	3.728	105	109	129	rBV	475891	764171	26.23%	2.190%
3	4.052	161	164	172	rVB	12783	20649	0.71%	0.059%
4	5.711	445	446	450	rBV3	2348	3225	0.11%	0.009%
5	6.099	511	512	516	rBV4	2613	3051	0.10%	0.009%
6	7.034	665	671	680	rBV	630986	1000687	34.35%	2.868%
7	7.211	695	701	709	rBV	497175	761539	26.14%	2.183%
8	7.393	725	732	743	rBV	640074	1025817	35.21%	2.940%
9	7.864	806	812	823	rVB	571383	929163	31.90%	2.663%
10	8.264	876	880	883	rBV6	2445	3157	0.11%	0.009%
11	8.581	927	934	949	rBV	728207	1226391	42.10%	3.515%
12	9.034	1003	1011	1023	rBV	601436	986363	33.86%	2.827%
13	9.752	1124	1133	1145	rBV	472632	807016	27.70%	2.313%
14	10.287	1215	1224	1236	rBV	727458	1214090	41.68%	3.480%
15	10.663	1281	1288	1300	rVB	796728	1308028	44.90%	3.749%
16	10.810	1304	1313	1332	rBV	710210	1280362	43.95%	3.669%
17	11.093	1360	1361	1365	rVB4	3216	3732	0.13%	0.011%
18	12.252	1552	1558	1569	rBV4	10805	22258	0.76%	0.064%
19	13.416	1749	1756	1760	rBV3	15429	26599	0.91%	0.076%
20	13.934	1837	1844	1858	rBV	1226291	1670226	57.34%	4.787%
21	14.204	1883	1890	1901	rBV	1355407	2035209	69.87%	5.833%
22	14.510	1935	1942	1952	rBV	1080075	1610576	55.29%	4.616%
23	14.722	1971	1978	1996	rBV	457167	796839	27.35%	2.284%
24	15.504	2104	2111	2122	rBV	1630680	2400994	82.42%	6.881%
25	15.634	2126	2133	2145	rVV	443441	634739	21.79%	1.819%
26	15.745	2147	2152	2156	rVB4	7546	11139	0.38%	0.032%
27	16.292	2241	2245	2249	rBV5	6185	7665	0.26%	0.022%
28	16.945	2352	2356	2359	rVB4	3979	4501	0.15%	0.013%
29	17.022	2366	2369	2370	rBV3	2977	3274	0.11%	0.009%
30	17.045	2371	2373	2376	rVV3	3727	4119	0.14%	0.012%
31	17.110	2381	2384	2387	rBV5	2087	3894	0.13%	0.011%
32	17.263	2404	2410	2420	rBV	1334608	1841383	63.21%	5.277%
33	17.363	2420	2427	2440	rBV	1808521	2585733	88.76%	7.411%
34	17.816	2500	2504	2507	rBV5	2408	4082	0.14%	0.012%
35	17.939	2523	2525	2530	rVB6	3046	3999	0.14%	0.011%
36	18.175	2561	2565	2570	rBV7	5108	9601	0.33%	0.028%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021424\
Data File : BN029805.D
Acq On : 15 Feb 2024 13:05
Operator : MA/JU
Sample : PB158950BL
Misc :
ALS Vial : 84 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK950

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Title : SVOA CALIBRATION

37	19.228	2740	2744	2748	rVV2	24778	32975	1.13%	0.095%
38	19.292	2752	2755	2761	rVV2	19318	27933	0.96%	0.080%
39	19.469	2779	2785	2787	rBV7	5108	8705	0.30%	0.025%
40	19.616	2808	2810	2812	rBV3	4878	4673	0.16%	0.013%
41	19.663	2812	2818	2827	rVV	2088828	2913040	100.00%	8.349%
42	21.463	3119	3124	3131	rBV	1532239	1896785	65.11%	5.436%
43	23.680	3493	3501	3510	rBV	1435928	2842562	97.58%	8.147%
44	23.786	3515	3519	3520	rVV2	87090	122555	4.21%	0.351%
45	23.833	3521	3527	3537	rVB	968117	1974439	67.78%	5.659%




Sum of corrected areas: 34892366

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021424\
Data File : BN029805.D
Acq On : 15 Feb 2024 13:05
Operator : MA/JU
Sample : PB158950BL
Misc :
ALS Vial : 84 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK950

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

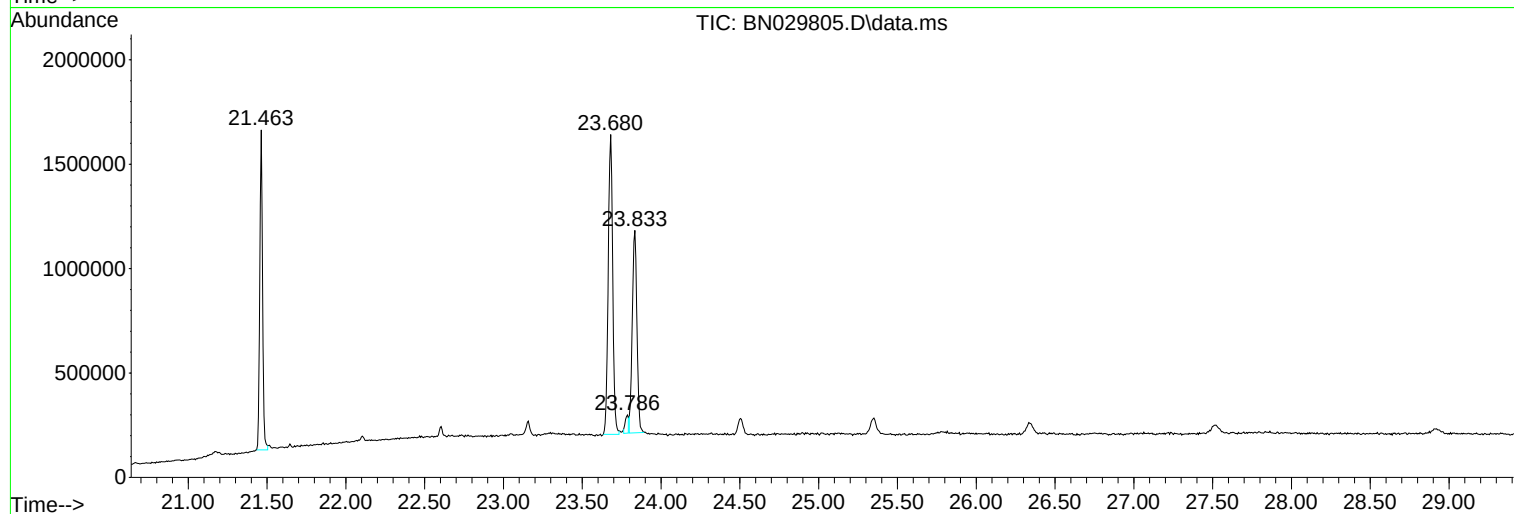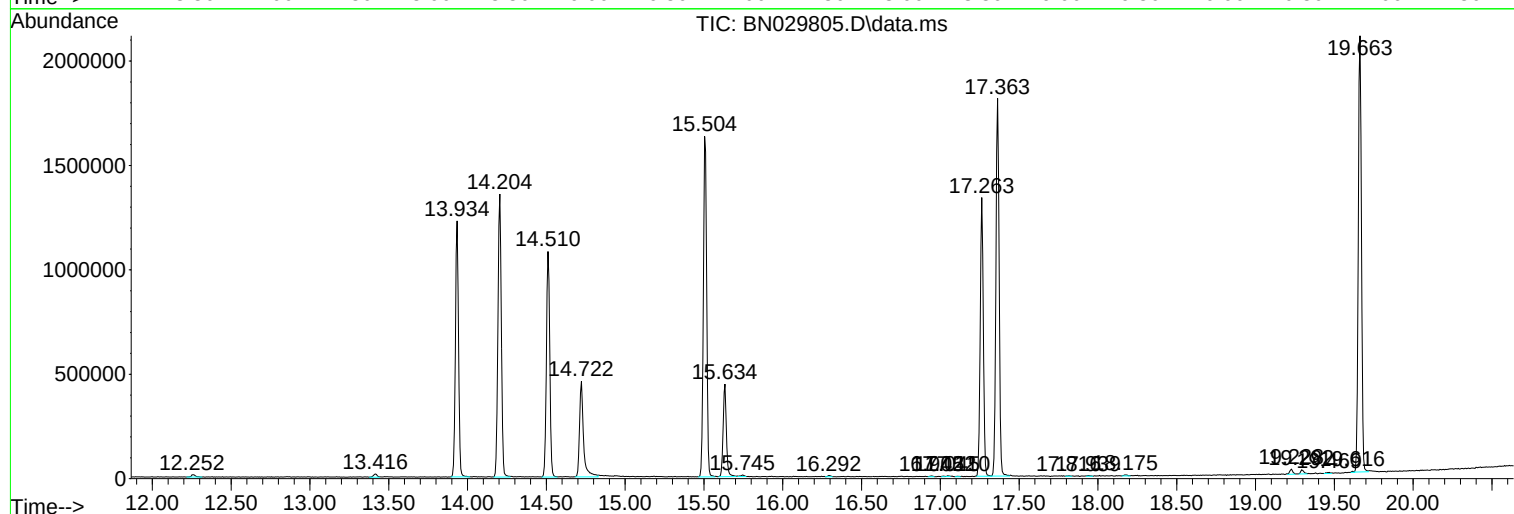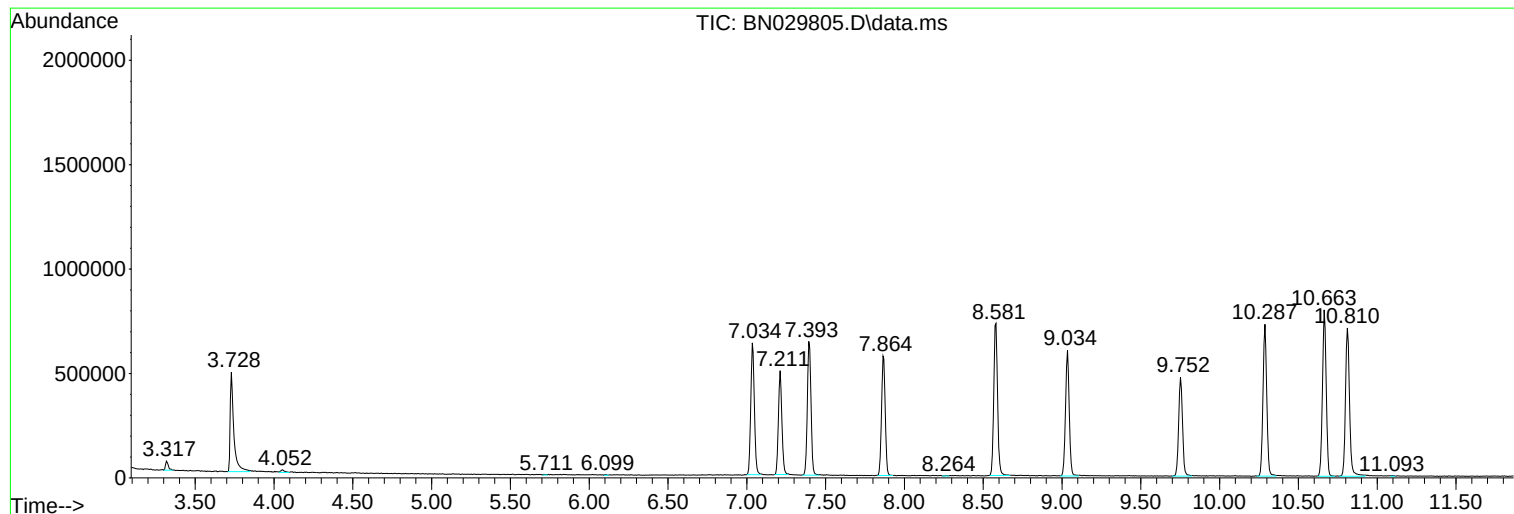

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021424\
Data File : BN029805.D
Acq On : 15 Feb 2024 13:05
Operator : MA/JU
Sample : PB158950BL
Misc :
ALS Vial : 84 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK950

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021424\
Data File : BN029805.D
Acq On : 15 Feb 2024 13:05
Operator : MA/JU
Sample : PB158950BL
Misc :
ALS Vial : 84 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK950

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------