

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021424\
 Data File : BN029811.D
 Acq On : 15 Feb 2024 17:16
 Operator : MA/JU
 Sample : P1445-10
 Misc :
 ALS Vial : 91 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SVOC-GPC2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029811.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.058	161	165	170	rVB2	11370	17046	0.87%	0.174%
2	4.911	308	310	315	rVB5	2108	2026	0.10%	0.021%
3	4.981	321	322	327	rVB4	3110	3583	0.18%	0.037%
4	5.105	341	343	346	rBV4	1951	2252	0.11%	0.023%
5	5.505	409	411	413	rBV3	2418	2176	0.11%	0.022%
6	5.875	472	474	480	rVB6	2635	4548	0.23%	0.046%
7	6.899	646	648	650	rBV3	2103	2123	0.11%	0.022%
8	7.028	669	670	673	rBV3	2067	2032	0.10%	0.021%
9	7.075	676	678	680	rBV3	1971	2323	0.12%	0.024%
10	7.093	680	681	685	rVB3	2293	2190	0.11%	0.022%
11	7.705	781	785	787	rBV5	2501	3355	0.17%	0.034%
12	7.869	806	813	820	rBV	578530	947435	48.12%	9.678%
13	8.081	845	849	851	rBV5	1696	2120	0.11%	0.022%
14	8.281	881	883	887	rBV3	2117	2122	0.11%	0.022%
15	8.487	913	918	920	rVB5	2475	3146	0.16%	0.032%
16	8.581	931	934	937	rBV5	1850	2924	0.15%	0.030%
17	9.058	1013	1015	1018	rVB4	2029	2356	0.12%	0.024%
18	9.169	1029	1034	1038	rVB5	1767	3268	0.17%	0.033%
19	9.222	1041	1043	1046	rVB4	2003	2257	0.11%	0.023%
20	9.581	1102	1104	1109	rVB4	1759	3147	0.16%	0.032%
21	9.640	1112	1114	1118	rBV5	1448	2154	0.11%	0.022%
22	10.663	1278	1288	1298	rBV	784197	1337557	67.94%	13.664%
23	11.493	1426	1429	1432	rBV4	1928	2476	0.13%	0.025%
24	12.187	1544	1547	1550	rBV5	1357	2315	0.12%	0.024%
25	12.840	1653	1658	1659	rBV4	1518	2107	0.11%	0.022%
26	13.075	1695	1698	1702	rBV5	1592	2081	0.11%	0.021%
27	13.504	1765	1771	1772	rVB5	1634	2306	0.12%	0.024%
28	14.081	1867	1869	1871	rVB3	2061	2014	0.10%	0.021%
29	14.110	1871	1874	1878	rBV6	2529	3440	0.17%	0.035%
30	14.210	1887	1891	1892	rBV3	2483	2344	0.12%	0.024%
31	14.510	1935	1942	1955	rBV	1102592	1618129	82.19%	16.530%
32	14.775	1983	1987	1989	rBV5	1821	2535	0.13%	0.026%
33	14.922	2008	2012	2013	rBV4	2003	2345	0.12%	0.024%
34	16.187	2222	2227	2230	rBV5	1689	2708	0.14%	0.028%
35	16.316	2245	2249	2251	rVB4	1725	2280	0.12%	0.023%
36	16.351	2251	2255	2256	rBV3	1768	2022	0.10%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021424\
 Data File : BN029811.D
 Acq On : 15 Feb 2024 17:16
 Operator : MA/JU
 Sample : P1445-10
 Misc :
 ALS Vial : 91 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SVOC-GPC2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

37	16.828	2332	2336	2337	rVB3	2242	2424	0.12%	0.025%
38	17.039	2370	2372	2373	rBV2	2436	2174	0.11%	0.022%
39	17.263	2403	2410	2423	rBV	1304419	1886327	95.81%	19.270%
40	17.363	2423	2427	2430	rVB6	2547	4455	0.23%	0.046%
41	17.457	2440	2443	2447	rBV5	1631	3057	0.16%	0.031%
42	17.628	2470	2472	2477	rVB5	2302	3599	0.18%	0.037%
43	17.669	2477	2479	2481	rBV3	2538	2161	0.11%	0.022%
44	17.692	2481	2483	2486	rBV3	2204	3240	0.16%	0.033%
45	18.139	2556	2559	2561	rBV4	2369	2964	0.15%	0.030%
46	18.286	2582	2584	2586	rVB3	2482	2044	0.10%	0.021%
47	18.310	2586	2588	2591	rBV3	2204	3044	0.15%	0.031%
48	18.410	2603	2605	2608	rBV4	1972	2407	0.12%	0.025%
49	18.704	2653	2655	2658	rBV4	1977	2040	0.10%	0.021%
50	19.422	2774	2777	2780	rBV5	4085	4962	0.25%	0.051%
51	19.616	2808	2810	2813	rBV3	3554	2540	0.13%	0.026%
52	19.733	2829	2830	2833	rBV3	3656	3090	0.16%	0.032%
53	19.951	2865	2867	2868	rBV2	3458	2157	0.11%	0.022%
54	19.969	2868	2870	2871	rBV2	3072	2211	0.11%	0.023%
55	21.463	3119	3124	3132	rBV	1455019	1884214	95.71%	19.248%
56	23.833	3520	3527	3539	rVB	976769	1968734	100.00%	20.112%




Sum of corrected areas: 9789086

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021424\
Data File : BN029811.D
Acq On : 15 Feb 2024 17:16
Operator : MA/JU
Sample : P1445-10
Misc :
ALS Vial : 91 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

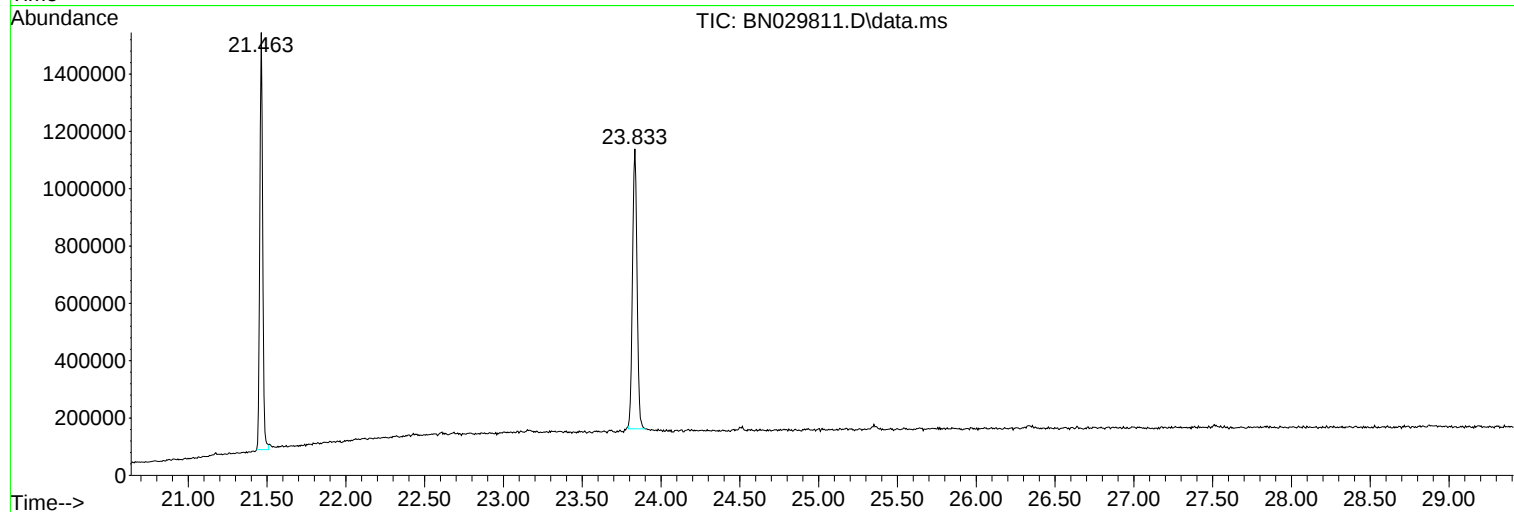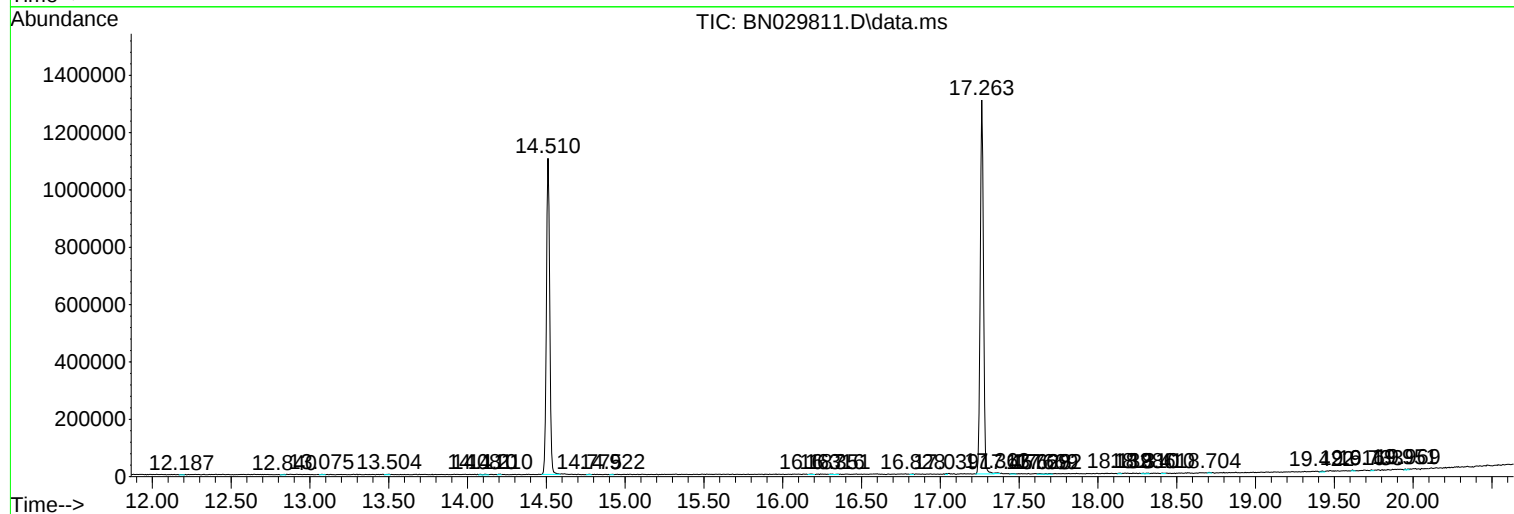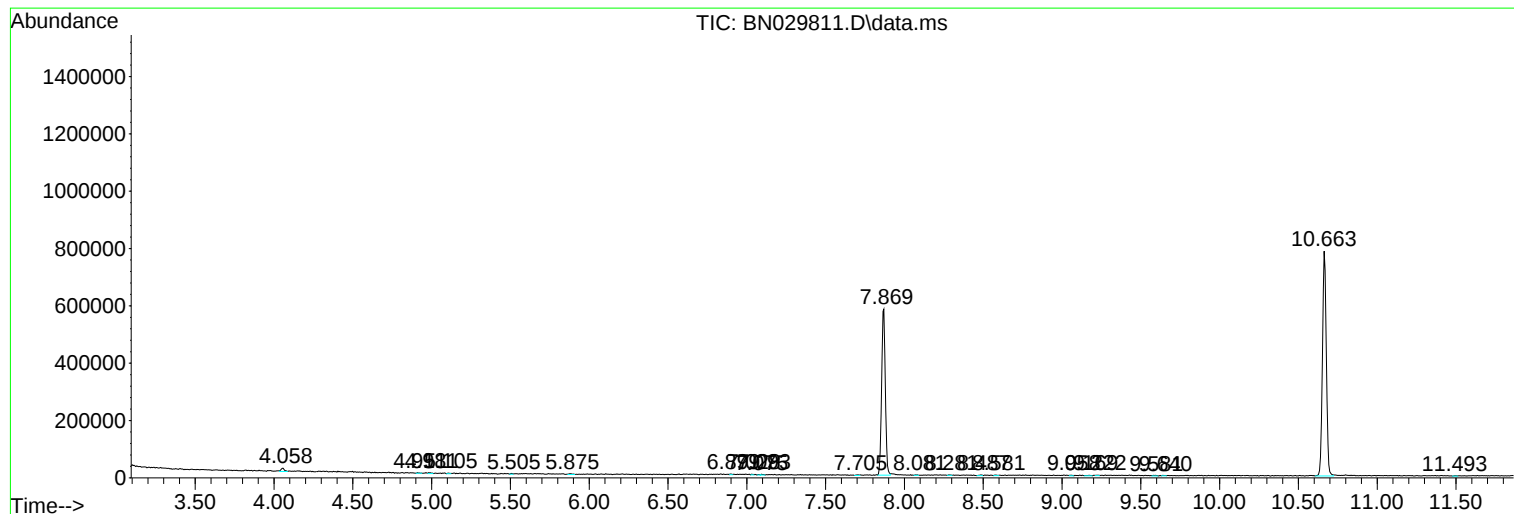

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021424\
Data File : BN029811.D
Acq On : 15 Feb 2024 17:16
Operator : MA/JU
Sample : P1445-10
Misc :
ALS Vial : 91 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021424\
Data File : BN029811.D
Acq On : 15 Feb 2024 17:16
Operator : MA/JU
Sample : P1445-10
Misc :
ALS Vial : 91 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc