

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021424\
 Data File : BN029824.D
 Acq On : 16 Feb 2024 12:10
 Operator : MA/JU
 Sample : PB158885TB 10X
 Misc :
 ALS Vial : 105 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SLEB885

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029824.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.322	36	40	50	rVB	48376	70327	2.26%	0.196%
2	3.728	106	109	126	rBV	520712	847595	27.25%	2.360%
3	4.052	161	164	171	rVB2	14952	19611	0.63%	0.055%
4	5.781	457	458	463	rVB4	2873	3470	0.11%	0.010%
5	6.399	562	563	568	rVB5	2453	3394	0.11%	0.009%
6	7.034	662	671	682	rBV	696543	1103380	35.48%	3.072%
7	7.210	695	701	716	rVB	549611	863659	27.77%	2.405%
8	7.393	725	732	743	rBV	711376	1130351	36.35%	3.147%
9	7.863	805	812	823	rVB	583573	938212	30.17%	2.612%
10	8.575	925	933	947	rBV	795804	1326846	42.66%	3.694%
11	9.034	1003	1011	1021	rVV	647449	1069216	34.38%	2.977%
12	9.134	1024	1028	1032	rVB6	2823	4294	0.14%	0.012%
13	9.751	1124	1133	1141	rBV	511401	854320	27.47%	2.379%
14	10.287	1216	1224	1239	rBV	764515	1300073	41.80%	3.620%
15	10.663	1280	1288	1298	rVB	782648	1291704	41.53%	3.596%
16	10.810	1304	1313	1333	rBV	760105	1361771	43.79%	3.792%
17	12.263	1553	1560	1564	rVB3	12081	18912	0.61%	0.053%
18	13.416	1752	1756	1760	rVB5	4867	6741	0.22%	0.019%
19	13.698	1800	1804	1809	rVB6	2127	3565	0.11%	0.010%
20	13.934	1837	1844	1854	rBV	1231090	1753423	56.38%	4.882%
21	14.204	1882	1890	1903	rBV	1418484	2118110	68.11%	5.897%
22	14.392	1919	1922	1924	rBV4	2702	3685	0.12%	0.010%
23	14.510	1935	1942	1949	rBV	1039565	1517970	48.81%	4.226%
24	14.722	1969	1978	1996	rBV	433542	813980	26.17%	2.266%
25	15.504	2104	2111	2124	rBV	1761648	2484866	79.90%	6.919%
26	15.628	2126	2132	2147	rVV	441884	637830	20.51%	1.776%
27	15.739	2147	2151	2155	rVB4	6604	8700	0.28%	0.024%
28	16.292	2240	2245	2249	rBV4	6628	9941	0.32%	0.028%
29	17.051	2371	2374	2378	rBV6	3536	6664	0.21%	0.019%
30	17.263	2403	2410	2420	rBV	1206557	1735842	55.81%	4.833%
31	17.363	2420	2427	2442	rVV	1827376	2646480	85.10%	7.369%
32	19.222	2739	2743	2748	rVB3	20296	28567	0.92%	0.080%
33	19.298	2752	2756	2760	rBV2	18023	25414	0.82%	0.071%
34	19.616	2805	2810	2812	rBV6	4071	6573	0.21%	0.018%
35	19.663	2812	2818	2825	rBV	2227485	3032324	97.50%	8.443%
36	21.463	3118	3124	3138	rBV	1320337	1855656	59.67%	5.167%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021424\
Data File : BN029824.D
Acq On : 16 Feb 2024 12:10
Operator : MA/JU
Sample : PB158885TB 10X
Misc :
ALS Vial : 105 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SLEB885

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Title : SVOA CALIBRATION

37	23.680	3493	3501	3513	rBV2	1548244	3110022	100.00%	8.659%
38	23.827	3520	3526	3536	rVB	954648	1902373	61.17%	5.297%




Sum of corrected areas: 35915861

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021424\
Data File : BN029824.D
Acq On : 16 Feb 2024 12:10
Operator : MA/JU
Sample : PB158885TB 10X
Misc :
ALS Vial : 105 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SLEB885

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

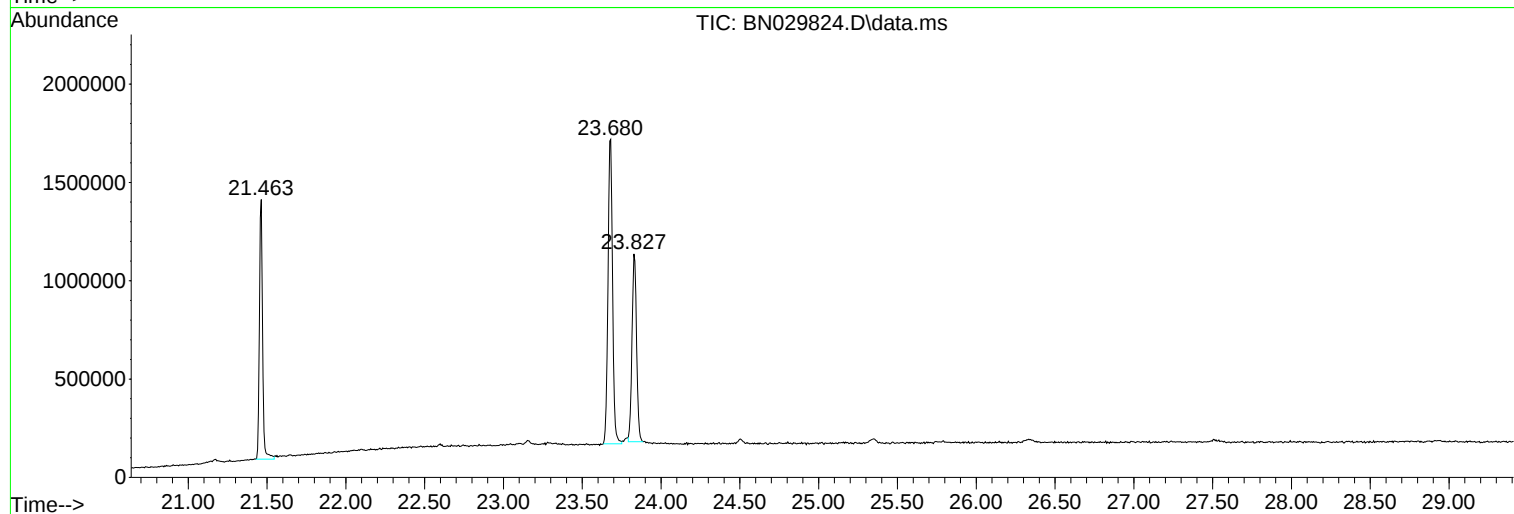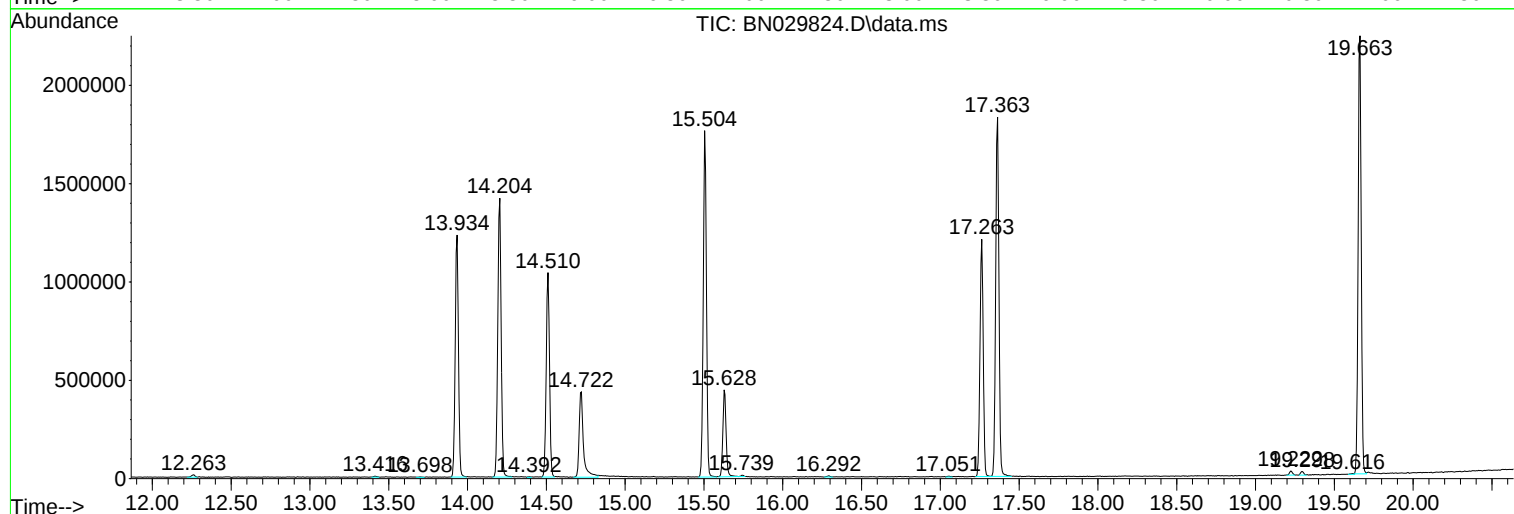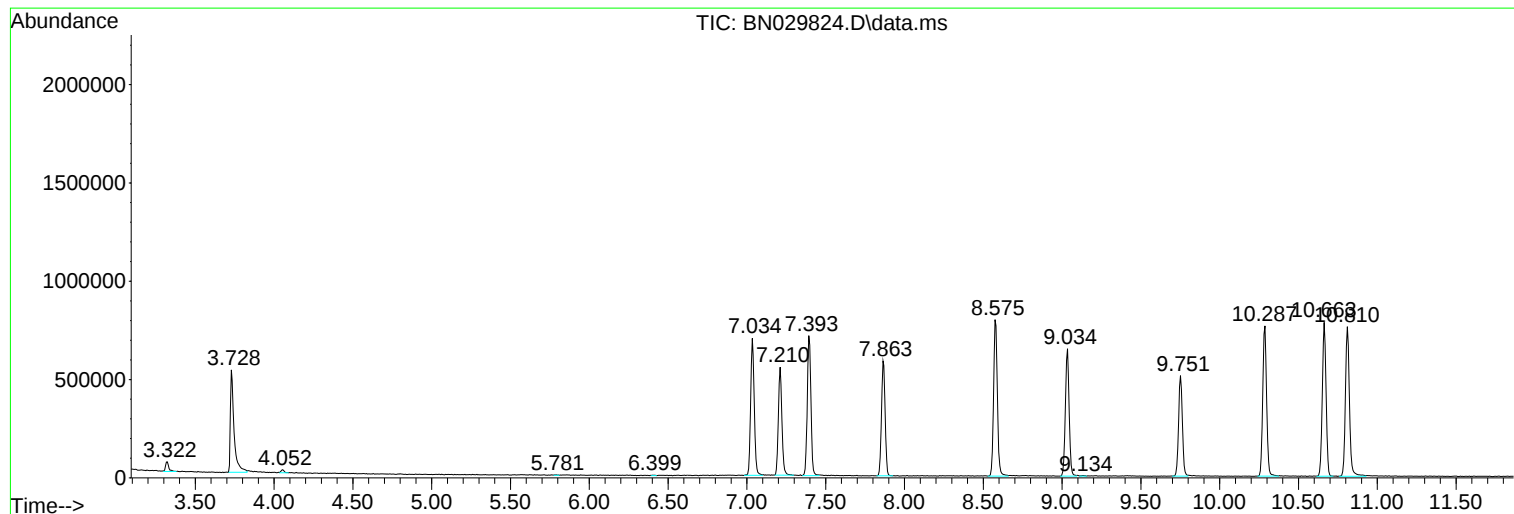

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021424\
Data File : BN029824.D
Acq On : 16 Feb 2024 12:10
Operator : MA/JU
Sample : PB158885TB 10X
Misc :
ALS Vial : 105 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SLEB885

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021424\
Data File : BN029824.D
Acq On : 16 Feb 2024 12:10
Operator : MA/JU
Sample : PB158885TB 10X
Misc :
ALS Vial : 105 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SLEB885

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc