
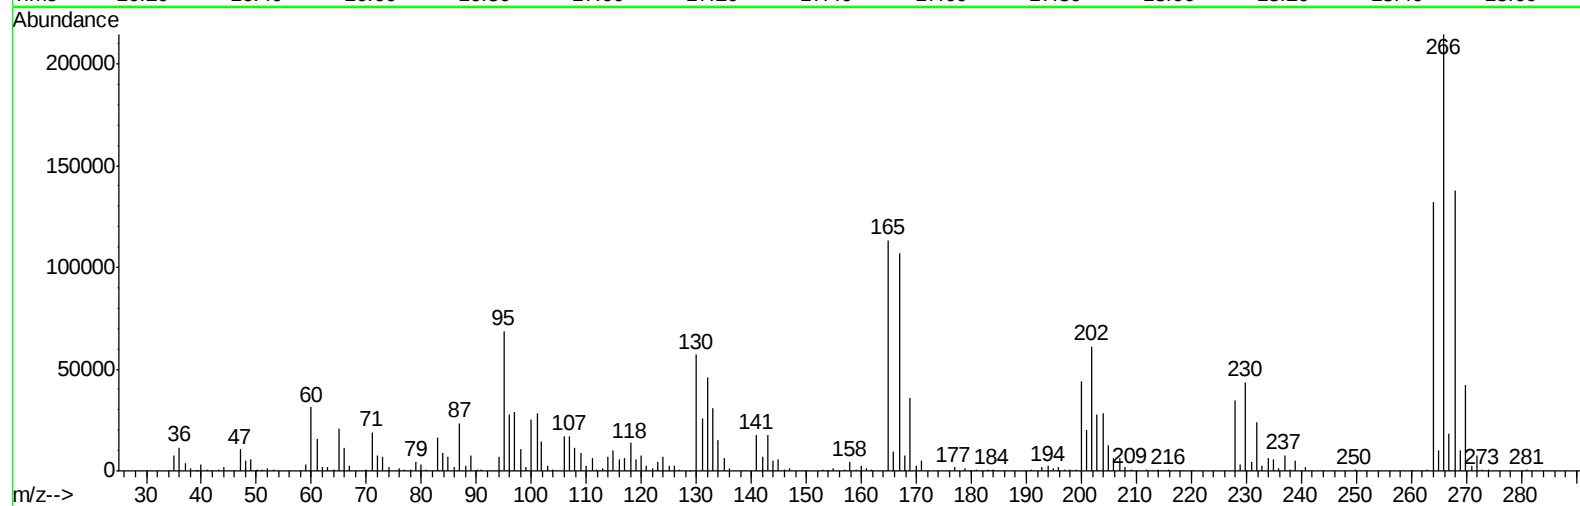


Data Path : Z:\HPCHEM1\BNA N\DATA\BN021518\
Data File : BN000085.D
Acq On : 15 Feb 2018 08:23
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 16 07:50:53 2018
Quant Method : Z:\HPCHEM1\BNA N\METHODS\8270-BN020718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 07 18:24:45 2018
Response via : Initial Calibration

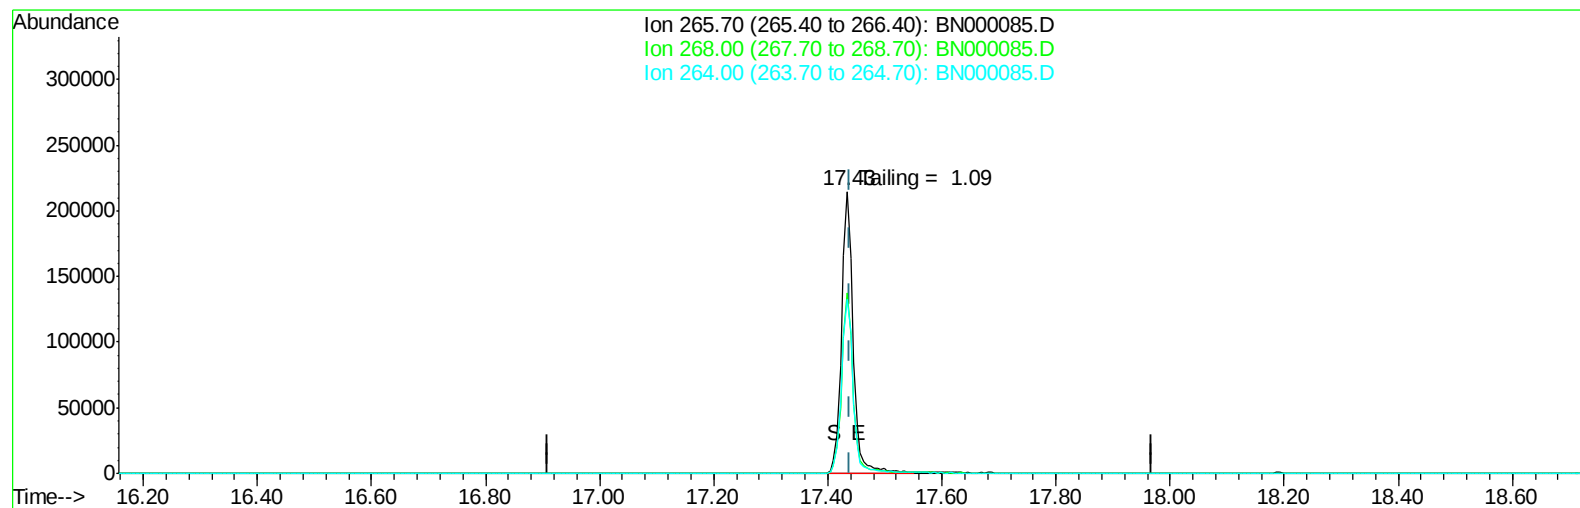

TIC: BN000085.D

(69) Pentachlorophenol (C)



17.434min (-0.005) 69122.51ng

response 300990

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	64.11
264.00	62.00	61.63
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA N\DATA\BN021518\
Data File : BN000085.D
Acq On : 15 Feb 2018 08:23
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 16 07:50:53 2018
Quant Method : Z:\HPCHEM1\BNA N\METHODS\8270-BN020718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 07 18:24:45 2018
Response via : Initial Calibration

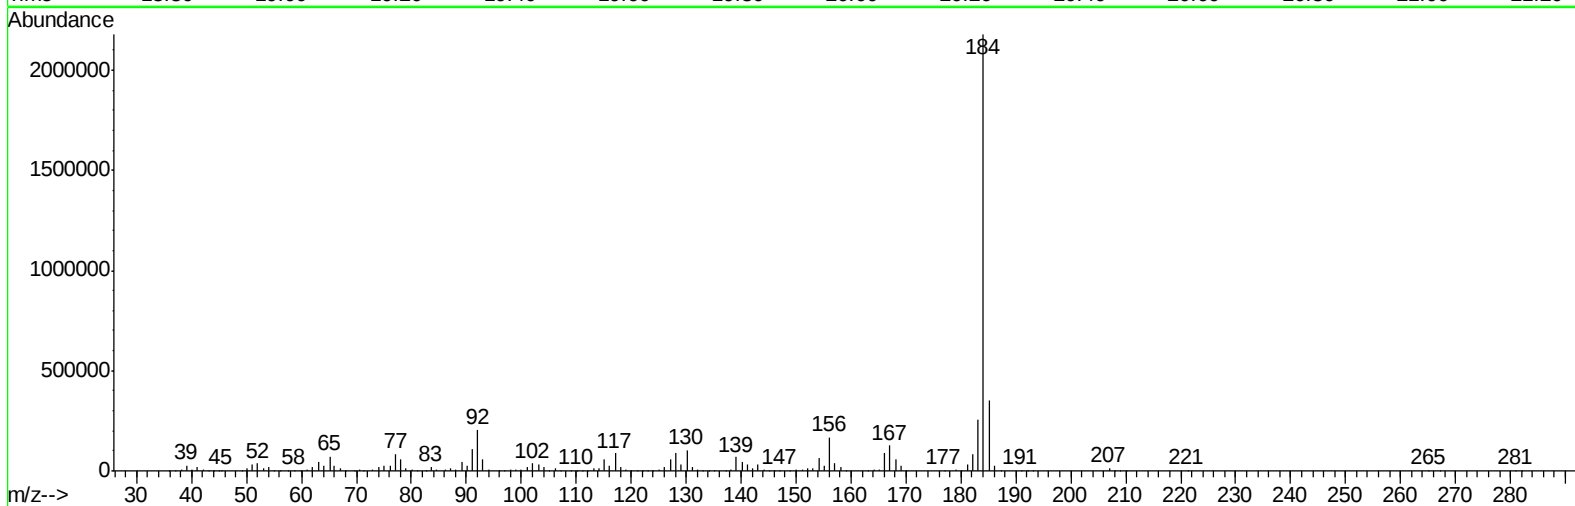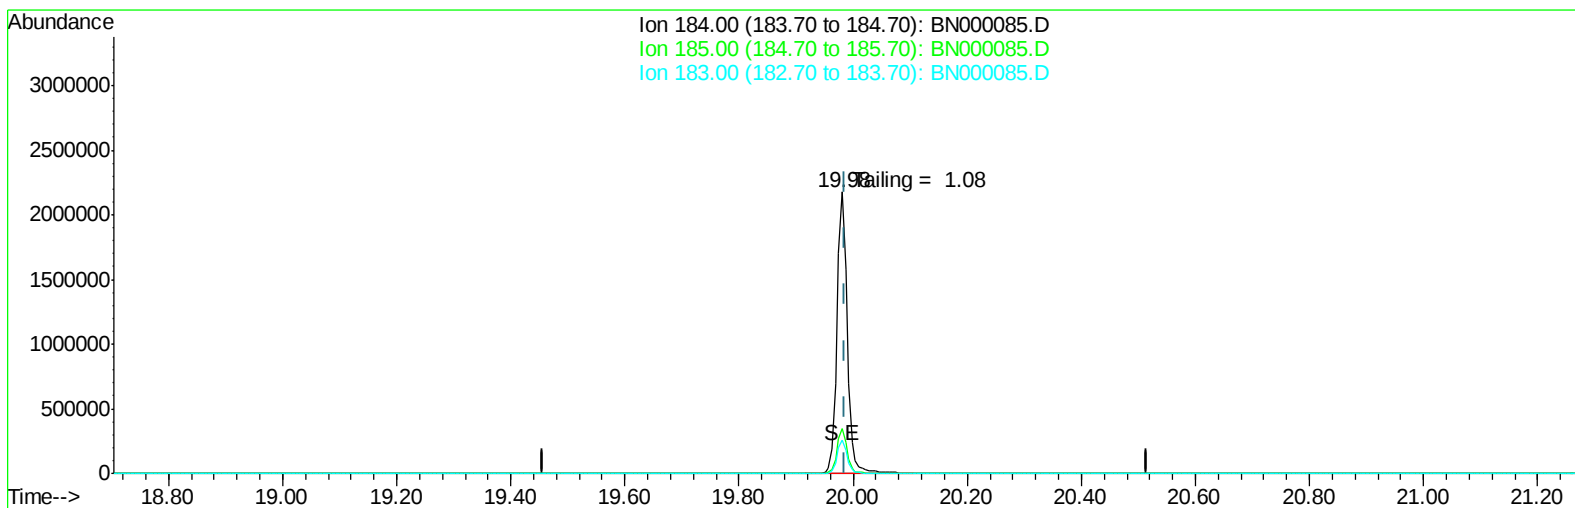

TIC: BN000085.D

(76) Benzidine

19.981min (-0.006) 7303.50ng

response 2721841

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	16.01
183.00	13.30	11.87
0.00	0.00	0.00