
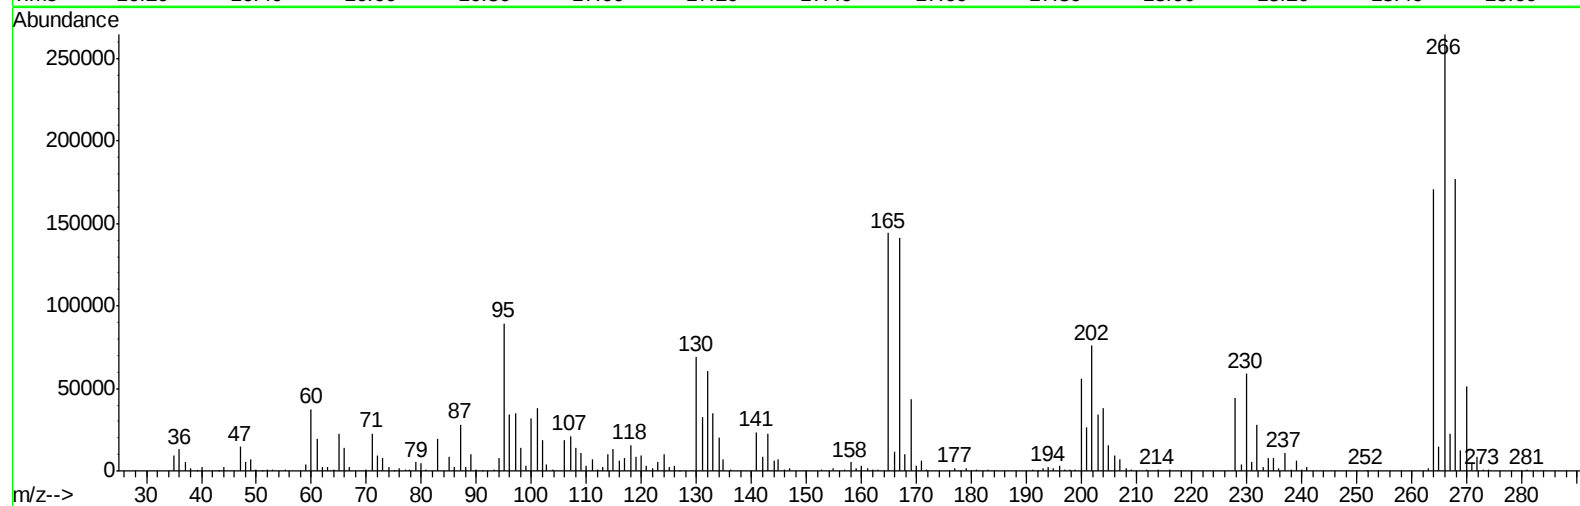


Data Path : Z:\HPCHEM1\BNA N\DATA\BN021518\
Data File : BN000099.D
Acq On : 15 Feb 2018 16:24
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 16 07:52:36 2018
Quant Method : Z:\HPCHEM1\BNA N\METHODS\8270-BN020718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 07 18:24:45 2018
Response via : Initial Calibration

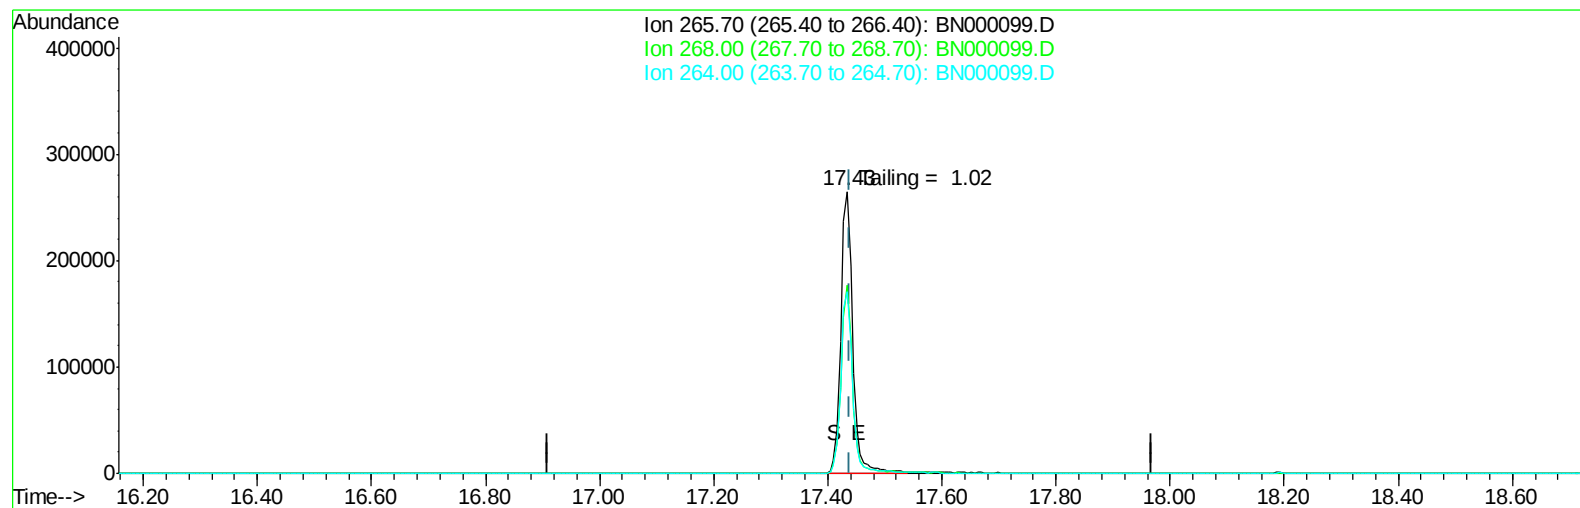

TIC: BN000099.D

(69) Pentachlorophenol (C)



17.433min (-0.006) 400662.82ng

response 383324

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	67.00
264.00	62.00	64.65
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA N\DATA\BN021518\
Data File : BN000099.D
Acq On : 15 Feb 2018 16:24
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 16 07:52:36 2018
Quant Method : Z:\HPCHEM1\BNA N\METHODS\8270-BN020718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 07 18:24:45 2018
Response via : Initial Calibration

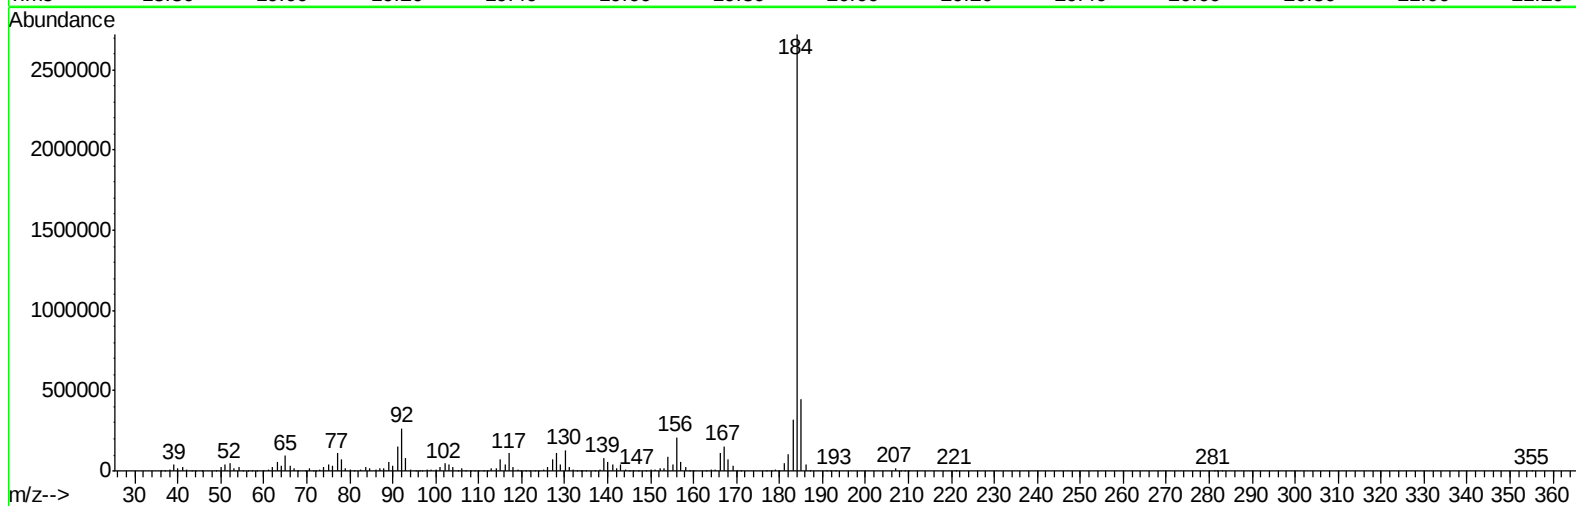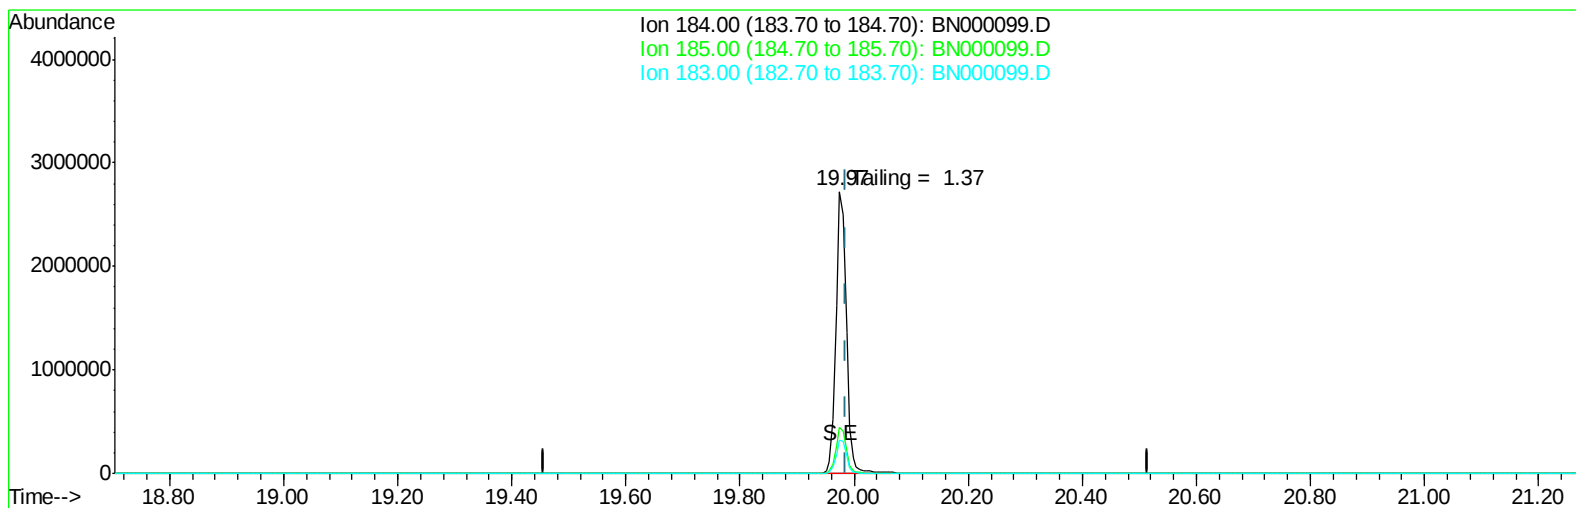

TIC: BN000099.D

(76) Benzidine

19.975min (-0.012) 112826.10ng

response 3441928

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	16.55
183.00	13.30	11.69
0.00	0.00	0.00