

Data Path : Z:\HPCHEM1\BNA N\DATA\BN021518\
Data File : BN000087.D
Acq On : 15 Feb 2018 09:31
Operator : JU/SJ
Sample : PB105903BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB105903BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_N\METHODS\8270-BN020718.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.940	494	502	523	rBV	10317510	16841130	44.91%	8.230%
2	7.587	773	782	797	rBV	10598298	18040111	48.10%	8.815%
3	7.981	841	849	864	rBV	10631253	18113505	48.30%	8.851%
4	8.463	923	931	940	rVB	2012869	3307281	8.82%	1.616%
5	8.792	979	987	997	rVB	7962098	13345312	35.58%	6.521%
6	9.639	1118	1131	1142	rBV	6198657	10508539	28.02%	5.135%
7	11.304	1405	1414	1422	rBV	3015838	5263955	14.04%	2.572%
8	13.704	1815	1822	1830	rBV	18487630	27053292	72.14%	13.220%
9	15.069	2047	2054	2067	rBV2	4601329	7203430	19.21%	3.520%
10	16.539	2297	2304	2332	rBV	11886753	17257112	46.01%	8.433%
11	17.792	2510	2517	2530	rBV2	6231861	8946541	23.86%	4.372%
12	20.357	2946	2953	2969	rBV	27344276	37503655	100.00%	18.327%
13	21.904	3211	3216	3227	rBV	7475780	10467850	27.91%	5.115%
14	24.392	3631	3639	3656	rVB2	5288447	10789562	28.77%	5.272%


Sum of corrected areas: 204641275

Data Path : Z:\HPCHEM1\BNA N\DATA\BN021518\
Data File : BN000087.D
Acq On : 15 Feb 2018 09:31
Operator : JU/SJ
Sample : PB105903BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB105903BL

Quant Method : Z:\HPCHEM1\BNA N\METHODS\8270-BN020718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

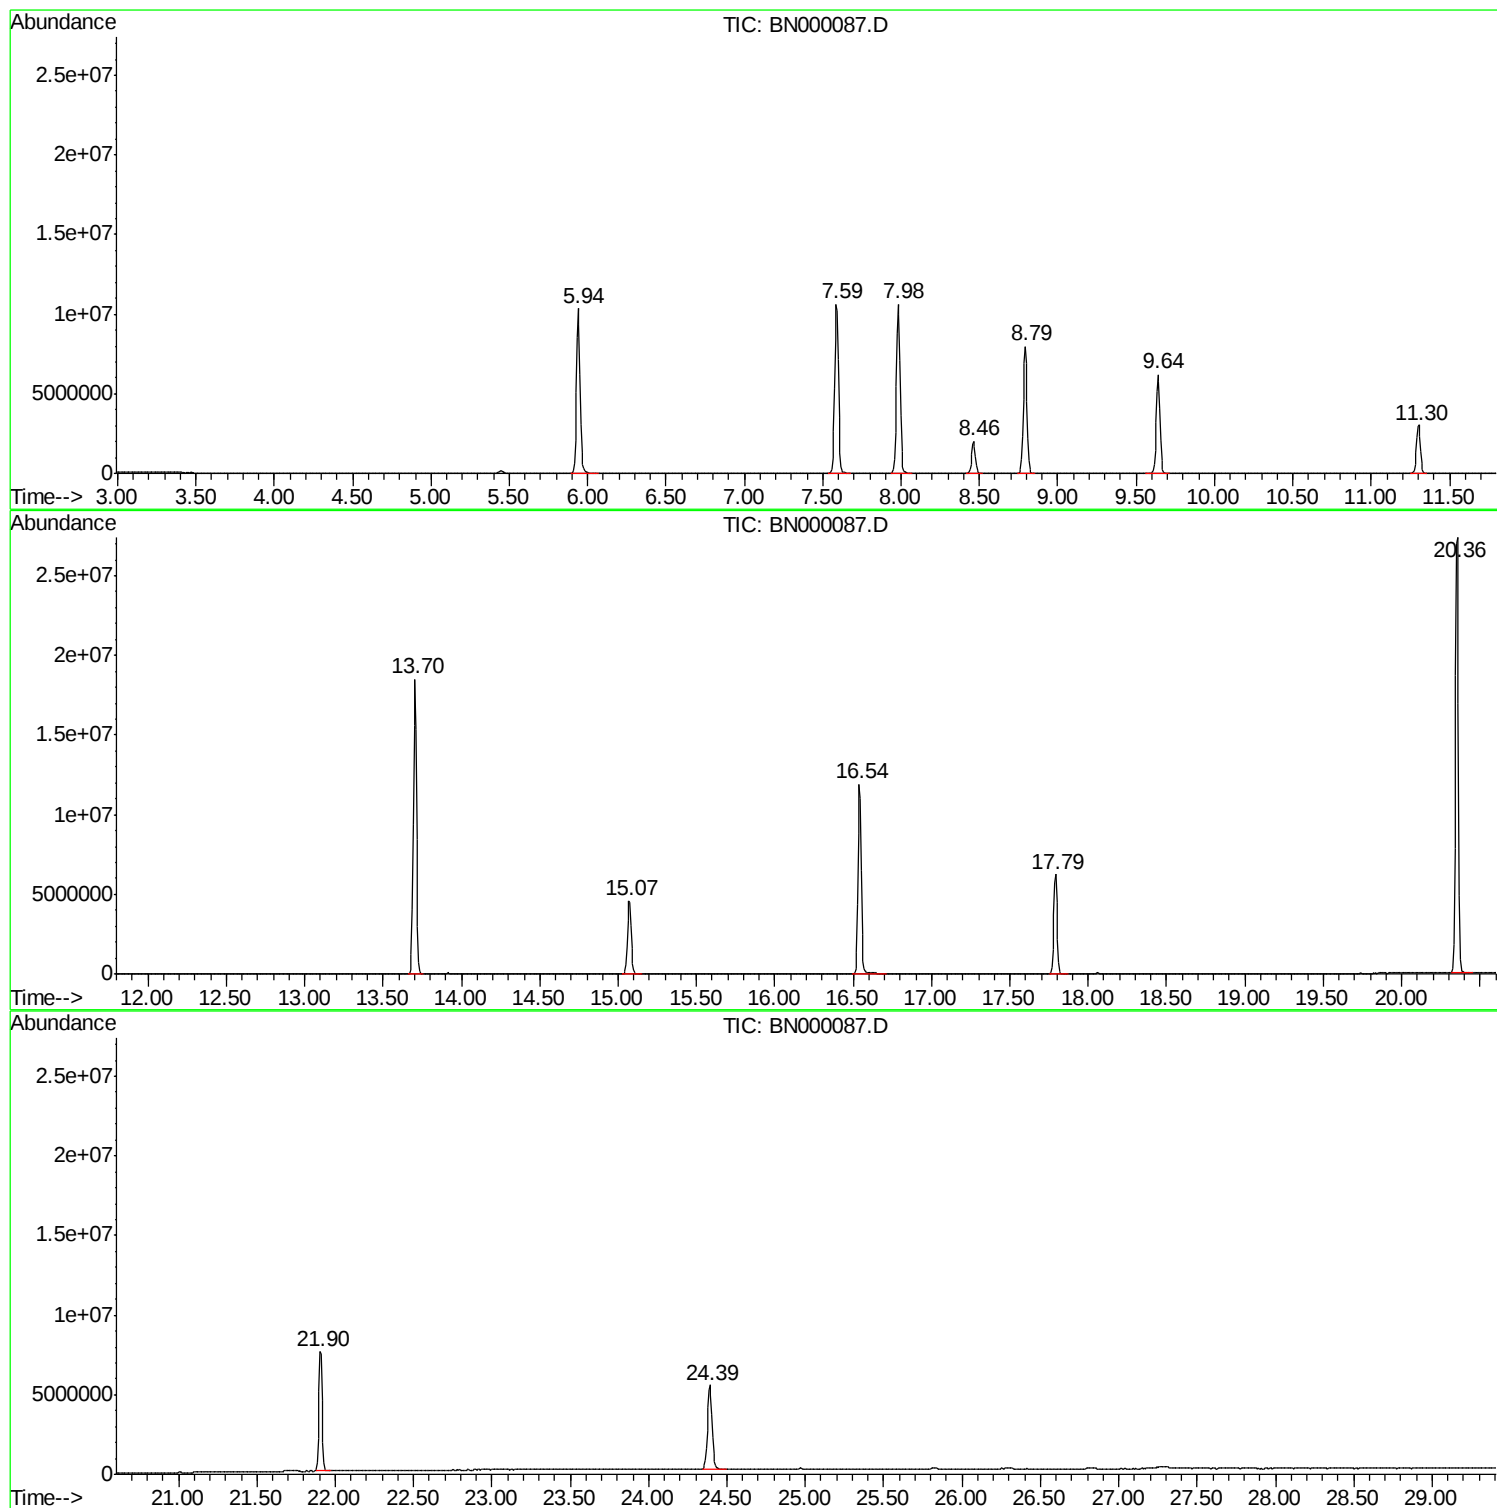

Data Path : Z:\HPCHEM1\BNA N\DATA\BN021518\
Data File : BN000087.D
Acq On : 15 Feb 2018 09:31
Operator : JU/SJ
Sample : PB105903BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB105903BL










Quant Method : Z:\HPCHEM1\BNA N\METHODS\8270-BN020718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.98 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.98	109.54 ng	18113500	1,4-Dichlorobenzene-d4	8.46

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	16
3		Tranvlcypropine-propionyl	189	C12H15NO	1000123-86-3	10
4		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9
5		4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	9

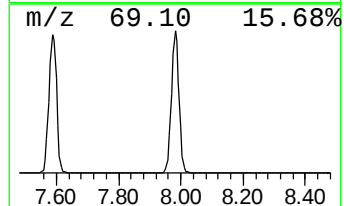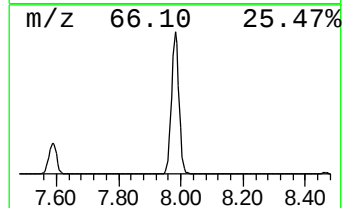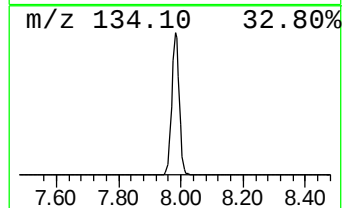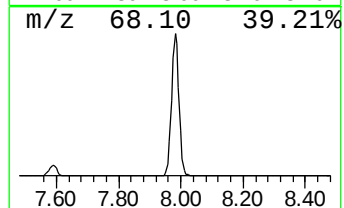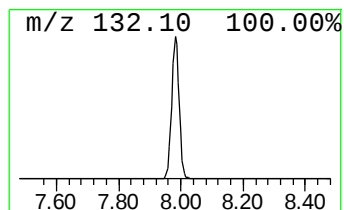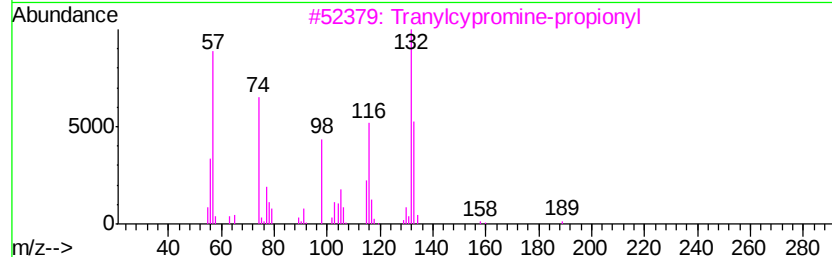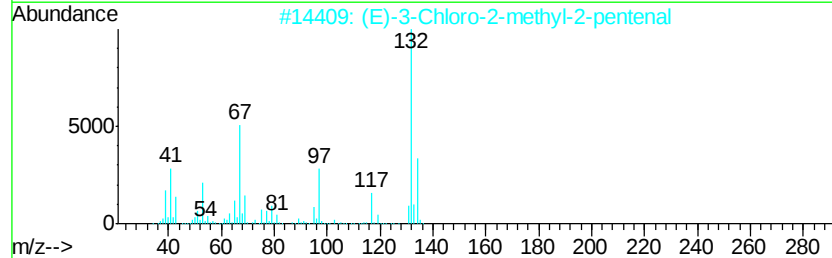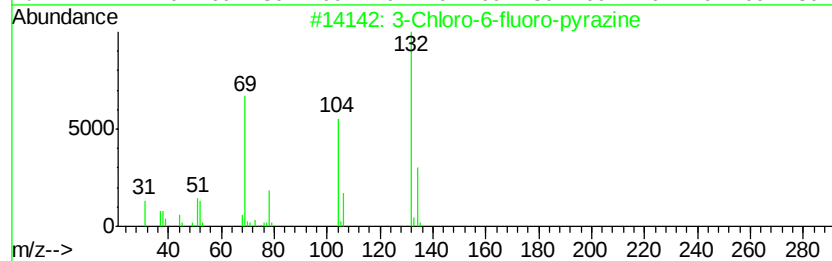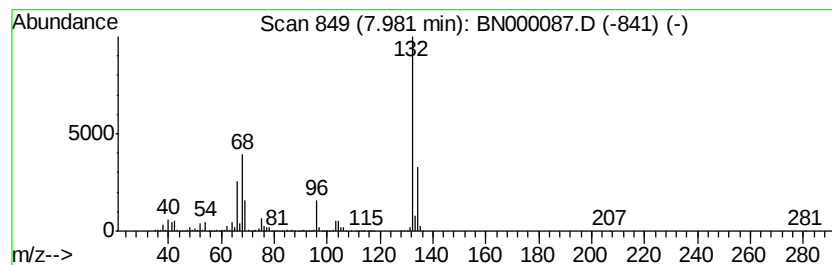

Data Path : Z:\HPCHEM1\BNA_N\DATA\BN021518\
Data File : BN000087.D
Acq On : 15 Feb 2018 09:31
Operator : JU/SJ
Sample : PB105903BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB105903BL

Quant Method : Z:\HPCHEM1\BNA_N\METHODS\8270-BN020718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.98	7.98	109.5	ng	18113500	1	8.46	3307280	20.0