


Data Path : Z:\HPCHEM1\BNA N\Data\BN021518\
 Data File : BN000085.D
 Acq On : 15 Feb 2018 08:23
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_N\METHODS\8270-BN020718.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Feb 07 18:24:45 2018

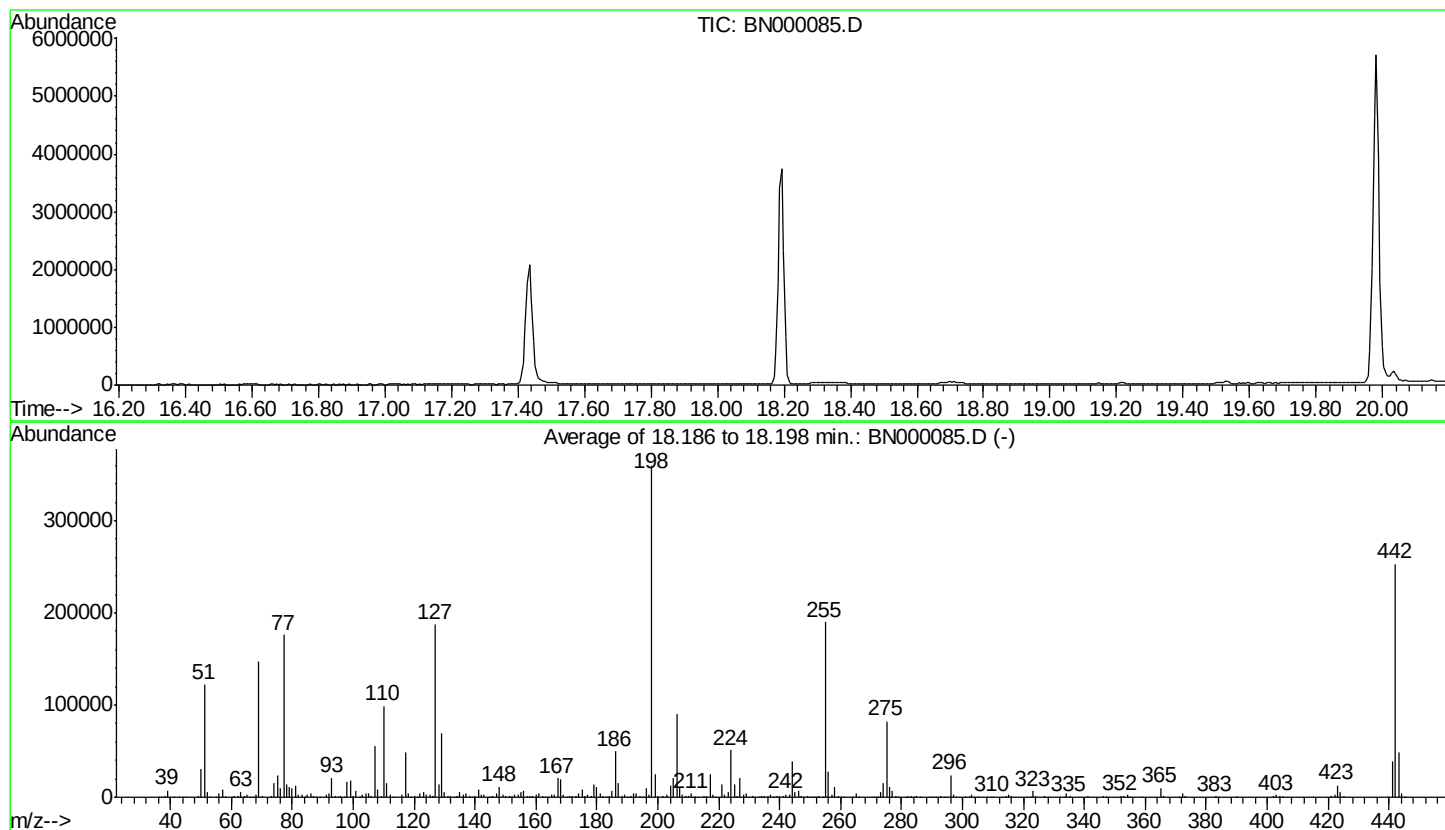

AutoFind: Scans 2584, 2585, 2586; Background Corrected with Scan 2577

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.8	121696	PASS
68	69	0.00	2	1.7	2544	PASS
69	198	0.00	100	40.9	147074	PASS
70	69	0.00	2	0.6	811	PASS
127	198	10	80	52.0	186968	PASS
197	198	0.00	2	0.6	2249	PASS
198	198	100	100	100.0	359722	PASS
199	198	5	9	6.9	24664	PASS
275	198	10	60	22.9	82538	PASS
365	198	1	100	2.8	10059	PASS
441	443	0.01	100	79.6	38274	PASS
442	198	50	100	70.4	253376	PASS
443	442	15	24	19.0	48109	PASS