


Data Path : Z:\HPCHEM1\BNA N\Data\BN021518\
 Data File : BN000099.D
 Acq On : 15 Feb 2018 16:24
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_N\METHODS\8270-BN020718.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Feb 07 18:24:45 2018

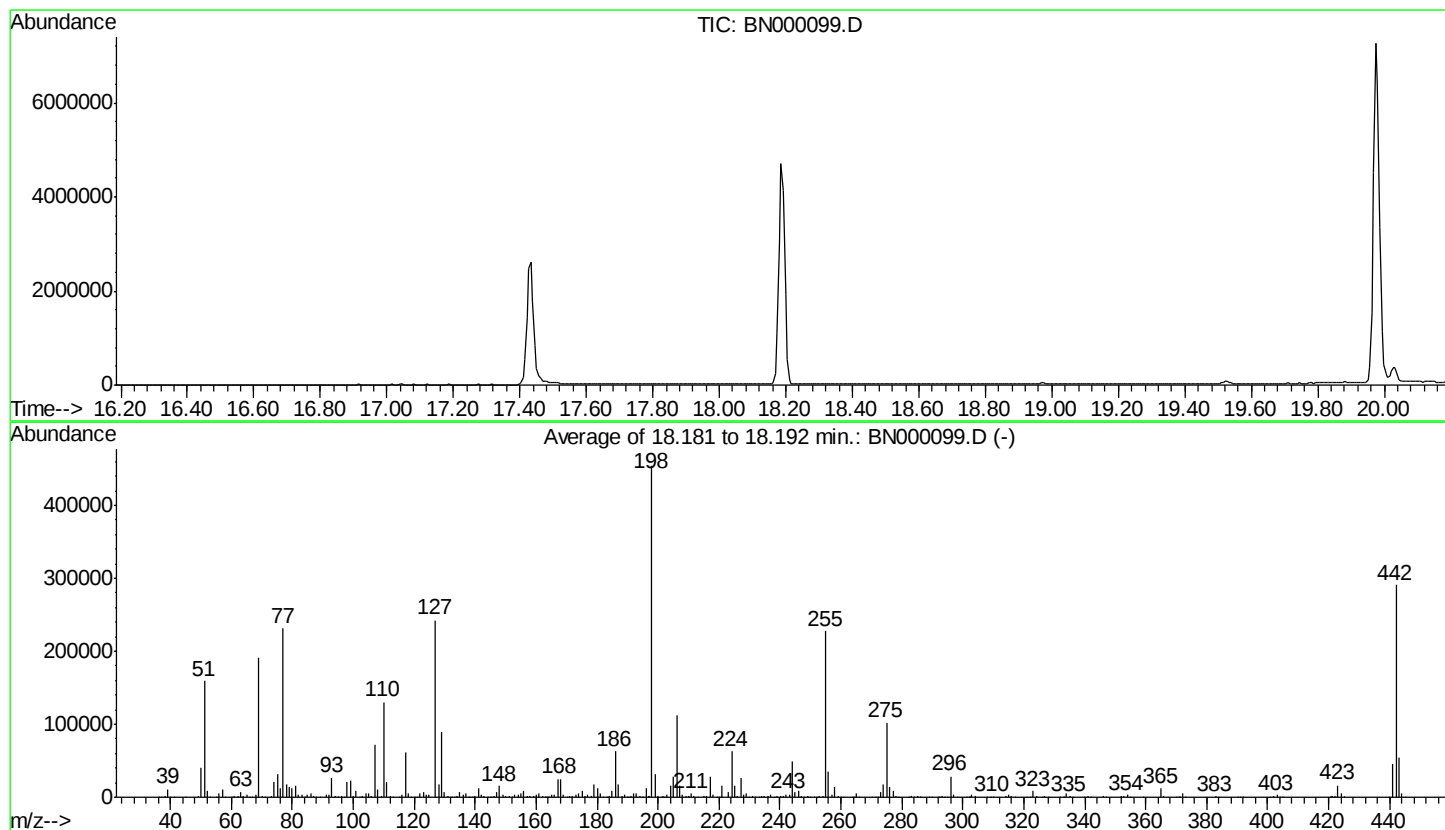

AutoFind: Scans 2583, 2584, 2585; Background Corrected with Scan 2576

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.0	158869	PASS
68	69	0.00	2	1.8	3514	PASS
69	198	0.00	100	42.3	192128	PASS
70	69	0.00	2	0.6	1131	PASS
127	198	10	80	53.3	242176	PASS
197	198	0.00	2	0.3	1571	PASS
198	198	100	100	100.0	454485	PASS
199	198	5	9	6.8	31045	PASS
275	198	10	60	22.6	102554	PASS
365	198	1	100	2.6	11941	PASS
441	443	0.01	100	83.7	46154	PASS
442	198	50	100	64.0	290688	PASS
443	442	15	24	19.0	55136	PASS