
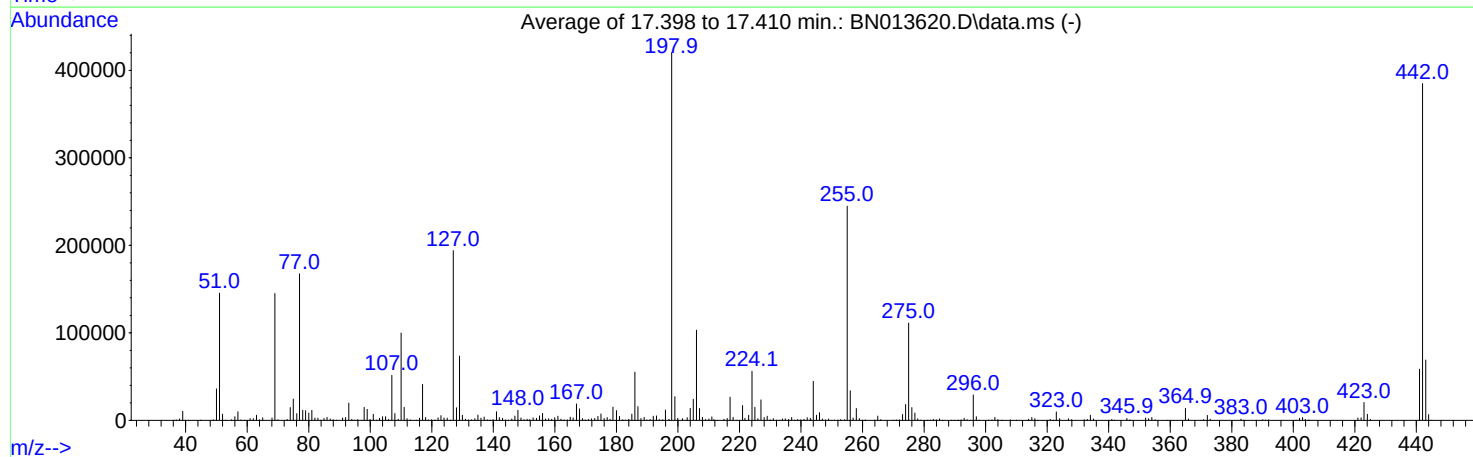


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021521\
 Data File : BN013620.D
 Acq On : 15 Feb 2021 12:44
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN020821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 08 15:13:18 2021

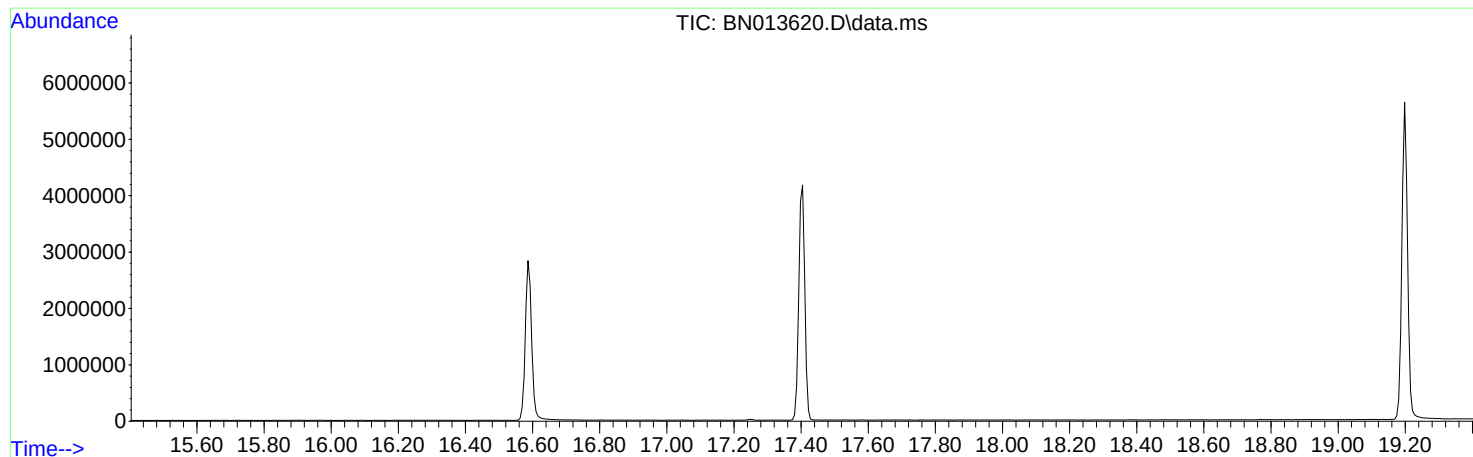




AutoFind: Scans 2433, 2434, 2435; Background Corrected with Scan 2426

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.6	145336	PASS
68	69	0.00	2	1.9	2687	PASS
69	198	0.00	100	34.5	144960	PASS
70	69	0.00	2	0.5	785	PASS
127	198	10	80	46.1	193976	PASS
197	198	0.00	2	0.3	1341	PASS
198	198	100	100	100.0	420416	PASS
199	198	5	9	6.4	27069	PASS
275	198	10	60	26.4	111152	PASS
365	198	1	100	3.3	13735	PASS
441	198	0.01	100	13.9	58576	PASS
442	442	50	100	100.0	384917	PASS
443	442	15	24	17.9	68947	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021521\
Data File : BN013620.D
Acq On : 15 Feb 2021 12:44
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Feb 16 06:02:54 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 16 05:39:20 2021
Response via : Initial Calibration

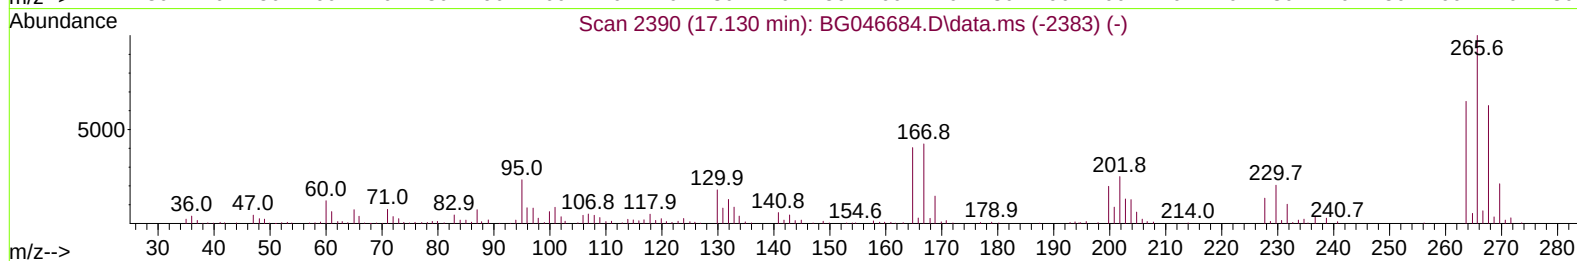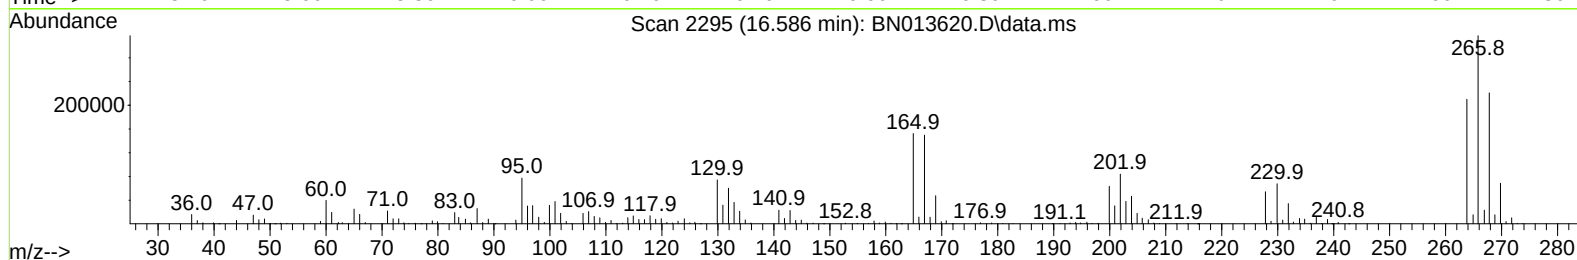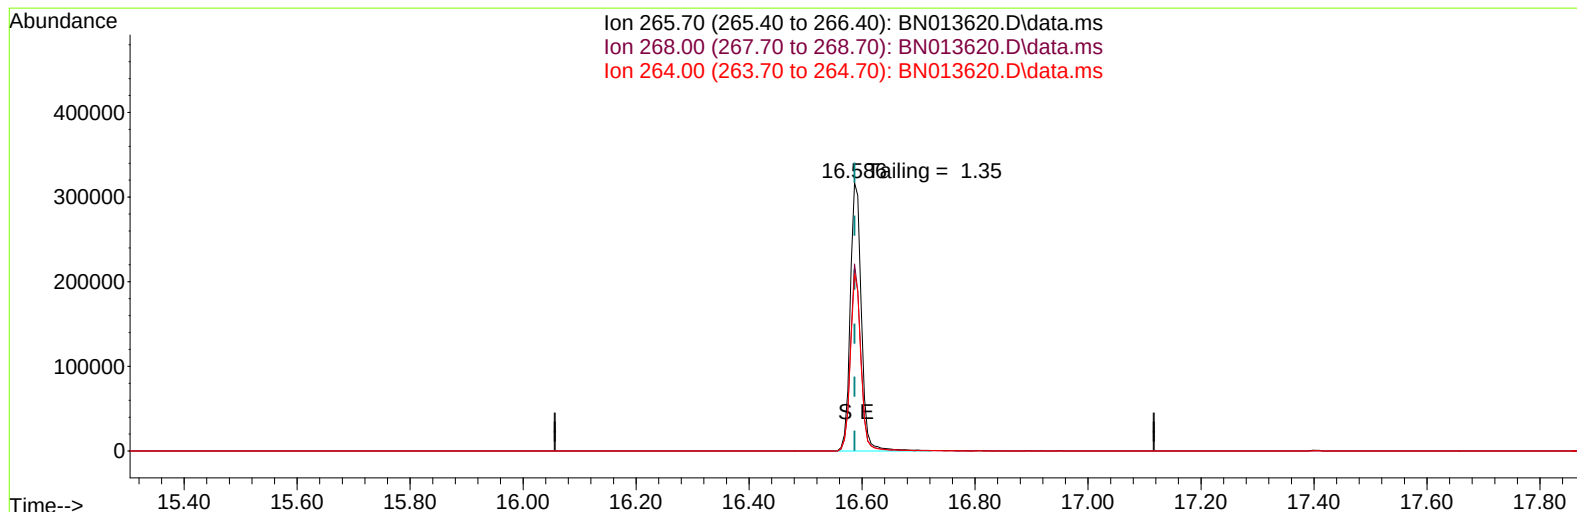

TIC: BN013620.D\data.ms

(70) Pentachlorophenol (C)

16.586min (-0.000) 17995.46 ng




response 435958

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	69.69
264.00	61.60	66.26
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021521\
 Data File : BN013620.D
 Acq On : 15 Feb 2021 12:44
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Feb 16 06:02:54 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 16 05:39:20 2021
 Response via : Initial Calibration

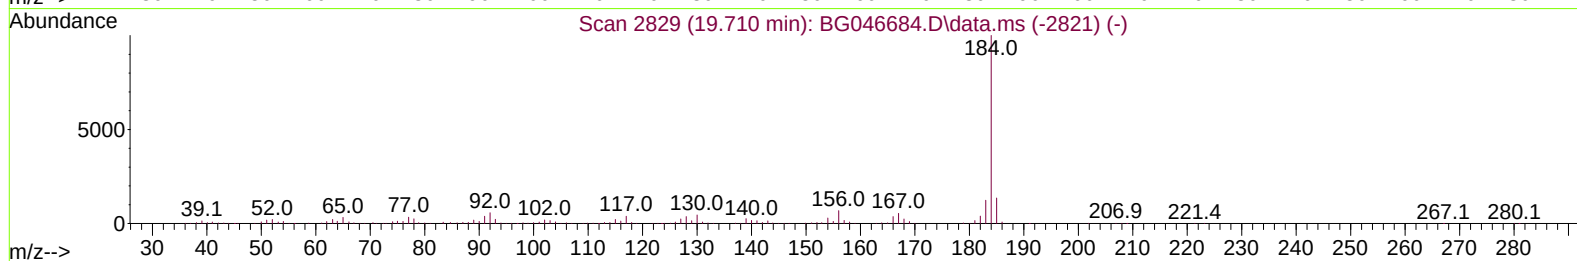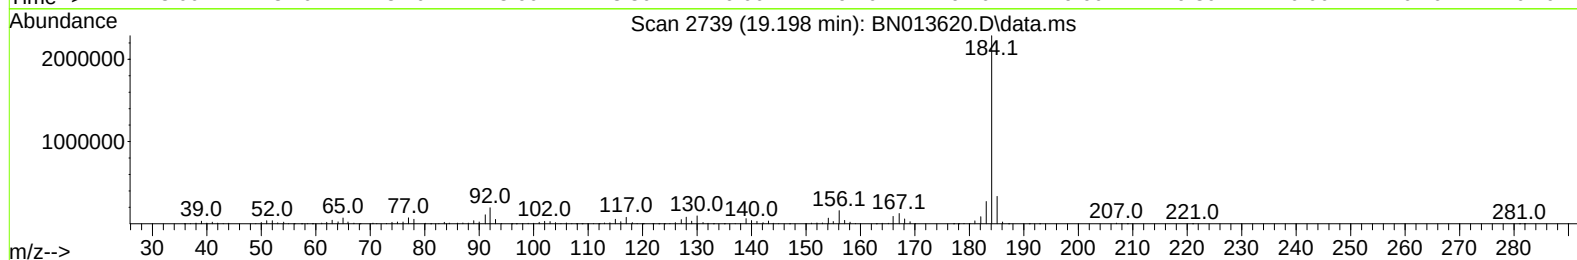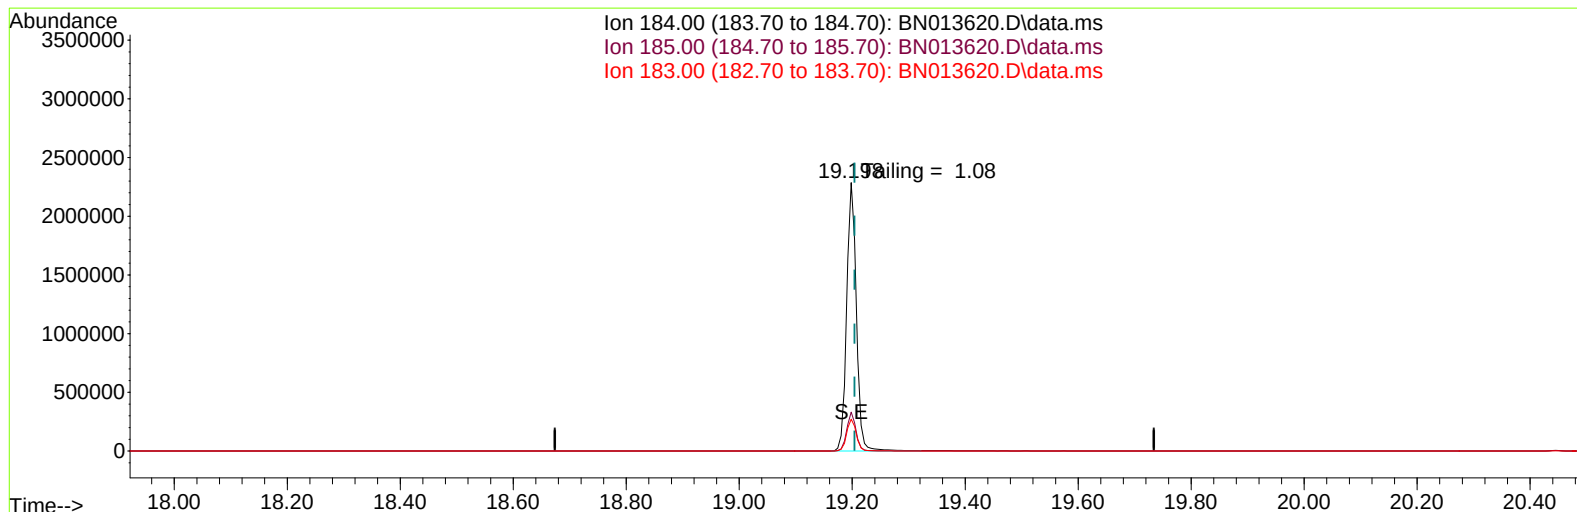

TIC: BN013620.D\data.ms

(77) Benzidine

19.198min (-0.006) 0.00 ng

response 2723236

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.53
183.00	13.20	11.86
0.00	0.00	0.00

DDT Breakdown

Instrument :
BNA_N
ClientSampleId :
DFTPP

Date	Instrument Name	DFTPP Data File
02/15/2021	BNA_N	<u>BN013620.D</u>
Compound Name	Response	Retention Time
DDT	1432653	20.44
DDD	8643	20
DDE	2344	19.49
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10987	1443640	0.76