

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021522\
 Data File : BN018614.D
 Acq On : 15 Feb 2022 14:37
 Operator : CG/JU
 Sample : SSTD16021
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTD160228

Quant Time: Feb 15 17:44:12 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN021522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 15 17:38:23 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.898	152	170679	20.000	ng/u1	0.00
20) Naphthalene-d8	10.713	136	636765	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.543	164	363170	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.291	188	645004	20.000	ng/u1	# 0.02
79) Chrysene-d12	21.458	240	599579	20.000	ng/u1	# 0.00
88) Perylene-d12	23.868	264	632243	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.280	96	253094	65.345	ng/uL	0.02
4) Pyridine-d5	3.685	84	1946527	148.296	ng/u1	0.00
7) Phenol-d5	7.064	99	2068034	149.512	ng/u1	0.02
9) Bis-(2-Chloroethyl)eth...	7.222	67	1192479	141.960	ng/u1	0.00
11) 2-Chlorophenol-d4	7.447	132	1698490	154.621	ng/u1	0.02
15) 4-Methylphenol-d8	8.619	113	1559520	146.234	ng/u1	0.02
21) Nitrobenzene-d5	9.069	128	790294	165.187	ng/u1	0.02
24) 2-Nitrophenol-d4	9.790	143	875161	169.466	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.330	165	1492039	150.210	ng/u1	0.00
31) 4-Chloroaniline-d4	10.849	131	1884941	145.038	ng/u1	0.02
46) Dimethylphthalate-d6	13.957	166	3868253	148.866	ng/u1	0.02
49) Acenaphthylene-d8	14.227	160	4590717	129.013	ng/u1	0.00
54) 4-Nitrophenol-d4	14.745	143	729819	166.724	ng/u1	0.02
60) Fluorene-d10	15.534	176	3169257	144.239	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.646	200	657603	168.942	ng/u1	0.00
73) Anthracene-d10	17.381	188	4361375	138.538	ng/u1	0.00
81) Pyrene-d10	19.679	212	5093775	173.851	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.711	264	5144890	157.073	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.303	88	310544	62.436	ng/uL#	87
5) Pyridine	3.708	79	1981732	153.827	ng/u1	98
6) Benzaldehyde	7.042	77	1324248	170.924	ng/u1	86
8) Phenol	7.087	94	1964715	140.189	ng/u1#	88
10) Bis(2-Chloroethyl)ether	7.335	93	1692802	146.560	ng/u1	90
12) 2-Chlorophenol	7.470	128	1751626	154.676	ng/u1	93
13) 2-Methylphenol	8.348	108	1607108	154.561	ng/u1	97
14) 2,2'-oxybis(1-Chloropr...	8.438	45	2152342	138.969	ng/u1	99
16) Acetophenone	8.731	105	2242897	140.017	ng/u1	99
17) N-Nitroso-di-n-propyla...	8.731	70	1080738	132.596	ng/u1	91
18) 4-Methylphenol	8.686	108	1598827	142.154	ng/u1	96
19) Hexachloroethane	9.001	117	759286	159.984	ng/u1	90
22) Nitrobenzene	9.114	77	1897549	157.049	ng/u1	95
23) Isophorone	9.655	82	3345526	161.661	ng/u1#	93
25) 2-Nitrophenol	9.835	139	921376	161.651	ng/u1#	83
26) 2,4-Dimethylphenol	9.880	107	1719579	142.551	ng/u1	95
27) Bis(2-Chloroethoxy)met...	10.128	93	2084006	149.802	ng/u1	98
29) 2,4-Dichlorophenol	10.376	162	1459651	141.232	ng/u1#	91
30) Naphthalene	10.758	128	4761516	135.701	ng/u1	99
32) 4-Chloroaniline	10.871	127	1898633	141.669	ng/u1	98
33) Hexachlorobutadiene	11.074	225	1085525	149.941	ng/u1	99
34) Caprolactam	11.659	113	254078	94.042	ng/u1	88
35) 4-Chloro-3-methylphenol	11.997	107	1530094	149.238	ng/u1	96
36) 2-Methylnaphthalene	12.380	142	3193504	143.002	ng/u1	97

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021522\
 Data File : BN018614.D
 Acq On : 15 Feb 2022 14:37
 Operator : CG/JU
 Sample : SSTD16021
 Misc :
 ALS Vial : 7 Sample Multiplier: 1


Instrument :
 BNA_N
 ClientSampleId :
 SSTD160228


Quant Time: Feb 15 17:44:12 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN021522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 15 17:38:23 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.606	142	3070996	130.169	ng/ul	98
39) 1,2,4,5-Tetrachloroben...	12.741	216	1613659	123.445	ng/ul#	94
40) Hexachlorocyclopentadiene	12.741	237	1269169	158.043	ng/ul	98
42) 2,4,5-Trichlorophenol	13.056	196	1218415	157.291	ng/ul	96
43) 1,1'-Biphenyl	13.371	154	3867946	124.877	ng/ul	99
44) 2-Chloronaphthalene	13.416	162	2966910	123.926	ng/ul#	90
45) 2-Nitroaniline	13.619	65	1023041	186.208	ng/ul	95
47) Dimethylphthalate	14.002	163	3837975	149.422	ng/ul	100
48) 2,6-Dinitrotoluene	14.115	165	789800	168.419	ng/ul	93
50) Acenaphthylene	14.272	152	4955733	143.093	ng/ul	100
51) 3-Nitroaniline	14.430	138	628330	134.752	ng/ul	98
52) Acenaphthene	14.610	153	3229545	144.199	ng/ul	99
53) 2,4-Dinitrophenol	14.655	184	527286	176.192	ng/ul#	71
55) 4-Nitrophenol	14.745	109	520142	130.303	ng/ul	88
56) Dibenzofuran	14.948	168	4533008	139.930	ng/ul	97
57) 2,4-Dinitrotoluene	14.903	165	1220913	176.384	ng/ul	92
58) 2,3,4,6-Tetrachlorophenol	15.173	232	985441	170.761	ng/ul#	89
59) Diethylphthalate	15.354	149	3511687	134.446	ng/ul	96
61) Fluorene	15.601	166	2950977	111.255	ng/ul	98
62) 4-Chlorophenyl-phenyle...	15.579	204	1685388	123.212	ng/ul#	88
63) 4-Nitroaniline	15.601	138	458987	121.638	ng/ul	93
66) 4,6-Dinitro-2-methylph...	15.669	198	758706	179.211	ng/ul#	92
67) N-Nitrosodiphenylamine	15.782	169	2656919	117.634	ng/ul	97
68) 4-Bromophenyl-phenylether	16.480	248	1147834	166.864	ng/ul#	86
69) Hexachlorobenzene	16.593	284	1156725	125.645	ng/ul#	79
70) Atrazine	16.750	200	1293009	164.621	ng/ul	98
71) Pentachlorophenol	16.930	266	839756	159.889	ng/ul	97
72) Phenanthrene	17.336	178	5308145	136.091	ng/ul	99
74) Anthracene	17.426	178	5323567	138.160	ng/ul	99
75) 1,2,3,4-Tetrachloroben...	13.349	216	1859484	140.608	ng/uL	99
76) Pentachlorobenzene	14.858	250	1449591	125.211	ng/uL	96
77) Carbazole	17.674	167	4318726	128.240	ng/ul#	97
78) Di-n-butylphthalate	18.237	149	5146604	143.219	ng/ul#	98
80) Fluoranthene	19.341	202	6528422	186.936	ng/ul#	93
82) Pyrene	19.701	202	5798451	150.977	ng/ul	99
83) Butylbenzylphthalate	20.580	149	2086885	219.987	ng/ul#	71
84) 3,3'-Dichlorobenzidine	21.368	252	1458794	137.643	ng/ul#	97
85) Benzo(a)anthracene	21.458	228	6031234	163.836	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.368	149	3736520	170.812	ng/ul#	95
87) Chrysene	21.503	228	5363406	172.332	ng/ul	95
89) Di-n-octyl phthalate	22.291	149	6731784	155.717	ng/ul	100
90) Benzo(b)fluoranthene	23.147	252	8213471	187.413	ng/ul#	97
91) Benzo(k)fluoranthene	23.192	252	4330502	111.416	ng/ul#	98
93) Benzo(a)pyrene	23.778	252	6379298	153.960	ng/ul#	94
94) Indeno(1,2,3-cd)pyrene	26.391	276	7548636	160.377	ng/ul	93
95) Dibenzo(a,h)anthracene	26.391	278	6195818	155.391	ng/ul	98
96) Benzo(g,h,i)perylene	27.157	276	6624372	165.050	ng/ul	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Feb 15 17:44:12 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN021522.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 15 17:38:23 2022
Response via : Initial Calibration




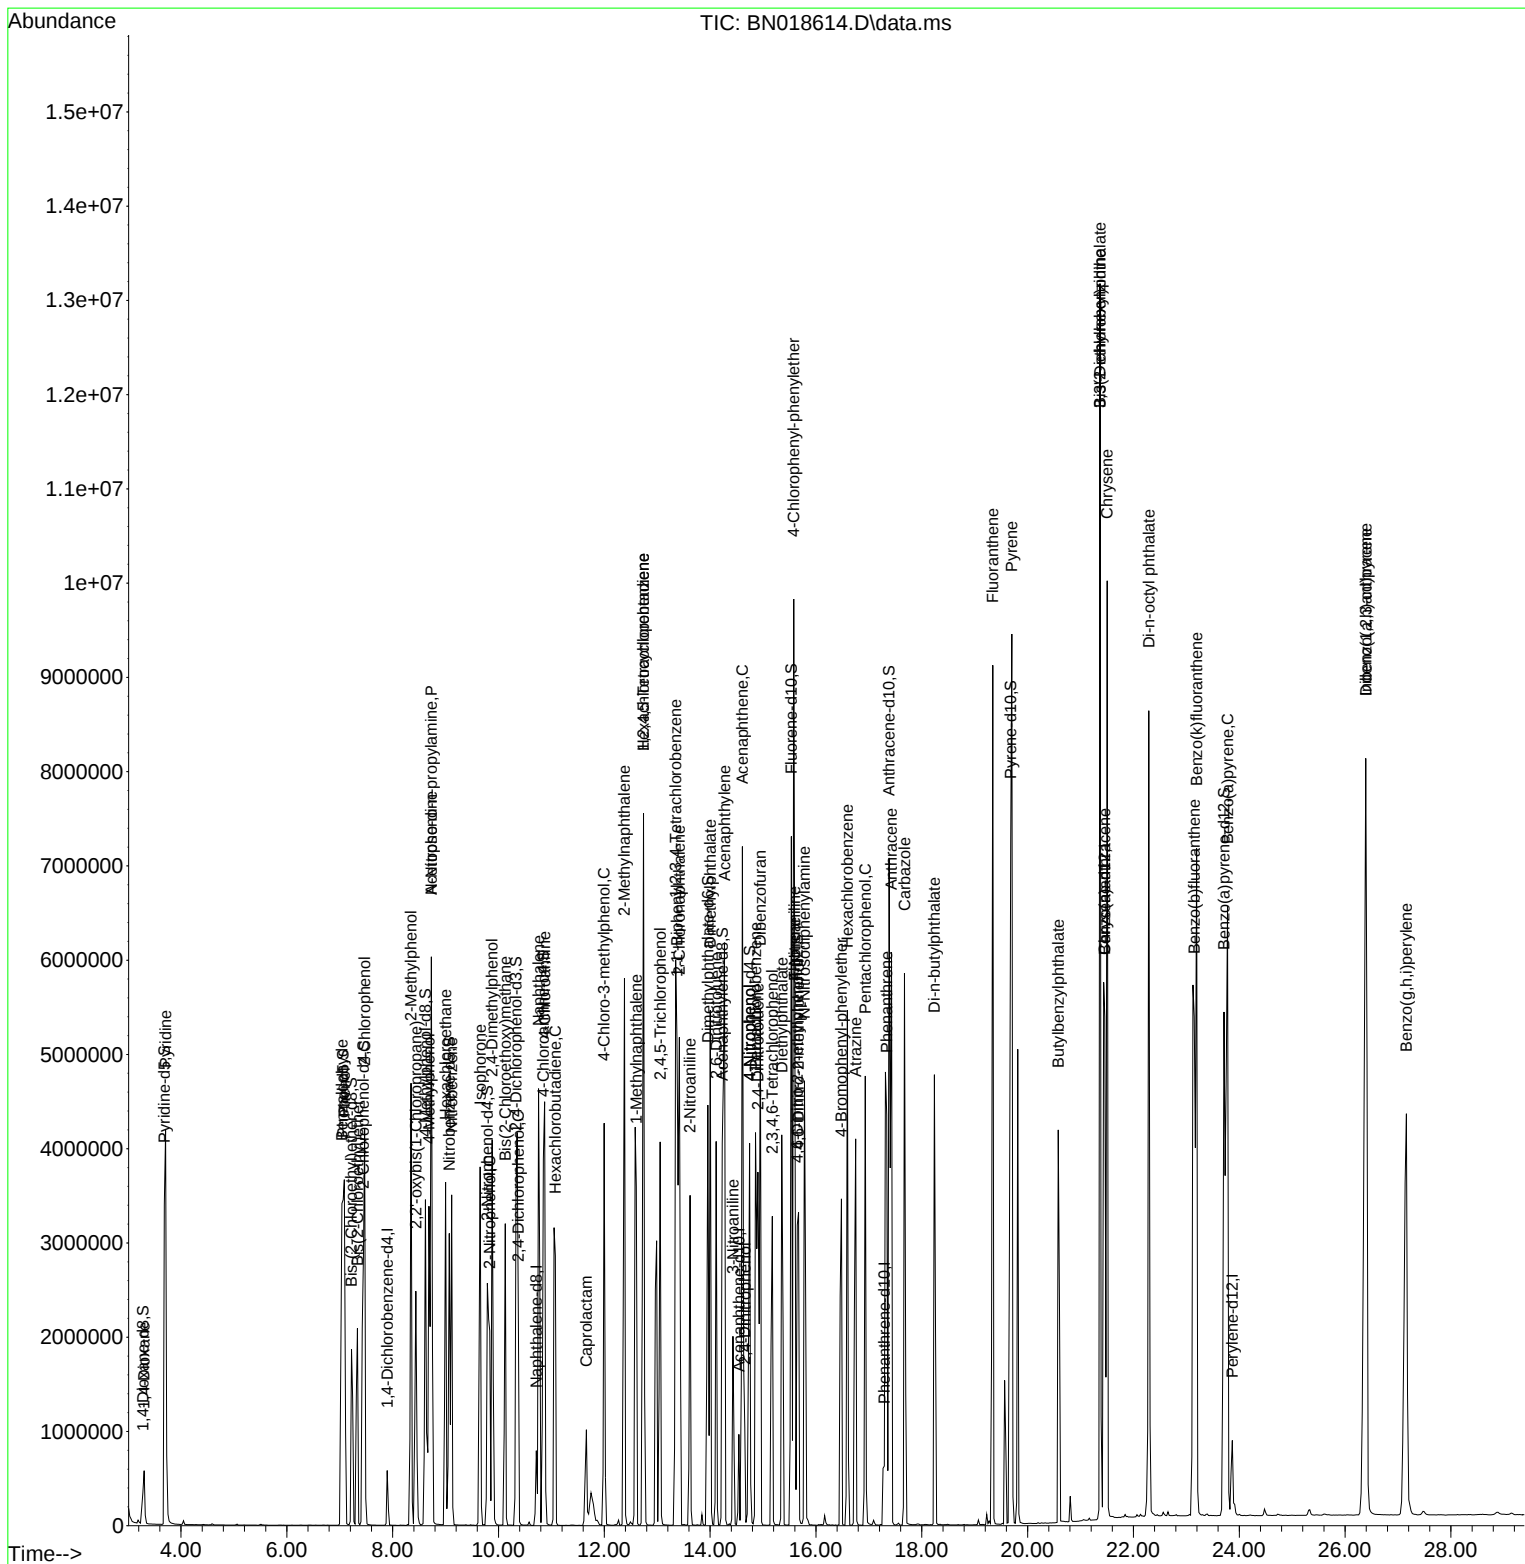


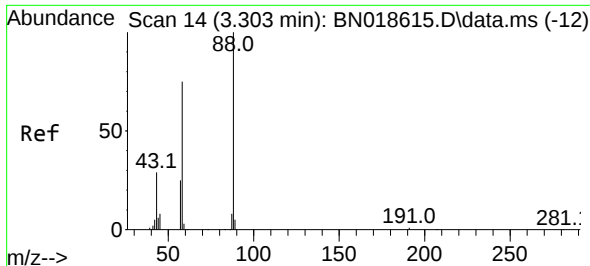

#2
 1,4-Dioxane
 Concen: 62.436 ng/uL
 RT: 3.303 min Scan# 14
 Delta R.T. -0.000 min
 Lab File: BN018614.D
 Acq: 15 Feb 2022 14:37




Instrument :
 BNA_N
 ClientSampleId :
 SSTD160228


Tgt Ion: 88 Resp: 310544
 Ion Ratio Lower Upper
 88 100
 43 33.7 21.9 32.9#
 58 80.9 56.3 84.5

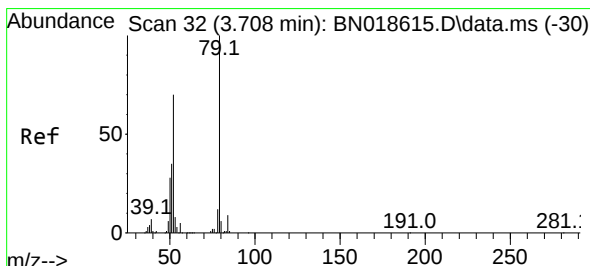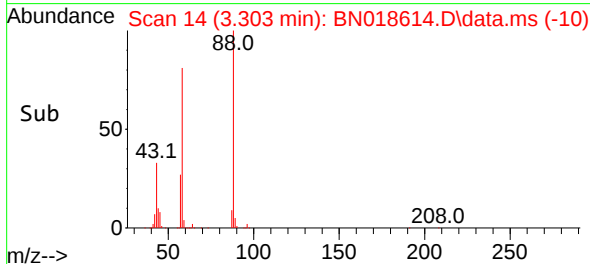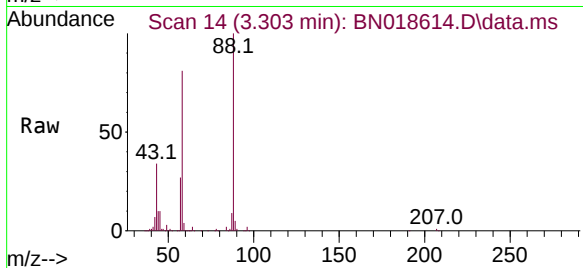

#5
 Pyridine
 Concen: 153.827 ng/uL
 RT: 3.708 min Scan# 32
 Delta R.T. -0.000 min
 Lab File: BN018614.D
 Acq: 15 Feb 2022 14:37

Tgt Ion: 79 Resp: 1981732
 Ion Ratio Lower Upper
 79 100
 52 77.7 62.9 94.3
 51 37.8 27.8 41.8


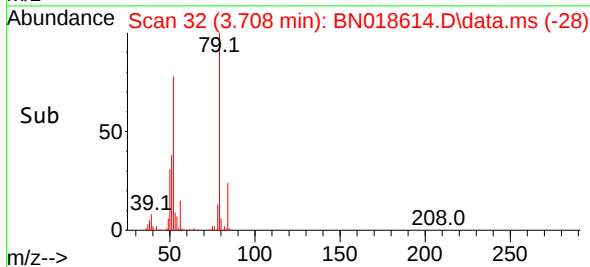

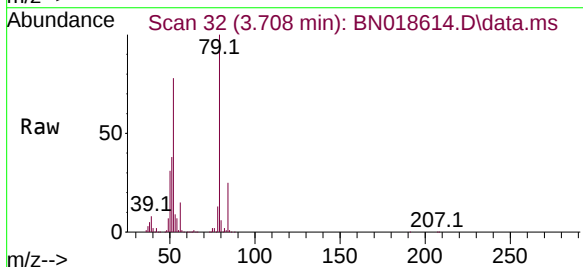




#6
Benzaldehyde
Concen: 170.924 ng/ul
RT: 7.042 min Scan# 180
Delta R.T. 0.023 min
Lab File: BN018614.D
Acq: 15 Feb 2022 14:37




Instrument :
BNA_N
ClientSampleId :
SSTD160228


Tgt Ion: 77 Resp: 1324248
Ion Ratio Lower Upper
77 100
105 104.8 73.5 110.3
106 100.8 69.9 104.9

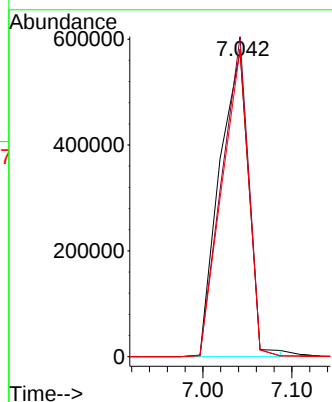

#8
Phenol
Concen: 140.189 ng/ul
RT: 7.087 min Scan# 182
Delta R.T. 0.023 min
Lab File: BN018614.D
Acq: 15 Feb 2022 14:37

Tgt Ion: 94 Resp: 1964715
Ion Ratio Lower Upper
94 100
65 32.6 21.8 32.6
66 45.9 30.2 45.4#

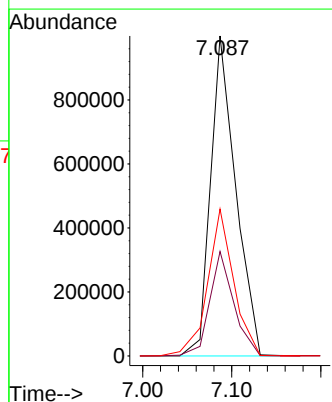



#10

Bis(2-Chloroethyl)ether

Concen: 146.560 ng/ul

RT: 7.335 min Scan# 193

Delta R.T. 0.023 min

Lab File: BN018614.D

Acq: 15 Feb 2022 14:37

Instrument :





BNA_N

ClientSampleId :

SSTD160228

Tgt Ion: 93 Resp: 1692802

Ion	Ratio	Lower	Upper
93	100		
63	67.0	63.4	95.0
95	32.6	25.9	38.9



#12

2-Chlorophenol

Concen: 154.676 ng/ul

RT: 7.470 min Scan# 199




Delta R.T. 0.023 min


Lab File: BN018614.D

Acq: 15 Feb 2022 14:37

Tgt Ion: 128 Resp: 1751626

Ion	Ratio	Lower	Upper
128	100		
64	48.5	44.2	66.2
130	32.5	25.0	37.6



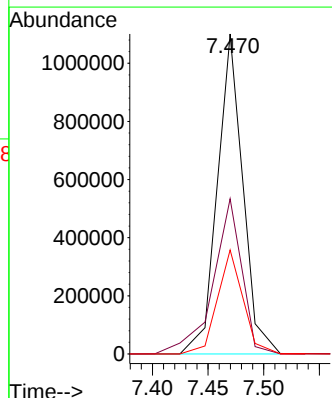





#13
2-Methylphenol
Concen: 154.561 ng/ul
RT: 8.348 min Scan# 21
Delta R.T. 0.023 min
Lab File: BN018614.D
Acq: 15 Feb 2022 14:37




Instrument :
BNA_N
ClientSampleId :
SSTD160228


Tgt Ion:108 Resp: 1607108
Ion Ratio Lower Upper
108 100
107 89.8 69.5 104.3



#14
2,2'-oxybis(1-Chloropropane)
Concen: 138.969 ng/ul
RT: 8.438 min Scan# 242
Delta R.T. 0.022 min
Lab File: BN018614.D
Acq: 15 Feb 2022 14:37

Tgt Ion: 45 Resp: 2152342
Ion Ratio Lower Upper
45 100
77 14.9 11.9 17.9
79 11.4 8.6 12.8









#16
Acetophenone
Concen: 140.017 ng/ul
RT: 8.731 min Scan# 21
Delta R.T. 0.023 min
Lab File: BN018614.D
Acq: 15 Feb 2022 14:37




Instrument :
BNA_N
ClientSampleId :
SSTD160228


Tgt Ion:105 Resp: 2242897
Ion Ratio Lower Upper
105 100
77 81.3 64.8 97.2
51 29.8 22.8 34.2



#17
N-Nitroso-di-n-propylamine
Concen: 132.596 ng/ul
RT: 8.731 min Scan# 255
Delta R.T. 0.023 min
Lab File: BN018614.D
Acq: 15 Feb 2022 14:37

Tgt Ion: 70 Resp: 1080738
Ion Ratio Lower Upper
70 100
42 61.6 42.4 63.6
101 9.5 6.6 10.0
130 18.0 13.6 20.4









#18
4-Methylphenol
Concen: 142.154 ng/ul
RT: 8.686 min Scan# 21
Delta R.T. 0.022 min
Lab File: BN018614.D
Acq: 15 Feb 2022 14:37




Instrument :
BNA_N
ClientSampleId :
SSTD160228


Tgt Ion:108 Resp: 1598827
Ion Ratio Lower Upper
108 100
107 115.6 89.4 134.0



#19
Hexachloroethane
Concen: 159.984 ng/ul
RT: 9.001 min Scan# 267
Delta R.T. 0.023 min
Lab File: BN018614.D
Acq: 15 Feb 2022 14:37

Tgt Ion:117 Resp: 759286
Ion Ratio Lower Upper
117 100
201 119.5 85.9 128.9
199 73.2 54.5 81.7









#22
Nitrobenzene
Concen: 157.049 ng/ul
RT: 9.114 min Scan# 21
Delta R.T. 0.022 min
Lab File: BN018614.D
Acq: 15 Feb 2022 14:37




Instrument :
BNA_N
ClientSampleId :
SSTD160228


Tgt Ion: 77 Resp: 1897549
Ion Ratio Lower Upper
77 100
123 43.9 32.0 48.0
65 14.1 10.7 16.1



#23
Isophorone
Concen: 161.661 ng/ul
RT: 9.655 min Scan# 296
Delta R.T. 0.022 min
Lab File: BN018614.D
Acq: 15 Feb 2022 14:37

Tgt Ion: 82 Resp: 3345526
Ion Ratio Lower Upper
82 100
95 8.1 5.7 8.5
138 18.7 11.9 17.9#









#25
2-Nitrophenol
Concen: 161.651 ng/ul
RT: 9.835 min Scan# 303
Delta R.T. 0.023 min
Lab File: BN018614.D
Acq: 15 Feb 2022 14:37




Instrument :
BNA_N
ClientSampleId :
SSTD160228


Tgt Ion:139 Resp: 921376
Ion Ratio Lower Upper
139 100
65 41.4 47.7 71.5#
109 31.7 27.0 40.4

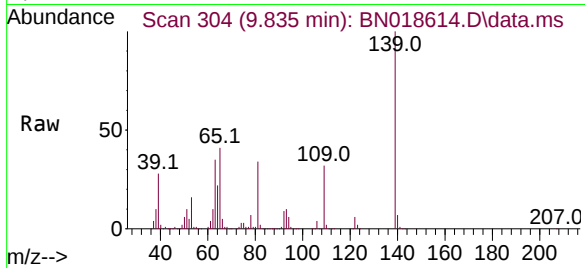

#26
2,4-Dimethylphenol
Concen: 142.551 ng/ul
RT: 9.880 min Scan# 306
Delta R.T. -0.000 min
Lab File: BN018614.D
Acq: 15 Feb 2022 14:37

Tgt Ion:107 Resp: 1719579
Ion Ratio Lower Upper
107 100
121 46.7 38.9 58.3
122 79.7 68.6 103.0

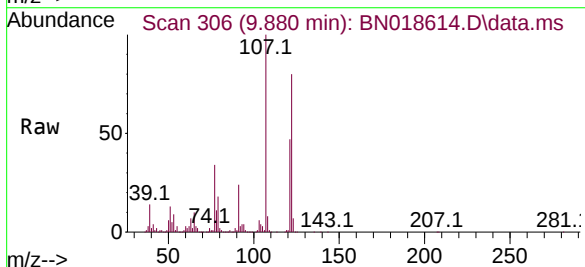



#27

Bis(2-Chloroethoxy)methane

Concen: 149.802 ng/ul

RT: 10.128 min Scan# 316

Delta R.T. 0.022 min

Lab File: BN018614.D

Acq: 15 Feb 2022 14:37

Instrument :

BNA_N

ClientSampleId :

SSTD160228





Tgt Ion: 93 Resp: 2084006

Ion Ratio Lower Upper

93 100

95 32.8 25.7 38.5

123 11.8 8.3 12.5



#29

2,4-Dichlorophenol

Concen: 141.232 ng/ul

RT: 10.376 min Scan# 328

Delta R.T. 0.023 min

Lab File: BN018614.D

Acq: 15 Feb 2022 14:37




Tgt Ion:162 Resp: 1459651


Ion Ratio Lower Upper

162 100

164 66.8 51.8 77.6

98 26.2 31.0 46.6#



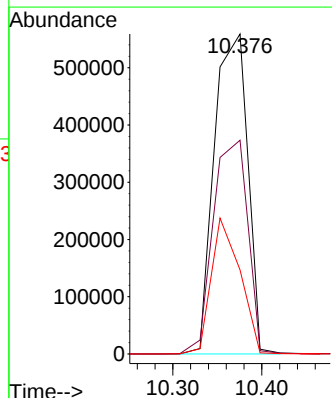





#30
Naphthalene
Concen: 135.701 ng/ul
RT: 10.758 min Scan# 34
Delta R.T. -0.000 min
Lab File: BN018614.D
Acq: 15 Feb 2022 14:37




Instrument :
BNA_N
ClientSampleId :
SSTD160228


Tgt Ion:128 Resp: 4761516
Ion Ratio Lower Upper
128 100
129 11.3 8.6 12.8
127 13.5 10.6 16.0



#32
4-Chloroaniline
Concen: 141.669 ng/ul
RT: 10.871 min Scan# 350
Delta R.T. 0.023 min
Lab File: BN018614.D
Acq: 15 Feb 2022 14:37

Tgt Ion:127 Resp: 1898633
Ion Ratio Lower Upper
127 100
129 32.4 25.0 37.6









#33
Hexachlorobutadiene
Concen: 149.941 ng/ul
RT: 11.074 min Scan# 311
Delta R.T. 0.022 min
Lab File: BN018614.D
Acq: 15 Feb 2022 14:37




Instrument :
BNA_N
ClientSampleId :
SSTD160228


Tgt Ion:225 Resp: 1085525
Ion Ratio Lower Upper
225 100
223 62.1 49.7 74.5
227 63.7 49.5 74.3

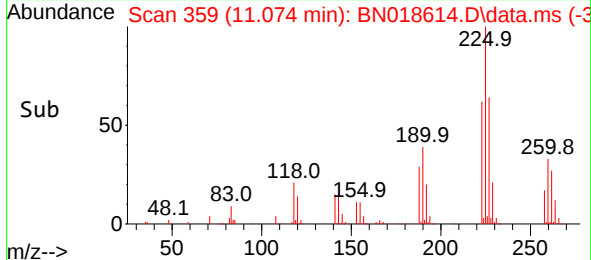

#34
Caprolactam
Concen: 94.042 ng/ul
RT: 11.659 min Scan# 385
Delta R.T. 0.068 min
Lab File: BN018614.D
Acq: 15 Feb 2022 14:37

Tgt Ion:113 Resp: 254078
Ion Ratio Lower Upper
113 100
55 162.7 147.4 221.2
56 126.1 107.6 161.4









#35
4-Chloro-3-methylphenol
Concen: 149.238 ng/ul
RT: 11.997 min Scan# 40
Delta R.T. 0.023 min
Lab File: BN018614.D
Acq: 15 Feb 2022 14:37




Instrument :
BNA_N
ClientSampleId :
SSTD160228


Tgt Ion:107 Resp: 1530094
Ion Ratio Lower Upper
107 100
144 24.1 19.4 29.0
142 73.8 62.3 93.5

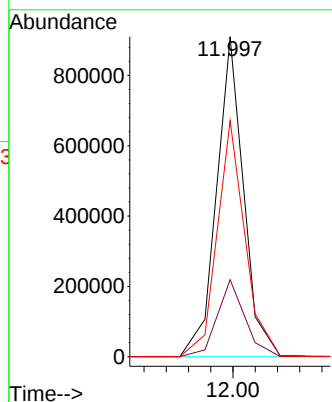

#36
2-Methylnaphthalene
Concen: 143.002 ng/ul
RT: 12.380 min Scan# 417
Delta R.T. 0.023 min
Lab File: BN018614.D
Acq: 15 Feb 2022 14:37

Tgt Ion:142 Resp: 3193504
Ion Ratio Lower Upper
142 100
141 90.4 70.2 105.4









#37
1-Methylnaphthalene
Concen: 130.169 ng/ul
RT: 12.606 min Scan# 426
Delta R.T. 0.023 min
Lab File: BN018614.D
Acq: 15 Feb 2022 14:37




Instrument :
BNA_N
ClientSampleId :
SSTD160228


Tgt Ion:142 Resp: 3070996
Ion Ratio Lower Upper
142 100
141 92.7 72.2 108.4
116 3.5 3.0 4.4



#39
1,2,4,5-Tetrachlorobenzene
Concen: 123.445 ng/ul
RT: 12.741 min Scan# 433
Delta R.T. -0.000 min
Lab File: BN018614.D
Acq: 15 Feb 2022 14:37

Tgt Ion:216 Resp: 1613659
Ion Ratio Lower Upper
216 100
214 79.0 64.4 96.6
179 24.1 15.1 22.7#
108 24.2 12.0 18.0#









#40
Hexachlorocyclopentadiene
Concen: 158.043 ng/ul
RT: 12.741 min Scan# 411
Delta R.T. 0.022 min
Lab File: BN018614.D
Acq: 15 Feb 2022 14:37




Instrument :
BNA_N
ClientSampleId :
SSTD160228


Tgt Ion:237 Resp: 1269169
Ion Ratio Lower Upper
237 100
235 63.3 49.1 73.7
272 14.2 10.6 16.0



#42
2,4,5-Trichlorophenol
Concen: 157.291 ng/ul
RT: 13.056 min Scan# 447
Delta R.T. 0.022 min
Lab File: BN018614.D
Acq: 15 Feb 2022 14:37

Tgt Ion:196 Resp: 1218415
Ion Ratio Lower Upper
196 100
198 98.9 75.3 112.9
200 31.4 24.2 36.2









#43
1,1'-Biphenyl
Concen: 124.877 ng/ul
RT: 13.371 min Scan# 461
Delta R.T. -0.000 min
Lab File: BN018614.D
Acq: 15 Feb 2022 14:37




Instrument :
BNA_N
ClientSampleId :
SSTD160228


Tgt Ion:154 Resp: 3867946
Ion Ratio Lower Upper
154 100
153 40.7 32.4 48.6
76 16.3 12.0 18.0



#44
2-Chloronaphthalene
Concen: 123.926 ng/ul
RT: 13.416 min Scan# 463
Delta R.T. -0.000 min
Lab File: BN018614.D
Acq: 15 Feb 2022 14:37

Tgt Ion:162 Resp: 2966910
Ion Ratio Lower Upper
162 100
164 32.2 26.8 40.2
127 46.3 28.8 43.2#









#45
2-Nitroaniline
Concen: 186.208 ng/ul
RT: 13.619 min Scan# 41
Delta R.T. 0.023 min
Lab File: BN018614.D
Acq: 15 Feb 2022 14:37




Instrument :
BNA_N
ClientSampleId :
SSTD160228


Tgt Ion: 65 Resp: 1023041
Ion Ratio Lower Upper
65 100
92 68.5 53.0 79.6
138 99.4 73.8 110.8

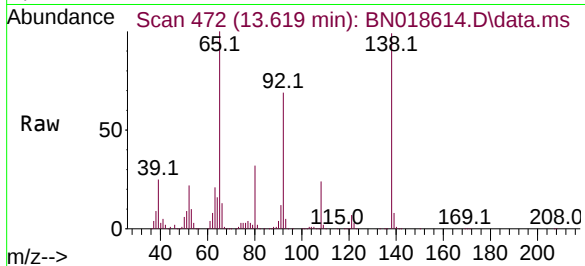

#47
Dimethylphthalate
Concen: 149.422 ng/ul
RT: 14.002 min Scan# 489
Delta R.T. 0.022 min
Lab File: BN018614.D
Acq: 15 Feb 2022 14:37

Tgt Ion:163 Resp: 3837975
Ion Ratio Lower Upper
163 100
194 4.2 3.6 5.4
164 10.3 8.2 12.4




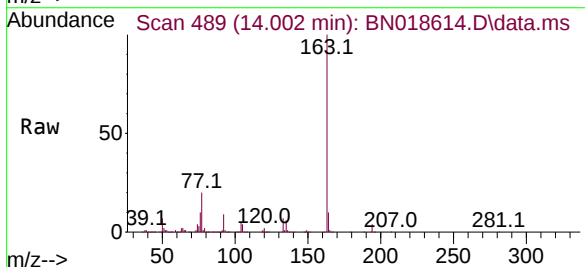




#48
2,6-Dinitrotoluene
Concen: 168.419 ng/ul
RT: 14.115 min Scan# 494
Delta R.T. 0.022 min
Lab File: BN018614.D
Acq: 15 Feb 2022 14:37




Instrument :
BNA_N
ClientSampleId :
SSTD160228


Tgt Ion:165 Resp: 789800
Ion Ratio Lower Upper
165 100
89 68.0 49.3 73.9
121 22.5 16.8 25.2

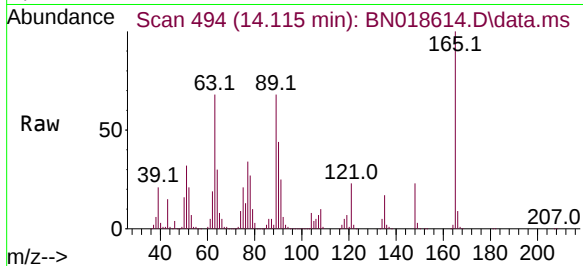

#50
Acenaphthylene
Concen: 143.093 ng/ul
RT: 14.272 min Scan# 501
Delta R.T. 0.023 min
Lab File: BN018614.D
Acq: 15 Feb 2022 14:37

Tgt Ion:152 Resp: 4955733
Ion Ratio Lower Upper
152 100
151 20.3 16.2 24.2
153 13.1 10.6 15.8




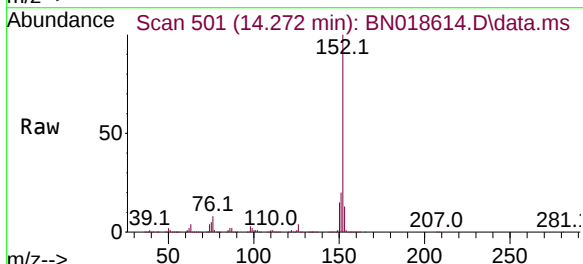




#51
3-Nitroaniline
Concen: 134.752 ng/ul
RT: 14.430 min Scan# 508
Delta R.T. -0.000 min
Lab File: BN018614.D
Acq: 15 Feb 2022 14:37




Instrument :
BNA_N
ClientSampleId :
SSTD160228


Tgt Ion:138 Resp: 628330
Ion Ratio Lower Upper
138 100
108 12.2 10.6 15.8
92 137.5 107.9 161.9

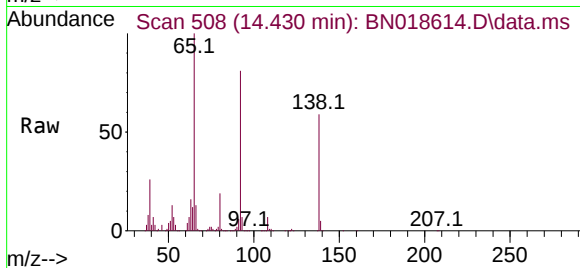

#52
Acenaphthene
Concen: 144.199 ng/ul
RT: 14.610 min Scan# 516
Delta R.T. -0.000 min
Lab File: BN018614.D
Acq: 15 Feb 2022 14:37

Tgt Ion:153 Resp: 3229545
Ion Ratio Lower Upper
153 100
152 47.4 37.5 56.3
154 88.5 69.8 104.6

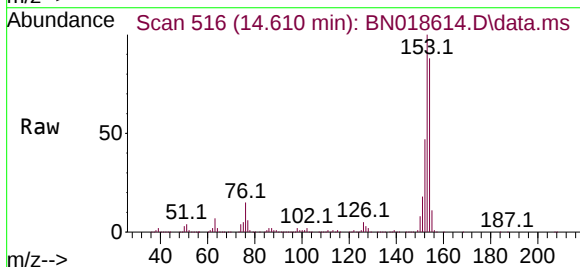



#53

2,4-Dinitrophenol

Concen: 176.192 ng/ul

RT: 14.655 min Scan# 517

Delta R.T. 0.023 min

Lab File: BN018614.D

Acq: 15 Feb 2022 14:37

Instrument :

BNA_N

ClientSampleId :

SSTD160228





Tgt Ion:184 Resp: 527286

Ion Ratio Lower Upper

184 100

63 30.1 58.6 87.8#

154 57.2 46.2 69.2

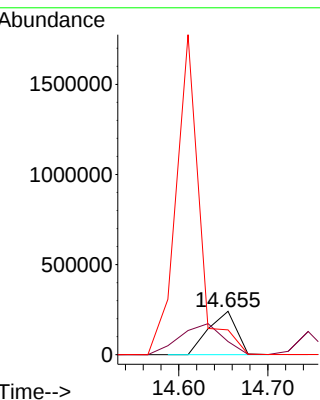

#55

4-Nitrophenol

Concen: 130.303 ng/ul

RT: 14.745 min Scan# 522

Delta R.T. 0.022 min

Lab File: BN018614.D

Acq: 15 Feb 2022 14:37




Tgt Ion:109 Resp: 520142


Ion Ratio Lower Upper

109 100

139 104.0 104.0 156.0

65 142.5 117.5 176.3



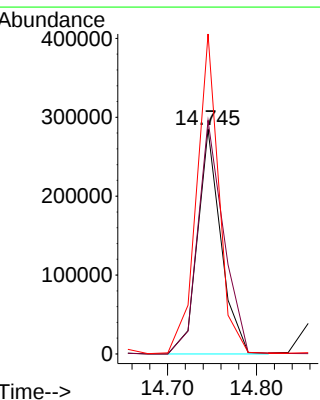





#56
Dibenzofuran
Concen: 139.930 ng/ul
RT: 14.948 min Scan# 51
Delta R.T. 0.023 min
Lab File: BN018614.D
Acq: 15 Feb 2022 14:37




Instrument :
BNA_N
ClientSampleId :
SSTD160228


Tgt Ion:168 Resp: 4533008
Ion Ratio Lower Upper
168 100
139 36.7 27.8 41.6



#57
2,4-Dinitrotoluene
Concen: 176.384 ng/ul
RT: 14.903 min Scan# 529
Delta R.T. 0.023 min
Lab File: BN018614.D
Acq: 15 Feb 2022 14:37

Tgt Ion:165 Resp: 1220913
Ion Ratio Lower Upper
165 100
63 39.6 36.0 54.0
182 2.9 2.2 3.2





#58

2,3,4,6-Tetrachlorophenol

Concen: 170.761 ng/ul

RT: 15.173 min Scan# 541

Delta R.T. 0.022 min

Lab File: BN018614.D


Acq: 15 Feb 2022 14:37

Instrument :

BNA_N

ClientSampleId :

SSTD160228



Tgt Ion:232 Resp: 985441




Ion Ratio Lower Upper

232 100

131 29.9 31.4 47.0#

130 1.6 1.8 2.6#

166 24.3 21.8 32.8



#59

Diethylphthalate

Concen: 134.446 ng/ul

RT: 15.354 min Scan# 549

Delta R.T. -0.000 min

Lab File: BN018614.D

Acq: 15 Feb 2022 14:37




Tgt Ion:149 Resp: 3511687


Ion Ratio Lower Upper

149 100

177 20.7 18.6 28.0

150 13.0 10.0 15.0









#61
Fluorene
Concen: 111.255 ng/ul
RT: 15.601 min Scan# 51
Delta R.T. 0.022 min
Lab File: BN018614.D
Acq: 15 Feb 2022 14:37




Instrument :
BNA_N
ClientSampleId :
SSTD160228


Tgt Ion:166 Resp: 2950977
Ion Ratio Lower Upper
166 100
165 96.4 79.0 118.4
167 12.5 11.0 16.4



#62
4-Chlorophenyl-phenylether
Concen: 123.212 ng/ul
RT: 15.579 min Scan# 559
Delta R.T. -0.000 min
Lab File: BN018614.D
Acq: 15 Feb 2022 14:37

Tgt Ion:204 Resp: 1685388
Ion Ratio Lower Upper
204 100
206 34.0 26.8 40.2
141 68.0 43.1 64.7#









#63
4-Nitroaniline
Concen: 121.638 ng/ul
RT: 15.601 min Scan# 51
Delta R.T. 0.022 min
Lab File: BN018614.D
Acq: 15 Feb 2022 14:37




Instrument :
BNA_N
ClientSampleId :
SSTD160228


Tgt Ion:138 Resp: 458987
Ion Ratio Lower Upper
138 100
92 55.3 45.6 68.4
108 94.2 68.0 102.0



#66
4,6-Dinitro-2-methylphenol
Concen: 179.211 ng/ul
RT: 15.669 min Scan# 563
Delta R.T. 0.022 min
Lab File: BN018614.D
Acq: 15 Feb 2022 14:37

Tgt Ion:198 Resp: 758706
Ion Ratio Lower Upper
198 100
182 3.3 3.4 5.2#
77 22.0 21.1 31.7









#67
N-Nitrosodiphenylamine
Concen: 117.634 ng/ul
RT: 15.782 min Scan# 509
Delta R.T. -0.000 min
Lab File: BN018614.D
Acq: 15 Feb 2022 14:37




Instrument :
BNA_N
ClientSampleId :
SSTD160228


Tgt Ion:169 Resp: 2656919
Ion Ratio Lower Upper
169 100
168 67.0 52.2 78.4
167 36.9 27.4 41.2

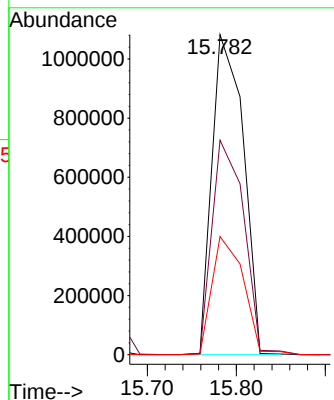

#68
4-Bromophenyl-phenylether
Concen: 166.864 ng/ul
RT: 16.480 min Scan# 599
Delta R.T. -0.000 min
Lab File: BN018614.D
Acq: 15 Feb 2022 14:37

Tgt Ion:248 Resp: 1147834
Ion Ratio Lower Upper
248 100
250 100.9 72.3 108.5
141 52.3 53.7 80.5#



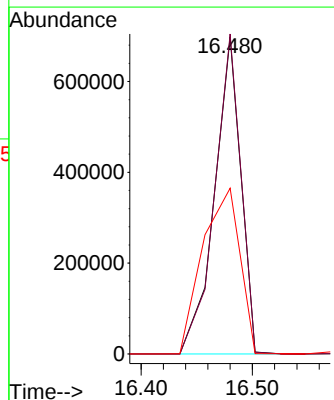





#69
Hexachlorobenzene
Concen: 125.645 ng/ul
RT: 16.593 min Scan# 604
Delta R.T. -0.000 min
Lab File: BN018614.D
Acq: 15 Feb 2022 14:37




Instrument :
BNA_N
ClientSampleId :
SSTD160228


Tgt Ion:284 Resp: 1156725
Ion Ratio Lower Upper
284 100
142 46.5 24.3 36.5#
249 36.7 23.8 35.6#



#70
Atrazine
Concen: 164.621 ng/ul
RT: 16.750 min Scan# 611
Delta R.T. 0.023 min
Lab File: BN018614.D
Acq: 15 Feb 2022 14:37

Tgt Ion:200 Resp: 1293009
Ion Ratio Lower Upper
200 100
173 24.3 20.2 30.2
215 48.5 39.7 59.5









#71
Pentachlorophenol
Concen: 159.889 ng/ul
RT: 16.930 min Scan# 619
Delta R.T. -0.000 min
Lab File: BN018614.D
Acq: 15 Feb 2022 14:37




Instrument :
BNA_N
ClientSampleId :
SSTD160228


Tgt Ion:266 Resp: 839756
Ion Ratio Lower Upper
266 100
264 63.8 52.0 78.0
268 63.2 53.5 80.3



#72
Phenanthrene
Concen: 136.091 ng/ul
RT: 17.336 min Scan# 637
Delta R.T. 0.023 min
Lab File: BN018614.D
Acq: 15 Feb 2022 14:37

Tgt Ion:178 Resp: 5308145
Ion Ratio Lower Upper
178 100
179 14.9 12.2 18.4
176 18.7 14.6 21.8









#74
 Anthracene
 Concen: 138.160 ng/uI
 RT: 17.426 min Scan# 641
 Delta R.T. 0.023 min
 Lab File: BN018614.D
 Acq: 15 Feb 2022 14:37




Instrument :
 BNA_N
 ClientSampleId :
 SSTD160228


Tgt Ion:178 Resp: 5323567
 Ion Ratio Lower Upper
 178 100
 179 15.2 12.3 18.5
 176 18.8 14.7 22.1



#75
 1,2,3,4-Tetrachlorobenzene
 Concen: 140.608 ng/uI
 RT: 13.349 min Scan# 460
 Delta R.T. -0.000 min
 Lab File: BN018614.D
 Acq: 15 Feb 2022 14:37

Tgt Ion:216 Resp: 1859484
 Ion Ratio Lower Upper
 216 100
 214 79.4 63.1 94.7
 218 47.7 39.8 59.6









#76
Pentachlorobenzene
Concen: 125.211 ng/uL
RT: 14.858 min Scan# 51
Delta R.T. -0.000 min
Lab File: BN018614.D
Acq: 15 Feb 2022 14:37




Instrument :
BNA_N
ClientSampleId :
SSTD160228


Tgt Ion:250 Resp: 1449591
Ion Ratio Lower Upper
250 100
248 64.8 49.5 74.3
252 62.6 52.7 79.1



#77
Carbazole
Concen: 128.240 ng/uL
RT: 17.674 min Scan# 652
Delta R.T. -0.000 min
Lab File: BN018614.D
Acq: 15 Feb 2022 14:37

Tgt Ion:167 Resp: 4318726
Ion Ratio Lower Upper
167 100
166 21.9 16.9 25.3
139 14.5 9.6 14.4#









#78
Di-n-butylphthalate
Concen: 143.219 ng/ul
RT: 18.237 min Scan# 61
Delta R.T. -0.000 min
Lab File: BN018614.D
Acq: 15 Feb 2022 14:37




Instrument :
BNA_N
ClientSampleId :
SSTD160228


Tgt Ion:149 Resp: 5146604
Ion Ratio Lower Upper
149 100
150 9.4 7.3 10.9
104 7.0 4.2 6.2#



#80
Fluoranthene
Concen: 186.936 ng/ul
RT: 19.341 min Scan# 726
Delta R.T. -0.000 min
Lab File: BN018614.D
Acq: 15 Feb 2022 14:37

Tgt Ion:202 Resp: 6528422
Ion Ratio Lower Upper
202 100
101 7.9 8.5 12.7#
100 6.0 6.4 9.6#









#82
Pyrene
Concen: 150.977 ng/ul
RT: 19.701 min Scan# 742
Delta R.T. -0.000 min
Lab File: BN018614.D
Acq: 15 Feb 2022 14:37




Instrument :
BNA_N
ClientSampleId :
SSTD160228


Tgt Ion:202 Resp: 5798451
Ion Ratio Lower Upper
202 100
101 12.5 9.6 14.4
100 10.3 7.8 11.8



#83
Butylbenzylphthalate
Concen: 219.987 ng/ul
RT: 20.580 min Scan# 781
Delta R.T. -0.023 min
Lab File: BN018614.D
Acq: 15 Feb 2022 14:37

Tgt Ion:149 Resp: 2086885
Ion Ratio Lower Upper
149 100
91 106.9 63.7 95.5#
206 13.4 19.1 28.7#


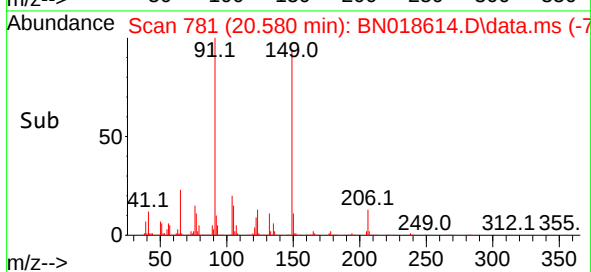






#84
3,3'-Dichlorobenzidine
Concen: 137.643 ng/ul
RT: 21.368 min Scan# 816
Delta R.T. -0.000 min
Lab File: BN018614.D
Acq: 15 Feb 2022 14:37




Instrument :
BNA_N
ClientSampleId :
SSTD160228


Tgt Ion:252 Resp: 1458794
Ion Ratio Lower Upper
252 100
254 63.4 51.5 77.3
126 14.3 7.9 11.9#

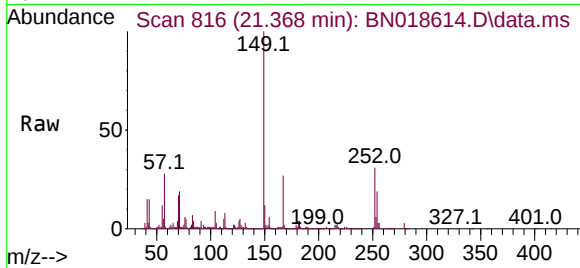

#85
Benzo(a)anthracene
Concen: 163.836 ng/ul
RT: 21.458 min Scan# 820
Delta R.T. 0.023 min
Lab File: BN018614.D
Acq: 15 Feb 2022 14:37

Tgt Ion:228 Resp: 6031234
Ion Ratio Lower Upper
228 100
229 19.0 15.4 23.2
226 26.9 21.0 31.6




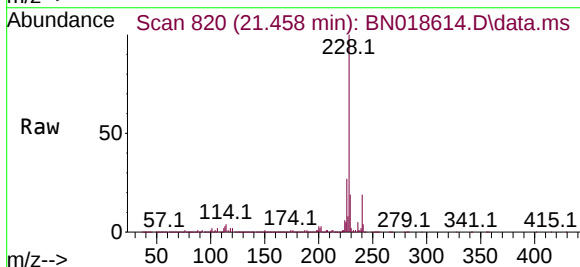




#86
 Bis(2-ethylhexyl)phthalate
 Concen: 170.812 ng/ul
 RT: 21.368 min Scan# 816
 Delta R.T. -0.000 min
 Lab File: BN018614.D
 Acq: 15 Feb 2022 14:37




Instrument :
 BNA_N
 ClientSampleId :
 SSTD160228


Tgt Ion:149 Resp: 3736520
 Ion Ratio Lower Upper
 149 100
 167 26.9 23.4 35.0
 279 2.7 4.1 6.1#



#87
 Chrysene
 Concen: 172.332 ng/ul
 RT: 21.503 min Scan# 822
 Delta R.T. -0.000 min
 Lab File: BN018614.D
 Acq: 15 Feb 2022 14:37

Tgt Ion:228 Resp: 5363406
 Ion Ratio Lower Upper
 228 100
 226 32.3 23.5 35.3
 229 20.7 15.0 22.4









#89
Di-n-octyl phthalate
Concen: 155.717 ng/ul
RT: 22.291 min Scan# 857
Delta R.T. -0.000 min
Lab File: BN018614.D
Acq: 15 Feb 2022 14:37




Instrument :
BNA_N
ClientSampleId :
SSTD160228


Tgt Ion:149 Resp: 6731784

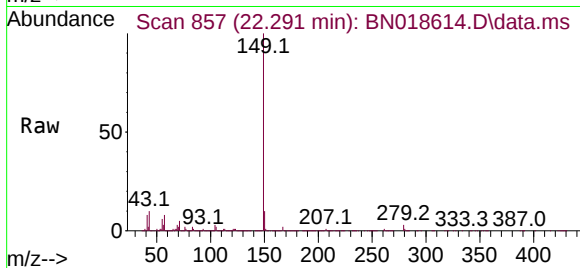

#90
Benzo(b)fluoranthene
Concen: 187.413 ng/ul
RT: 23.147 min Scan# 895
Delta R.T. 0.023 min
Lab File: BN018614.D
Acq: 15 Feb 2022 14:37

Tgt Ion:252 Resp: 8213471
Ion Ratio Lower Upper
252 100
253 21.8 17.8 26.6
125 5.9 7.2 10.8#




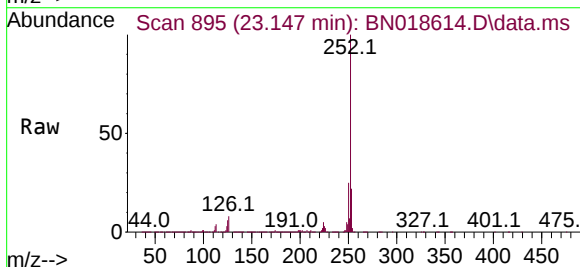




#91
Benzo(k)fluoranthene
Concen: 111.416 ng/ul
RT: 23.192 min Scan# 896
Delta R.T. 0.023 min
Lab File: BN018614.D
Acq: 15 Feb 2022 14:37




Instrument :
BNA_N
ClientSampleId :
SSTD160228


Tgt Ion:252 Resp: 4330502
Ion Ratio Lower Upper
252 100
253 21.6 17.3 25.9
125 6.6 6.9 10.3#



#93
Benzo(a)pyrene
Concen: 153.960 ng/ul
RT: 23.778 min Scan# 923
Delta R.T. 0.023 min
Lab File: BN018614.D
Acq: 15 Feb 2022 14:37

Tgt Ion:252 Resp: 6379298
Ion Ratio Lower Upper
252 100
253 21.8 19.3 28.9
125 6.7 8.0 12.0#

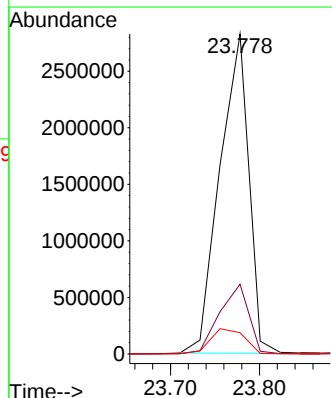

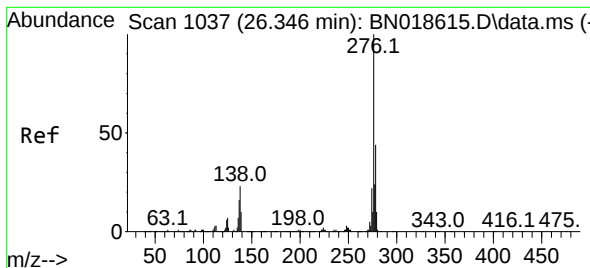

#94

Indeno(1,2,3-cd)pyrene

Concen: 160.377 ng/ul

RT: 26.391 min Scan# 1039

Delta R.T. 0.045 min

Lab File: BN018614.D

Acq: 15 Feb 2022 14:37

Instrument :

BNA_N

ClientSampleId :

SSTD160228





Tgt Ion:276 Resp: 7548636

Ion Ratio Lower Upper

276 100

138 24.5 16.6 24.8

277 26.8 19.1 28.7

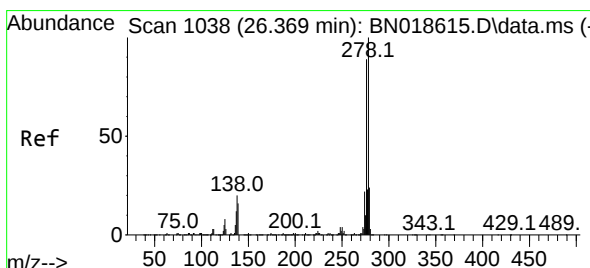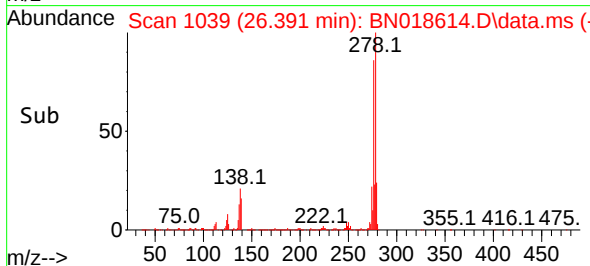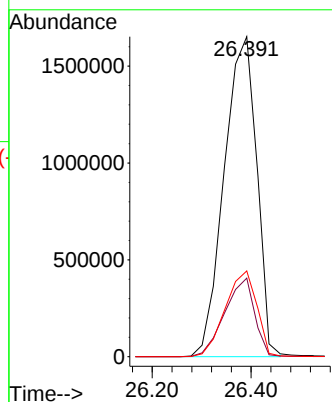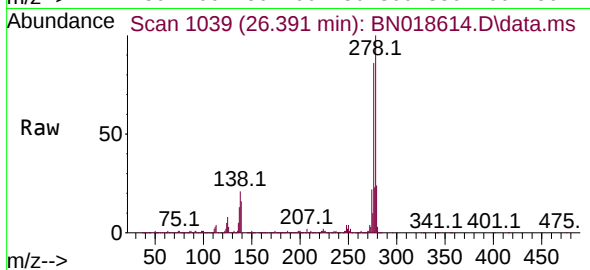

#95

Dibenzo(a,h)anthracene

Concen: 155.391 ng/ul

RT: 26.391 min Scan# 1039

Delta R.T. 0.023 min

Lab File: BN018614.D

Acq: 15 Feb 2022 14:37




Tgt Ion:278 Resp: 6195818


Ion Ratio Lower Upper

278 100

139 16.4 11.7 17.5


279 24.3 19.1 28.7

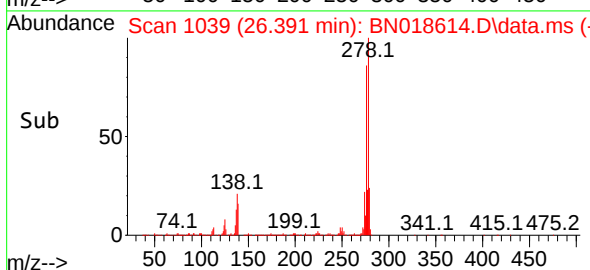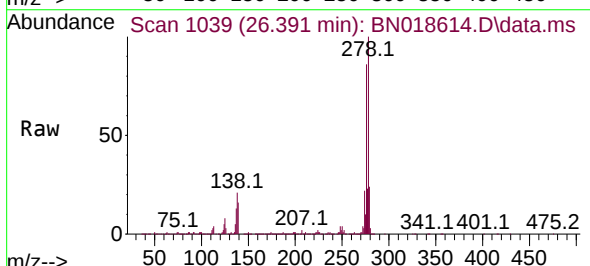



#96
 Benzo(g,h,i)perylene
 Concen: 165.050 ng/ul
 RT: 27.157 min Scan# 1073
 Delta R.T. 0.045 min
 Lab File: BN018614.D
 Acq: 15 Feb 2022 14:37

Instrument :
 BNA_N
 ClientSampleId :
 SSTD160228



Tgt Ion:276 Resp: 6624372

Ion	Ratio	Lower	Upper
276	100		
138	18.1	15.6	23.4
277	23.8	17.8	26.6

