
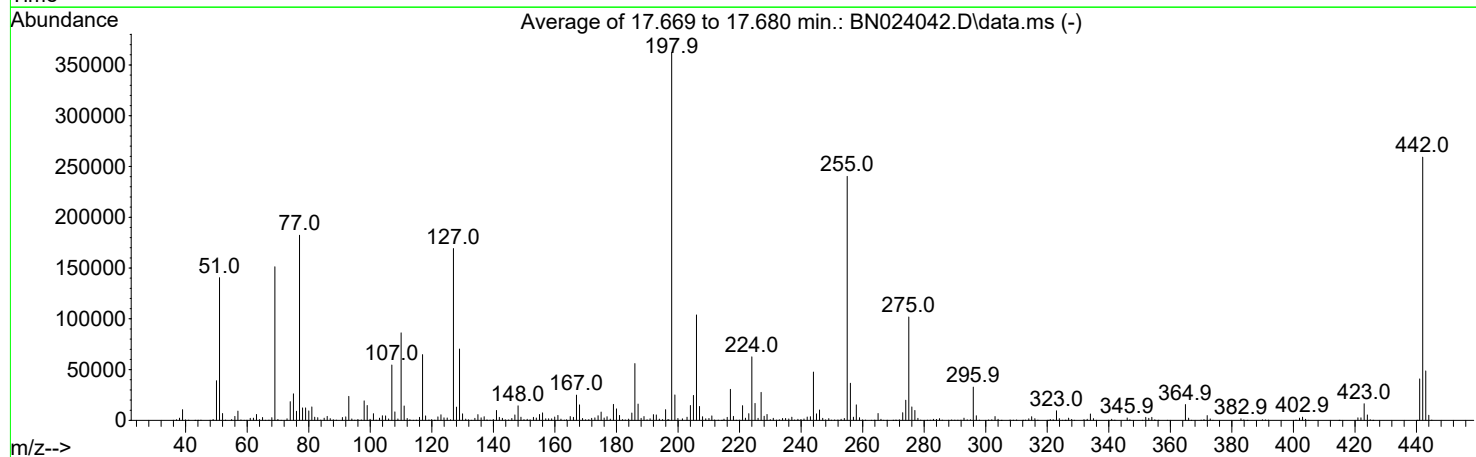


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021523\
Data File : BN024042.D
Acq On : 15 Feb 2023 09:10
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN020723.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Feb 15 02:55:51 2023

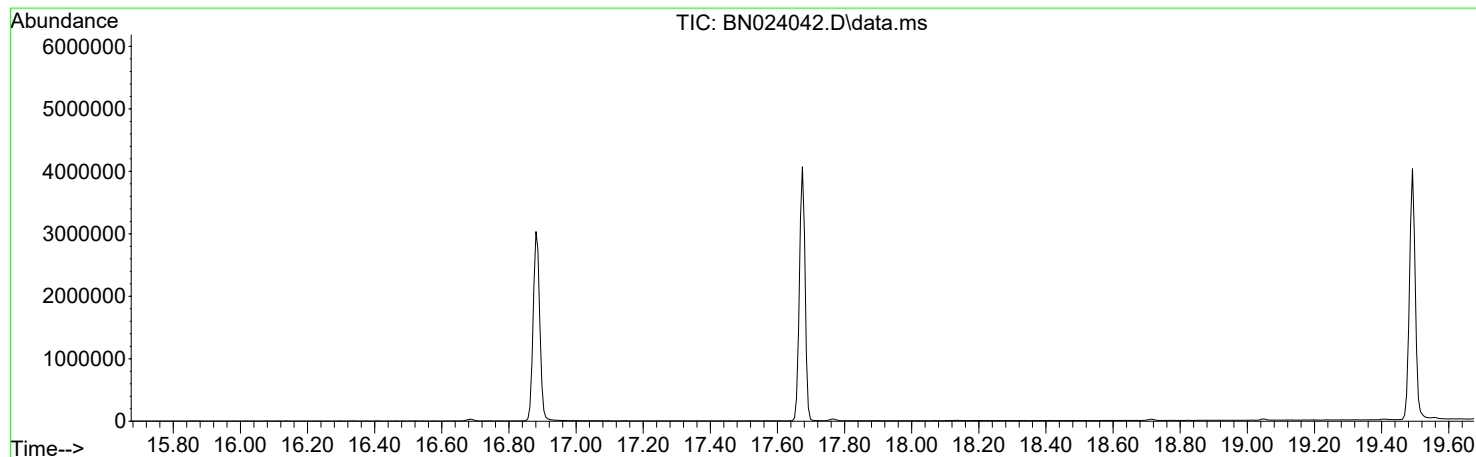




AutoFind: Scans 2479, 2480, 2481; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.8	140565	PASS
68	69	0.00	2	1.8	2706	PASS
69	198	0.00	100	41.8	151312	PASS
70	69	0.00	2	0.6	880	PASS
127	198	10	80	46.7	169301	PASS
197	198	0.00	2	0.2	859	PASS
198	198	100	100	100.0	362240	PASS
199	198	5	9	6.9	25011	PASS
275	198	10	60	28.1	101733	PASS
365	198	1	100	4.3	15614	PASS
441	198	0.01	100	11.2	40739	PASS
442	442	50	100	100.0	259221	PASS
443	442	15	24	18.8	48629	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021523\
 Data File : BN024042.D
 Acq On : 15 Feb 2023 09:10
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Feb 16 03:59:37 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 16 03:59:32 2023
 Response via : Initial Calibration

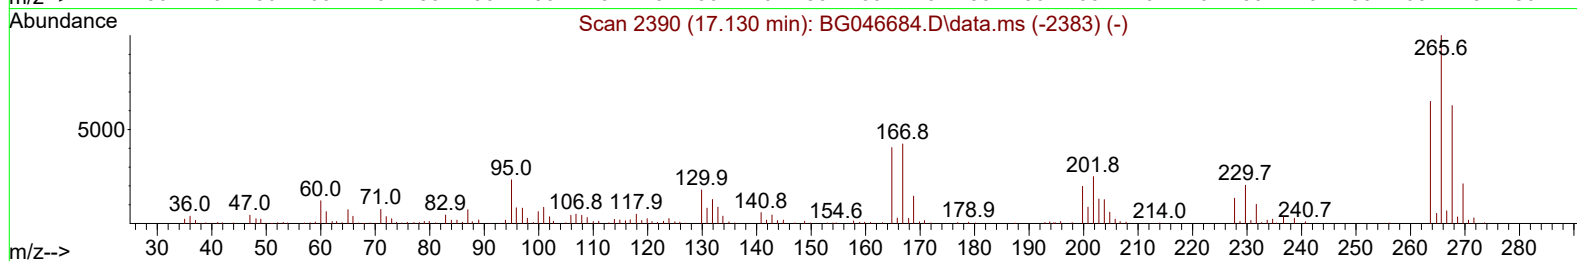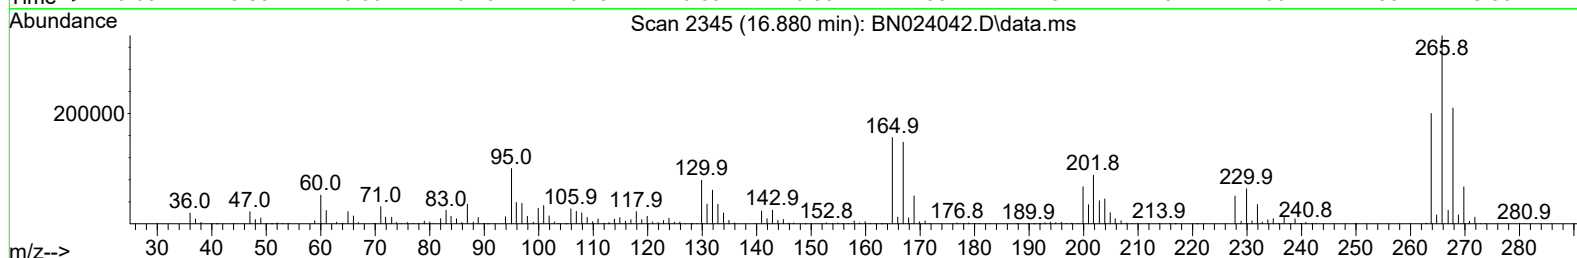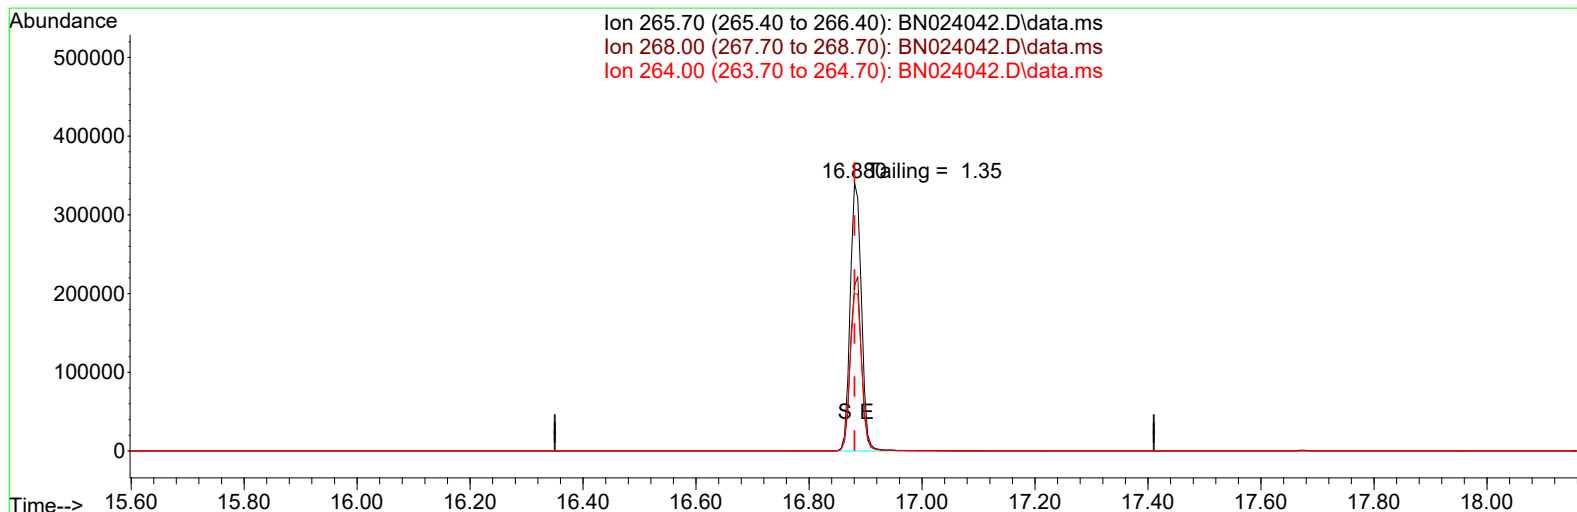

TIC: BN024042.D\data.ms

(70) Pentachlorophenol (C)

16.880min (0.000) 21879.52 ng




response 473734

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.59
264.00	61.60	58.66
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021523\
Data File : BN024042.D
Acq On : 15 Feb 2023 09:10
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Feb 16 03:59:37 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 16 03:59:32 2023
Response via : Initial Calibration

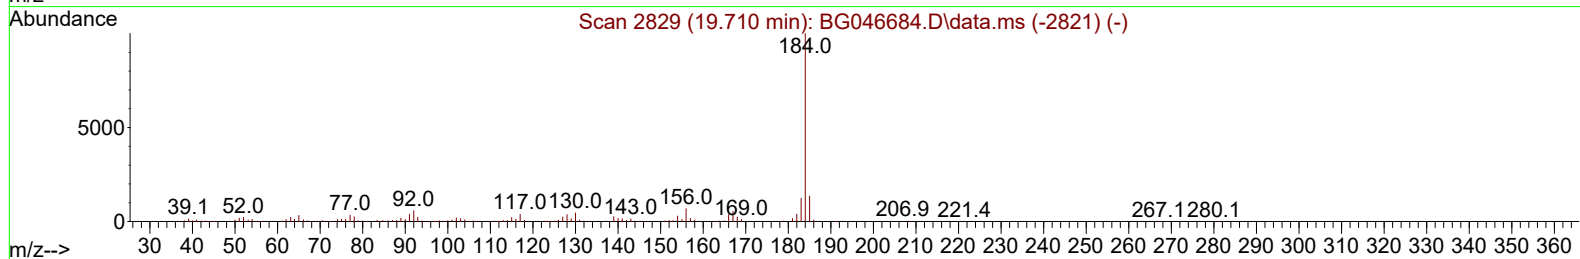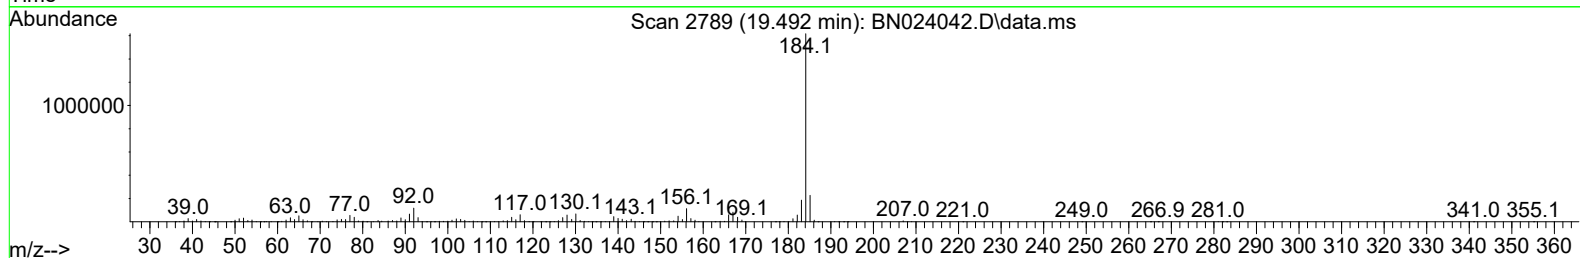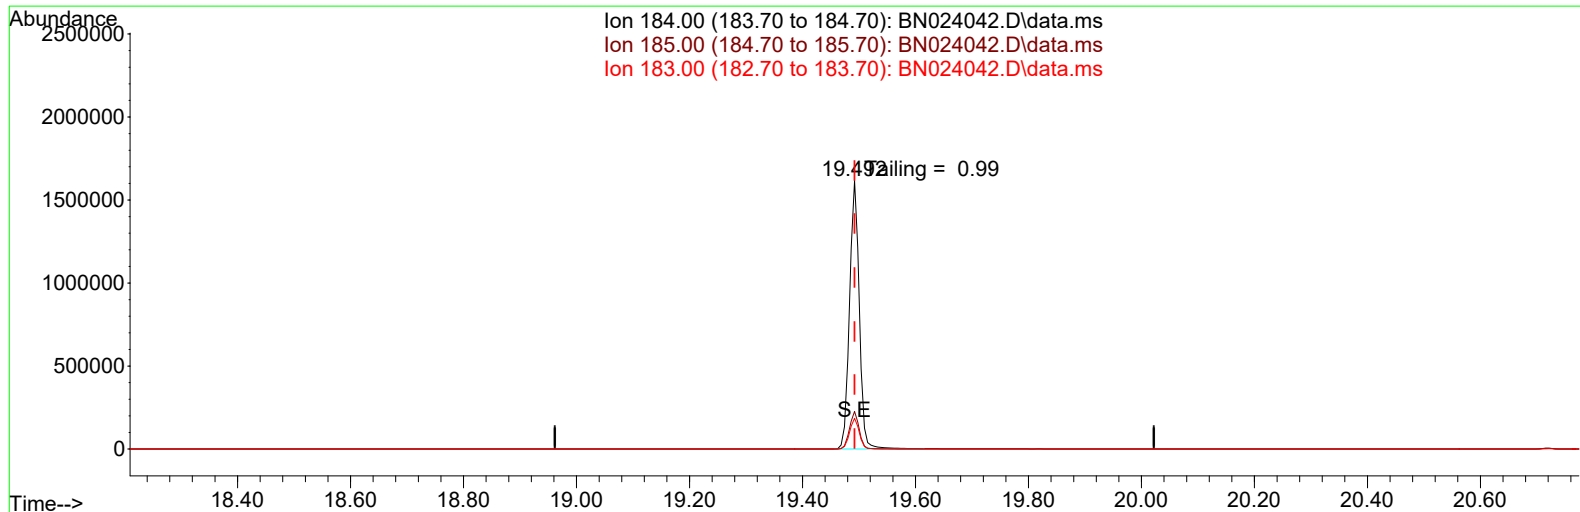

TIC: BN024042.D\data.ms

(77) Benzidine

19.492min (0.000) 0.00 ng

response 1950639

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.03
183.00	13.20	11.48
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/15/2023	BNA_N	<u>BN024042.D</u>
Compound Name	Response	Retention Time
DDT	1308764	20.721
DDD	20387	20.28
DDE	1518	19.768
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
21905	1330669	1.65

Instrument :
BNA_N
ClientSampleId :
DFTPP