


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN021621\
Data File : BN013639.D
Acq On : 16 Feb 2021 15:11
Operator : CG/JU
Sample : M1349-17
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBGS9

Manual Integrations
APPROVED

mohammad
2/17/2021 1:48:52 PM

Quant Time: Feb 16 15:42:49 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN020421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 16 10:14:45 2021
Response via : Initial Calibration

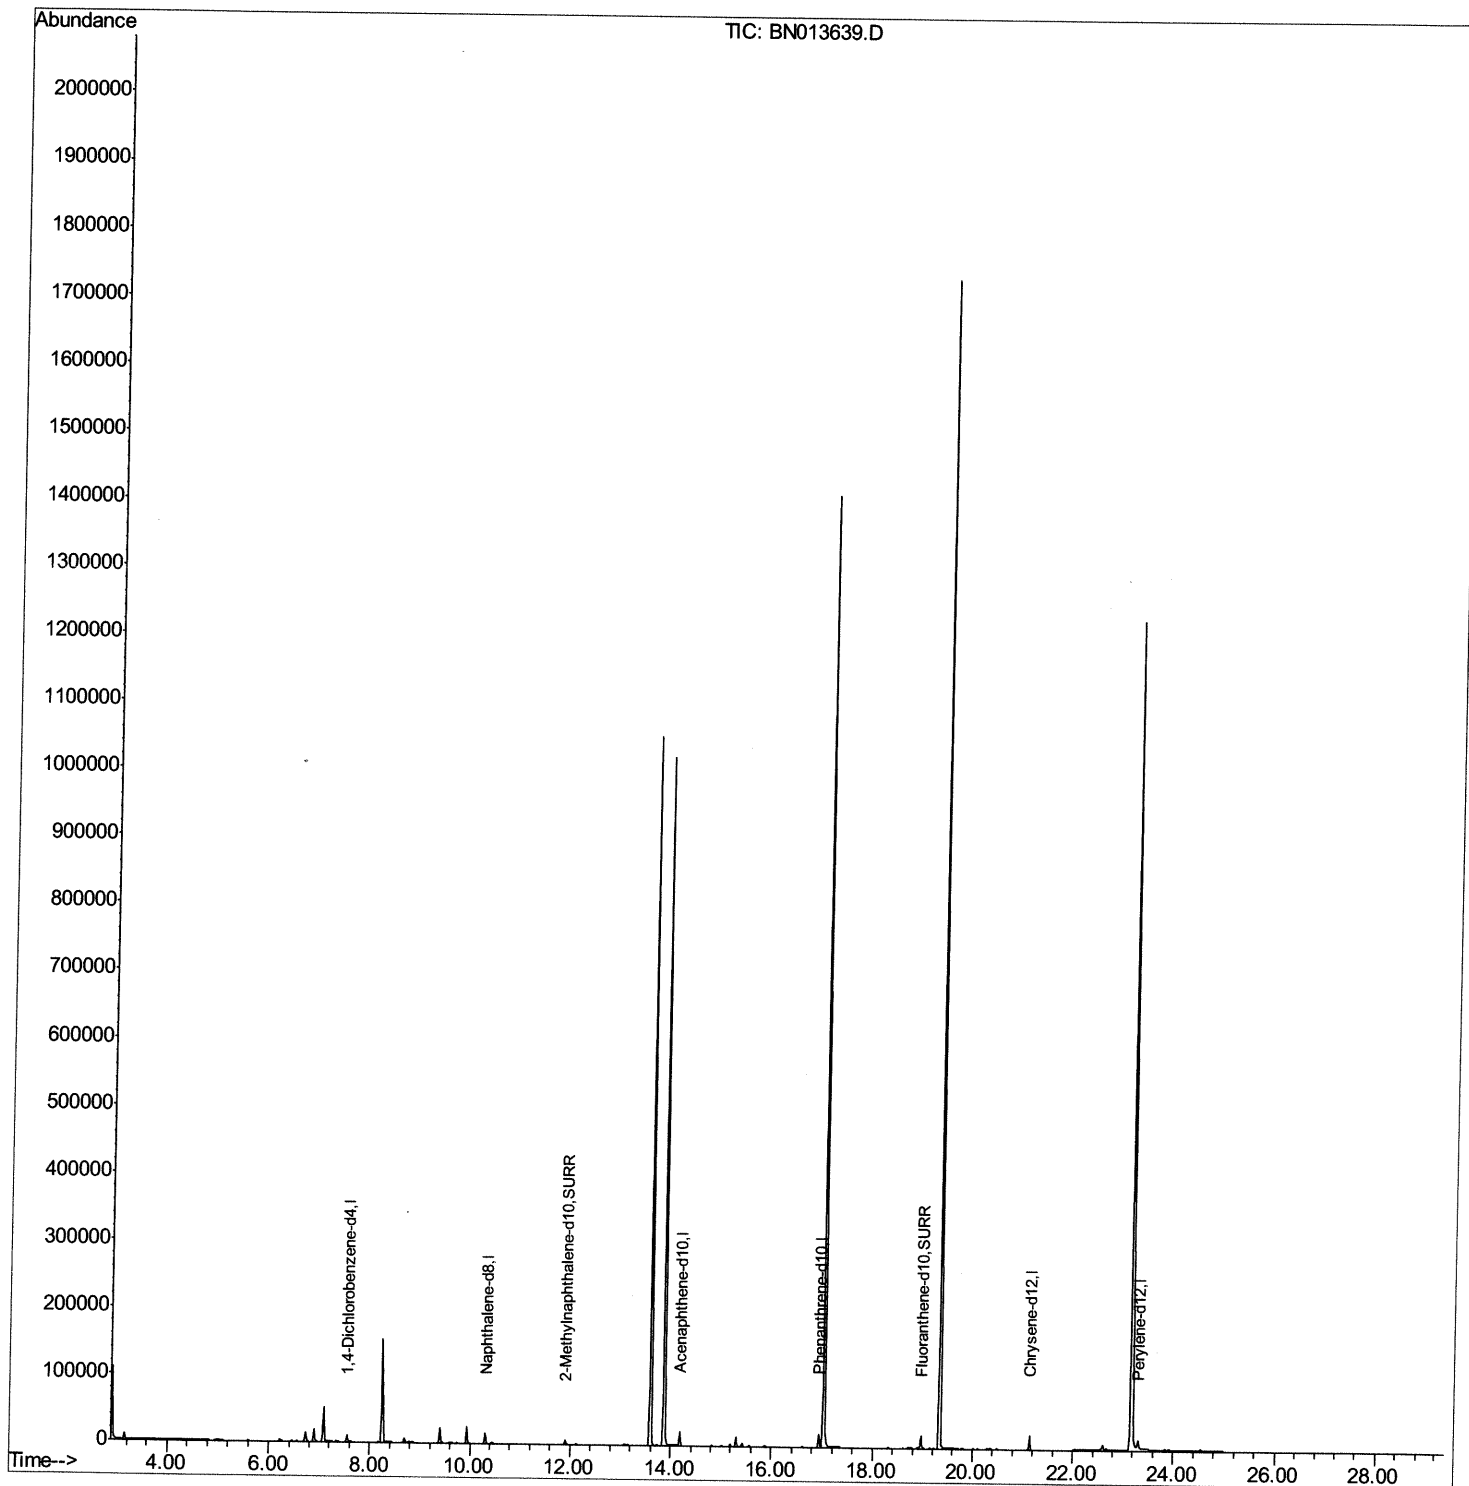

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN021621\
 Data File : BN013639.D
 Acq On : 16 Feb 2021 15:11
 Operator : CG/JU
 Sample : M1349-17
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBGS9

Manual Integrations
 APPROVED

mohammad
 2/17/2021 1:48:52 PM

Quant Time: Feb 16 15:41:24 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN020421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 16 10:14:45 2021
 Response via : Initial Calibration

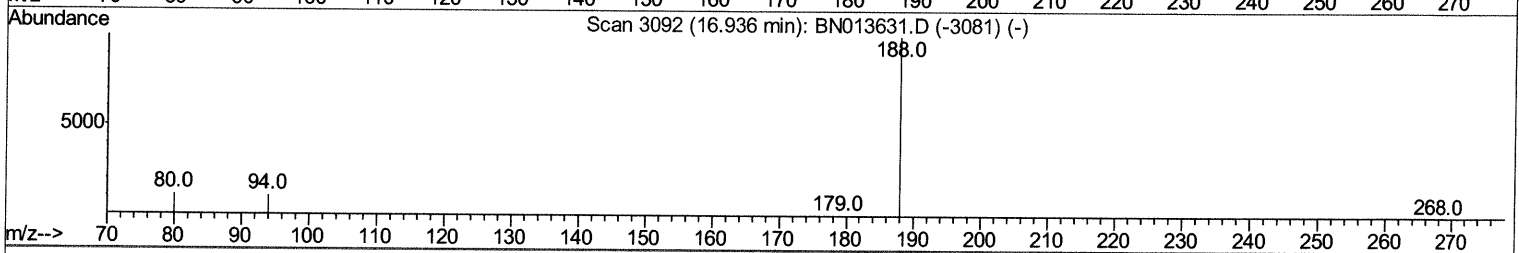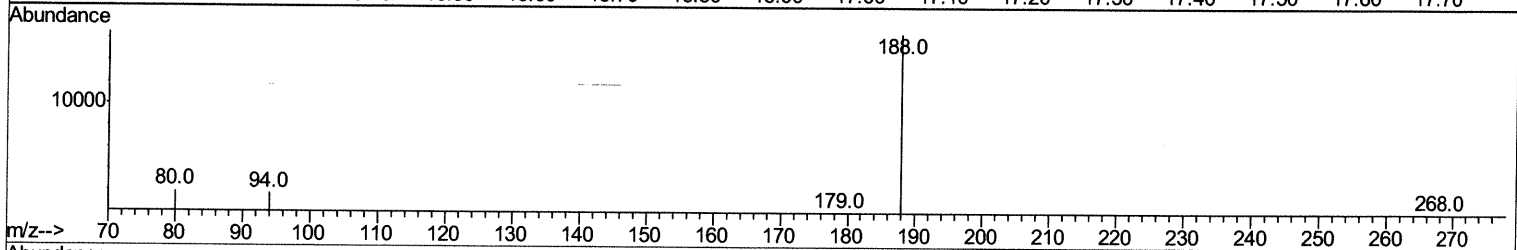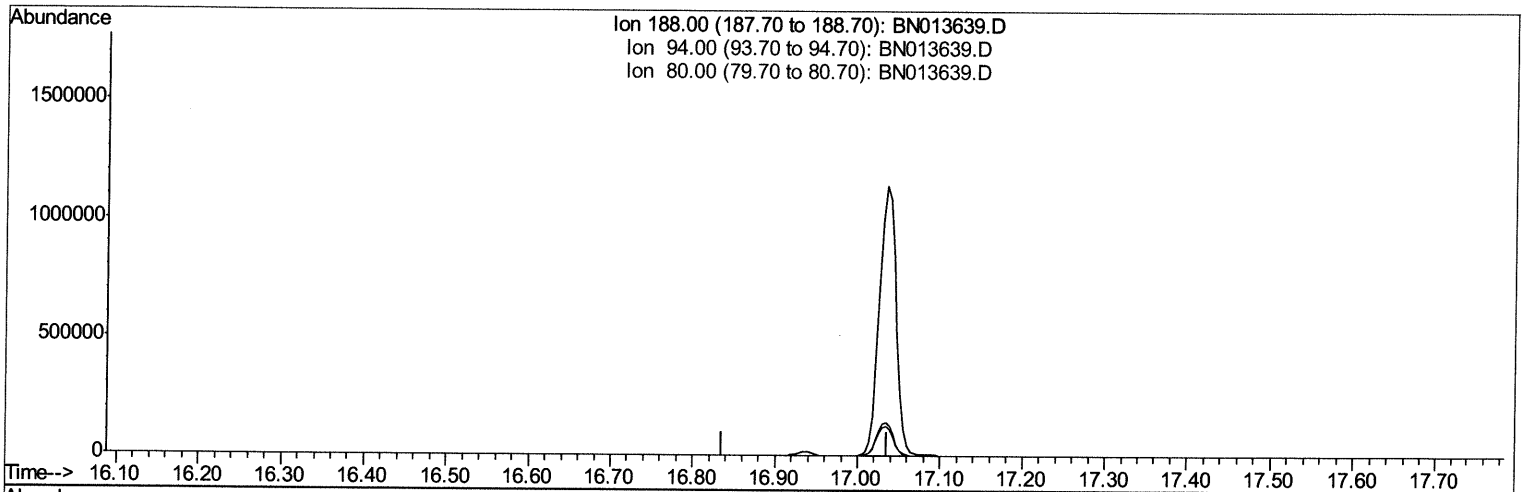

TIC: BN013639.D

(10) Phenanthrene-d10 (I)

16.936min (-16.936) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	10.60	0.00#
80.00	11.30	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN021621\
Data File : BN013639.D
Acq On : 16 Feb 2021 15:11
Operator : CG/JU
Sample : M1349-17
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBGS9

Manual Integrations
APPROVED

mohammad
2/17/2021 1:48:52 PM

Quant Time: Feb 16 15:41:24 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN020421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 16 10:14:45 2021
Response via : Initial Calibration

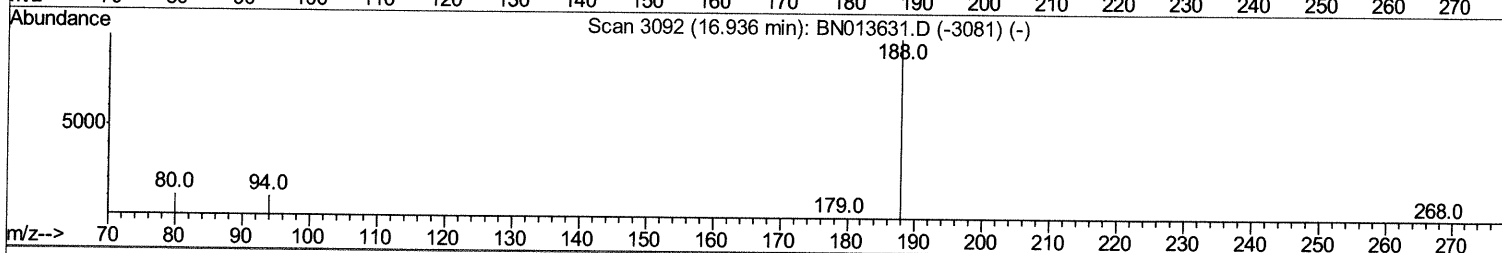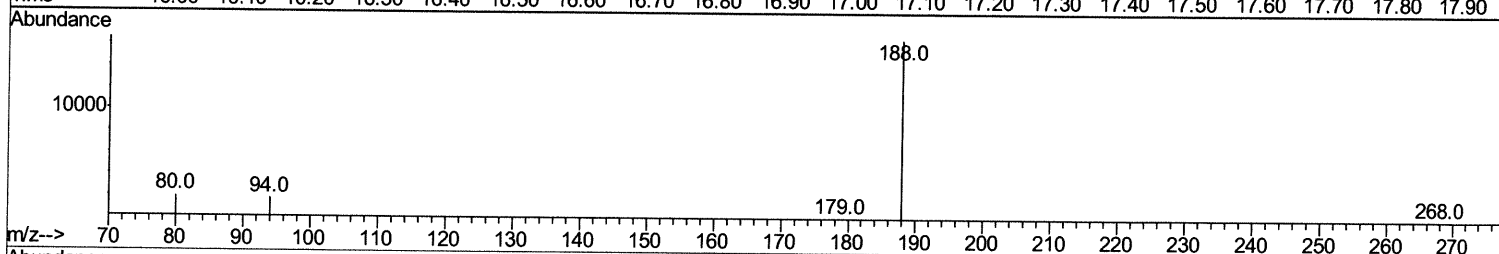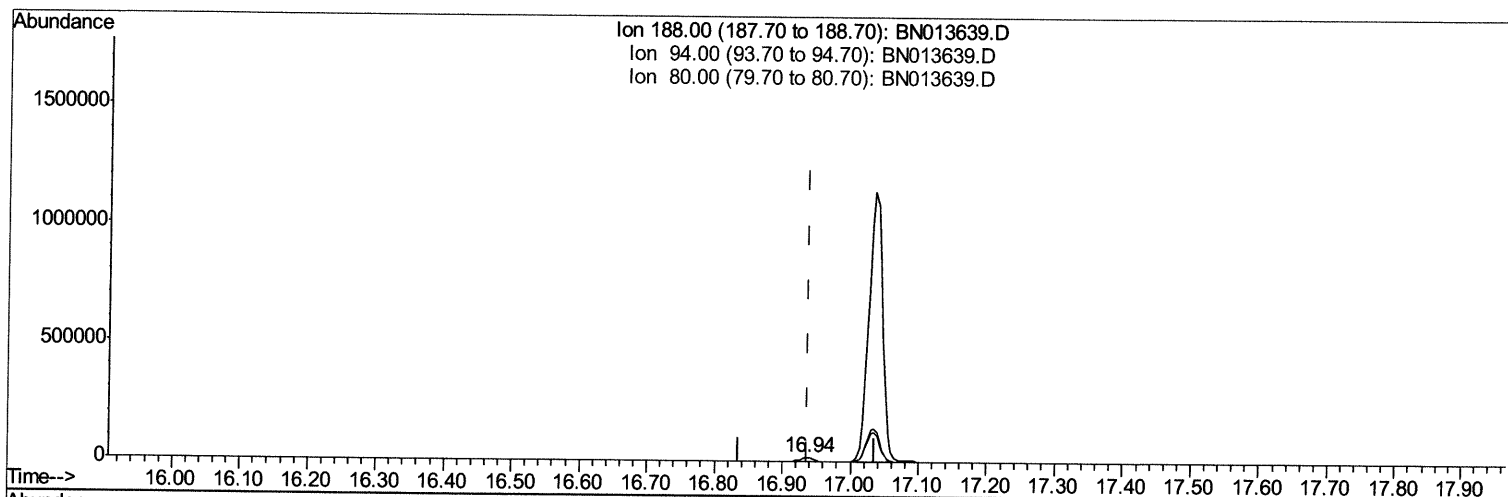

TIC: BN013639.D

(10) Phenanthrene-d10 (I)

16.937min (+0.000) 0.40ng/ul m 02/16/21 JU

response 22896

Ion	Exp%	Act%
188.00	100	100
94.00	10.60	10.33
80.00	11.30	11.25
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN021621\
 Data File : BN013639.D
 Acq On : 16 Feb 2021 15:11
 Operator : CG/JU
 Sample : M1349-17
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBGS9

Manual Integrations
 APPROVED

mohammad
 2/17/2021 1:48:52 PM

Quant Time: Feb 16 15:42:49 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN020421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 16 10:14:45 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.55	152	5049	0.40	ng/ul	0.00
2) Naphthalene-d8	10.31	136	19824	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.19	164	11294	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.94	188	22896m >	0.40	ng/ul >	0.00
16) Chrysene-d12	21.14	240	19272	0.40	ng/ul	0.00
20) Perylene-d12	23.31	264	18601	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.91	152	8087	0.29	ng/ul	0.00
14) Fluoranthene-d10	18.97	212	20025	0.36	ng/ul	0.00

Target Compounds Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed