

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021623\
 Data File : BN024056.D
 Acq On : 16 Feb 2023 16:17
 Operator : CG/JU
 Sample : PB150778BS
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SLCS878

Quant Time: Feb 17 05:37:14 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020623.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Feb 17 05:33:41 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.828	152	166636	20.000	ng/u1	0.00
20) Naphthalene-d8	10.640	136	751699	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.487	164	493773	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.233	188	1082231	20.000	ng/u1	0.00
79) Chrysene-d12	21.427	240	899199	20.000	ng/u1	0.00
88) Perylene-d12	23.804	264	796166	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.222	96	26389	6.404	ng/uL	0.00
4) Pyridine-d5	3.646	84	368601	32.246	ng/u1	0.00
7) Phenol-d5	7.005	99	523260	36.732	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.169	67	327266	36.406	ng/u1	0.00
11) 2-Chlorophenol-d4	7.358	132	407400	36.771	ng/u1	0.00
15) 4-Methylphenol-d8	8.552	113	421864	37.908	ng/u1	0.00
21) Nitrobenzene-d5	9.005	128	209105	34.845	ng/u1	0.00
24) 2-Nitrophenol-d4	9.722	143	233981	34.725	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.263	165	445875	35.509	ng/u1	0.00
31) 4-Chloroaniline-d4	10.787	131	543446	32.023	ng/u1	0.00
46) Dimethylphthalate-d6	13.904	166	1325620	34.735	ng/u1	0.00
49) Acenaphthylene-d8	14.181	160	1488999	35.218	ng/u1	0.00
54) 4-Nitrophenol-d4	14.704	143	242798	36.985	ng/u1	0.01
60) Fluorene-d10	15.481	176	1127872	35.100	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.610	200	260048	34.779	ng/u1	0.00
73) Anthracene-d10	17.333	188	1703423	34.553	ng/u1	0.00
81) Pyrene-d10	19.633	212	1970452	36.378	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.645	264	1445847	35.496	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.258	88	51649	11.850	ng/uL#	90
5) Pyridine	3.664	79	367864	32.010	ng/u1	94
6) Benzaldehyde	6.969	77	304177	49.283	ng/u1	98
8) Phenol	7.028	94	531667	36.975	ng/u1	99
10) Bis(2-Chloroethyl)ether	7.258	93	425081	36.372	ng/u1	99
12) 2-Chlorophenol	7.393	128	415646	36.897	ng/u1	99
13) 2-Methylphenol	8.281	108	399243	37.064	ng/u1	95
14) 2,2'-oxybis(1-Chloropr...	8.369	45	550799	37.832	ng/u1	100
16) Acetophenone	8.663	105	657918	37.897	ng/u1	98
17) N-Nitroso-di-n-propyla...	8.657	70	367469	39.413	ng/u1	95
18) 4-Methylphenol	8.616	108	445540	38.393	ng/u1	99
19) Hexachloroethane	8.905	117	178680	37.961	ng/u1	91
22) Nitrobenzene	9.046	77	537249	35.288	ng/u1	99
23) Isophorone	9.575	82	1016150	36.270	ng/u1	98
25) 2-Nitrophenol	9.757	139	252881	35.873	ng/u1	98
26) 2,4-Dimethylphenol	9.822	107	496315	35.337	ng/u1	97
27) Bis(2-Chloroethoxy)met...	10.057	93	611172	35.120	ng/u1	97
29) 2,4-Dichlorophenol	10.287	162	430887	35.385	ng/u1	99
30) Naphthalene	10.687	128	1371574	34.026	ng/u1	99
32) 4-Chloroaniline	10.804	127	510234	30.118	ng/u1	96
33) Hexachlorobutadiene	10.969	225	291855	33.423	ng/u1	97
34) Caprolactam	11.604	113	83498	24.113	ng/u1	92
35) 4-Chloro-3-methylphenol	11.940	107	479756	37.495	ng/u1	100
36) 2-Methylnaphthalene	12.304	142	952781	35.106	ng/u1	99

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021623\
 Data File : BN024056.D
 Acq On : 16 Feb 2023 16:17
 Operator : CG/JU
 Sample : PB150778BS
 Misc :
 ALS Vial : 8 Sample Multiplier: 1


Instrument :
 BNA_N
 ClientSampleId :
 SLCS878


Quant Time: Feb 17 05:37:14 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020623.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Feb 17 05:33:41 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.522	142	954733	34.577	ng/ul	96
39) 1,2,4,5-Tetrachloroben...	12.675	216	577019	33.356	ng/ul	96
40) Hexachlorocyclopentadiene	12.646	237	380723	30.374	ng/ul	97
41) 2,4,6-Trichlorophenol	12.916	196	377650	34.401	ng/ul	93
42) 2,4,5-Trichlorophenol	12.987	196	413632	34.794	ng/ul	99
43) 1,1'-Biphenyl	13.316	154	1311673	33.363	ng/ul	98
44) 2-Chloronaphthalene	13.357	162	1026665	33.593	ng/ul	99
45) 2-Nitroaniline	13.575	65	334678	38.367	ng/ul	98
47) Dimethylphthalate	13.951	163	1352794	35.586	ng/ul	100
48) 2,6-Dinitrotoluene	14.075	165	282181	37.977	ng/ul	98
50) Acenaphthylene	14.204	152	1574404	34.978	ng/ul	99
51) 3-Nitroaniline	14.404	138	282595	43.186	ng/ul	94
52) Acenaphthene	14.551	153	1085276	34.517	ng/ul	99
53) 2,4-Dinitrophenol	14.610	184	173166	34.661	ng/ul	95
55) 4-Nitrophenol	14.716	109	214344	36.890	ng/ul	95
56) Dibenzofuran	14.887	168	1548242	34.806	ng/ul	99
57) 2,4-Dinitrotoluene	14.863	165	398984	38.689	ng/ul	97
58) 2,3,4,6-Tetrachlorophenol	15.116	232	368584	35.646	ng/ul	98
59) Diethylphthalate	15.316	149	1306793	35.207	ng/ul	98
61) Fluorene	15.534	166	1267512	34.767	ng/ul	97
62) 4-Chlorophenyl-phenyle...	15.528	204	659249	34.370	ng/ul	96
63) 4-Nitroaniline	15.575	138	268345	47.862	ng/ul	97
66) 4,6-Dinitro-2-methylph...	15.628	198	256237	35.238	ng/ul	96
67) N-Nitrosodiphenylamine	15.745	169	1061375	34.031	ng/ul	98
68) 4-Bromophenyl-phenylether	16.428	248	431966	34.064	ng/ul	92
69) Hexachlorobenzene	16.539	284	503804	34.772	ng/ul	99
70) Atrazine	16.704	200	370381	30.399	ng/ul	97
71) Pentachlorophenol	16.886	266	302384	32.856	ng/ul	96
72) Phenanthrene	17.281	178	1966566	34.137	ng/ul	98
74) Anthracene	17.369	178	2009326	34.834	ng/ul	99
75) 1,2,3,4-Tetrachloroben...	13.281	216	570264	32.850	ng/ul	95
76) Pentachlorobenzene	14.804	250	557099	32.334	ng/ul	98
77) Carbazole	17.645	167	1755578	35.314	ng/ul	99
78) Di-n-butylphthalate	18.204	149	2183931	26.304	ng/ul	98
80) Fluoranthene	19.298	202	2326729	36.102	ng/ul	99
82) Pyrene	19.663	202	2386729	36.381	ng/ul	99
83) Butylbenzylphthalate	20.563	149	901777	35.086	ng/ul	99
84) 3,3'-Dichlorobenzidine	21.351	252	701999	33.189	ng/ul	97
85) Benzo(a)anthracene	21.410	228	2079329	33.371	ng/ul	98
86) Bis(2-ethylhexyl)phtha...	21.339	149	1239550	32.501	ng/ul	98
87) Chrysene	21.463	228	1995162	34.601	ng/ul	98
89) Di-n-octyl phthalate	22.257	149	1938678	35.220	ng/ul	100
90) Benzo(b)fluoranthene	23.080	252	1917598	36.557	ng/ul	98
91) Benzo(k)fluoranthene	23.127	252	1890097	37.818	ng/ul	97
93) Benzo(a)pyrene	23.698	252	1669170	37.481	ng/ul	96
94) Indeno(1,2,3-cd)pyrene	26.268	276	2025600	35.240	ng/ul	98
95) Dibenzo(a,h)anthracene	26.280	278	1702599	35.696	ng/ul	98
96) Benzo(g,h,i)perylene	27.027	276	1616870	34.781	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Feb 17 05:37:14 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020623.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Feb 17 05:33:41 2023
Response via : Initial Calibration









#2
 1,4-Dioxane
 Concen: 11.850 ng/uL
 RT: 3.258 min Scan# 29
 Delta R.T. 0.000 min
 Lab File: BN024056.D
 Acq: 16 Feb 2023 16:17




Instrument :
 BNA_N
 ClientSampleId :
 SLCS878


Tgt Ion: 88 Resp: 51649
 Ion Ratio Lower Upper
 88 100
 43 32.2 33.4 50.2#
 58 70.9 52.9 79.3

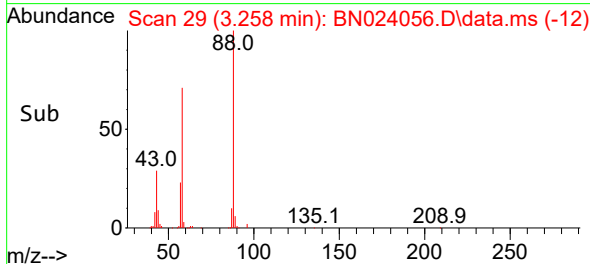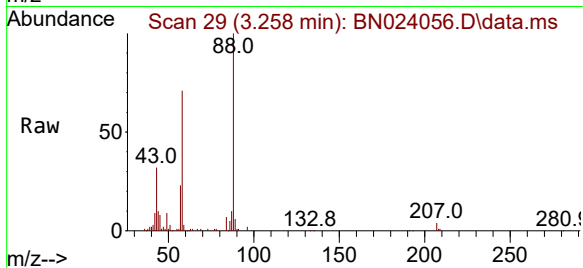

#5
 Pyridine
 Concen: 32.010 ng/uL
 RT: 3.664 min Scan# 98
 Delta R.T. -0.000 min
 Lab File: BN024056.D
 Acq: 16 Feb 2023 16:17

Tgt Ion: 79 Resp: 367864
 Ion Ratio Lower Upper
 79 100
 52 70.3 52.1 78.1
 51 34.9 26.0 39.0


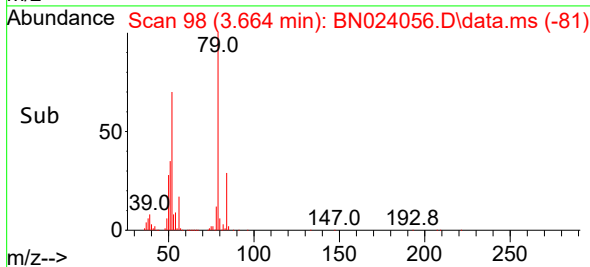

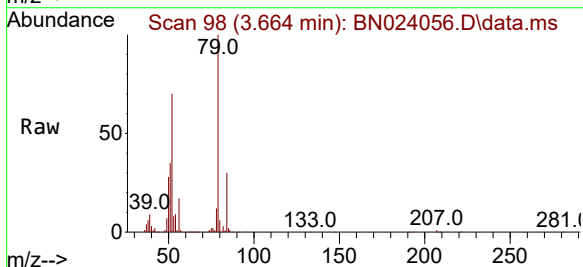




#6
Benzaldehyde
Concen: 49.283 ng/ul
RT: 6.969 min Scan# 660
Delta R.T. 0.000 min
Lab File: BN024056.D
Acq: 16 Feb 2023 16:17




Instrument :
BNA_N
ClientSampleId :
SLCS878


Tgt Ion: 77 Resp: 304177
Ion Ratio Lower Upper
77 100
105 88.9 71.3 106.9
106 85.6 71.1 106.7

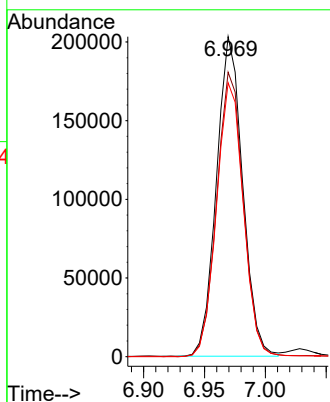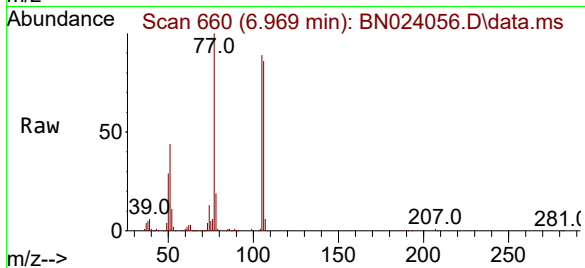

#8
Phenol
Concen: 36.975 ng/ul
RT: 7.028 min Scan# 670
Delta R.T. 0.006 min
Lab File: BN024056.D
Acq: 16 Feb 2023 16:17

Tgt Ion: 94 Resp: 531667
Ion Ratio Lower Upper
94 100
65 30.8 24.7 37.1
66 40.2 31.4 47.2

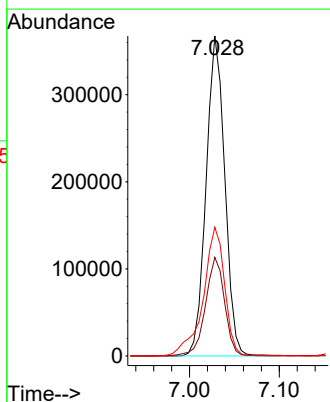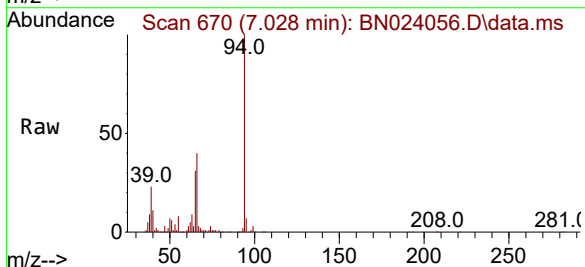







#10
 Bis(2-Chloroethyl)ether
 Concen: 36.372 ng/ul
 RT: 7.258 min Scan# 709
 Delta R.T. -0.000 min
 Lab File: BN024056.D
 Acq: 16 Feb 2023 16:17

Instrument :
 BNA_N
 ClientSampleId :
 SLCS878

Tgt Ion: 93 Resp: 425081




Ion	Ratio	Lower	Upper
93	100		
63	76.3	60.2	90.2
95	32.1	26.2	39.4

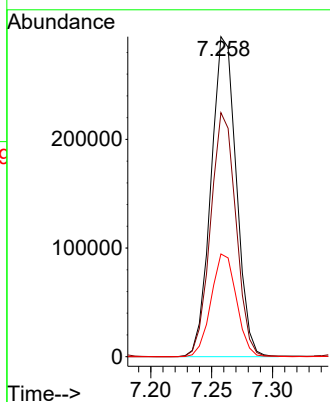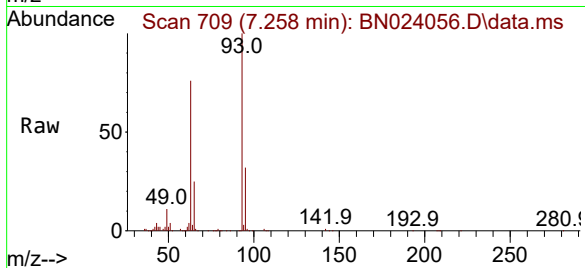


#12
 2-Chlorophenol
 Concen: 36.897 ng/ul
 RT: 7.393 min Scan# 732
 Delta R.T. 0.006 min
 Lab File: BN024056.D
 Acq: 16 Feb 2023 16:17

Tgt Ion:128 Resp: 415646

Ion	Ratio	Lower	Upper
128	100		
64	48.0	37.8	56.6
130	31.7	25.6	38.4

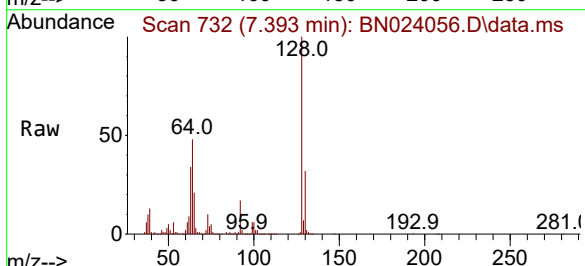



#13

2-Methylphenol

Concen: 37.064 ng/ul

RT: 8.281 min Scan# 883

Delta R.T. 0.000 min

Lab File: BN024056.D

Acq: 16 Feb 2023 16:17

Instrument :

BNA_N

ClientSampleId :





SLCS878

Tgt Ion:108 Resp: 399243

Ion Ratio Lower Upper

108 100

107 91.4 69.3 103.9

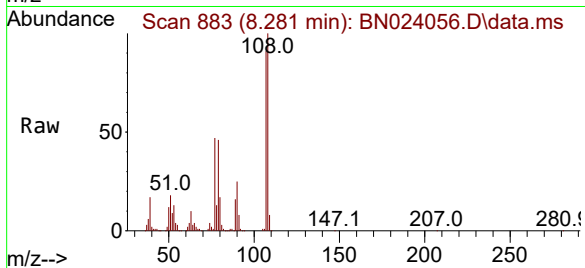

#14

2,2'-oxybis(1-Chloropropane)

Concen: 37.832 ng/ul

RT: 8.369 min Scan# 898

Delta R.T. 0.012 min

Lab File: BN024056.D

Acq: 16 Feb 2023 16:17




Tgt Ion: 45 Resp: 550799


Ion Ratio Lower Upper

45 100

77 16.1 12.8 19.2

79 12.3 9.9 14.9


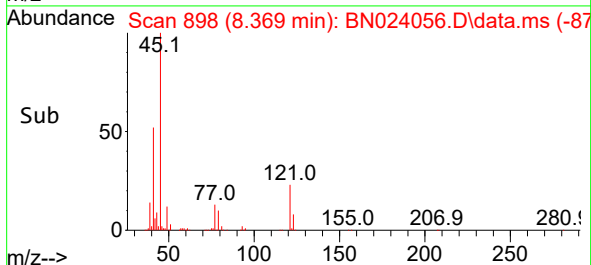
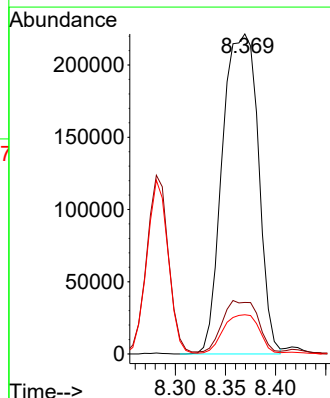
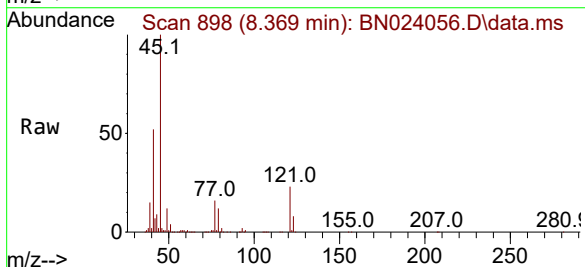




#16
Acetophenone
Concen: 37.897 ng/ul
RT: 8.663 min Scan# 947
Delta R.T. 0.006 min
Lab File: BN024056.D
Acq: 16 Feb 2023 16:17




Instrument :
BNA_N
ClientSampleId :
SLCS878


Tgt Ion:105 Resp: 657918
Ion Ratio Lower Upper
105 100
77 80.9 66.4 99.6
51 27.2 22.2 33.2



#17
N-Nitroso-di-n-propylamine
Concen: 39.413 ng/ul
RT: 8.657 min Scan# 947
Delta R.T. 0.012 min
Lab File: BN024056.D
Acq: 16 Feb 2023 16:17

Tgt Ion: 70 Resp: 367469
Ion Ratio Lower Upper
70 100
42 57.1 49.6 74.4
101 8.9 7.4 11.2
130 20.2 16.4 24.6









#18
4-Methylphenol
Concen: 38.393 ng/ul
RT: 8.616 min Scan# 940
Delta R.T. 0.006 min
Lab File: BN024056.D
Acq: 16 Feb 2023 16:17




Instrument :
BNA_N
ClientSampleId :
SLCS878


Tgt Ion:108 Resp: 445540
Ion Ratio Lower Upper
108 100
107 114.5 90.8 136.2

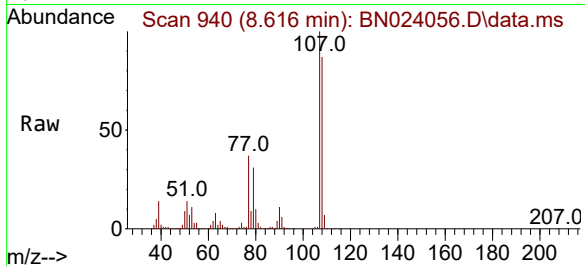

#19
Hexachloroethane
Concen: 37.961 ng/ul
RT: 8.905 min Scan# 989
Delta R.T. -0.000 min
Lab File: BN024056.D
Acq: 16 Feb 2023 16:17

Tgt Ion:117 Resp: 178680
Ion Ratio Lower Upper
117 100
201 101.3 92.7 139.1
199 62.2 50.4 75.6




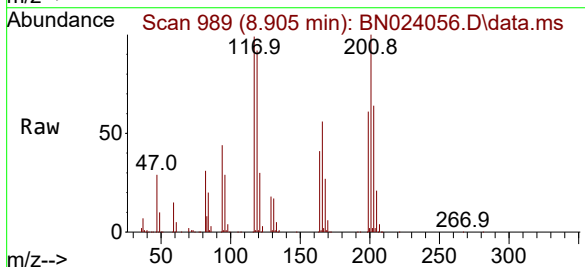




#22
Nitrobenzene
Concen: 35.288 ng/ul
RT: 9.046 min Scan# 1103
Delta R.T. 0.006 min
Lab File: BN024056.D
Acq: 16 Feb 2023 16:17




Instrument :
BNA_N
ClientSampleId :
SLCS878


Tgt Ion: 77 Resp: 537249
Ion Ratio Lower Upper
77 100
123 41.7 33.8 50.6
65 13.6 10.6 15.8



#23
Isophorone
Concen: 36.270 ng/ul
RT: 9.575 min Scan# 1103
Delta R.T. 0.006 min
Lab File: BN024056.D
Acq: 16 Feb 2023 16:17

Tgt Ion: 82 Resp: 1016150
Ion Ratio Lower Upper
82 100
95 7.1 6.0 9.0
138 16.3 13.6 20.4


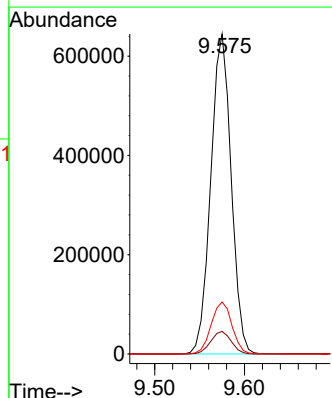






#25
2-Nitrophenol
Concen: 35.873 ng/ul
RT: 9.757 min Scan# 1134
Delta R.T. 0.006 min
Lab File: BN024056.D
Acq: 16 Feb 2023 16:17




Instrument :
BNA_N
ClientSampleId :
SLCS878


Tgt Ion:139 Resp: 252881
Ion Ratio Lower Upper
139 100
65 55.8 46.9 70.3
109 34.0 27.1 40.7

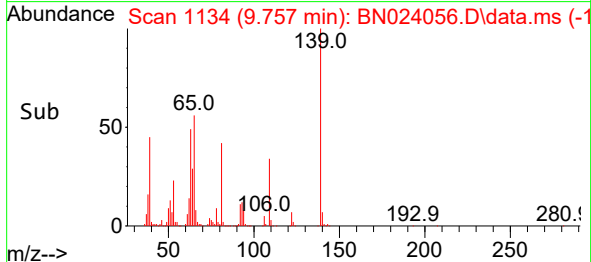

#26
2,4-Dimethylphenol
Concen: 35.337 ng/ul
RT: 9.822 min Scan# 1145
Delta R.T. 0.006 min
Lab File: BN024056.D
Acq: 16 Feb 2023 16:17

Tgt Ion:107 Resp: 496315
Ion Ratio Lower Upper
107 100
121 49.8 38.9 58.3
122 85.3 65.9 98.9

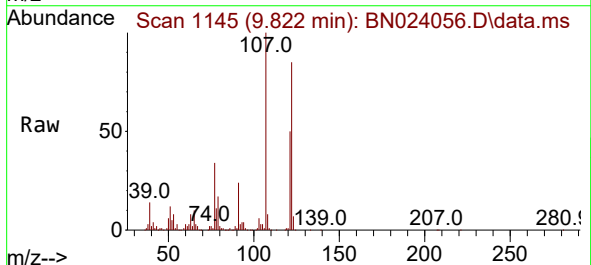



#27

Bis(2-Chloroethoxy)methane

Concen: 35.120 ng/ul

RT: 10.057 min Scan# 1184

Delta R.T. 0.006 min

Lab File: BN024056.D

Acq: 16 Feb 2023 16:17

Instrument :

BNA_N

ClientSampleId :

SLCS878





Tgt Ion: 93 Resp: 611172

Ion Ratio Lower Upper

93 100

95 30.5 25.9 38.9

123 10.5 8.9 13.3

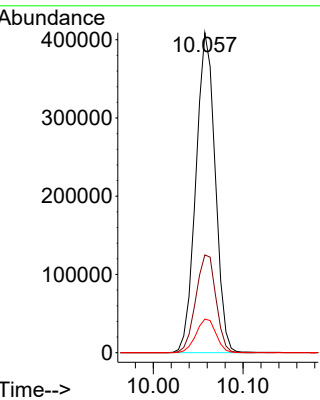

#29

2,4-Dichlorophenol

Concen: 35.385 ng/ul

RT: 10.287 min Scan# 1224

Delta R.T. -0.000 min

Lab File: BN024056.D

Acq: 16 Feb 2023 16:17




Tgt Ion:162 Resp: 430887


Ion Ratio Lower Upper

162 100

164 63.9 52.2 78.4

98 36.7 29.4 44.0

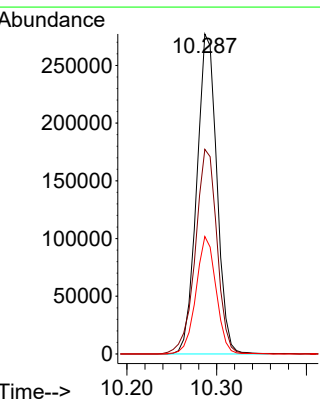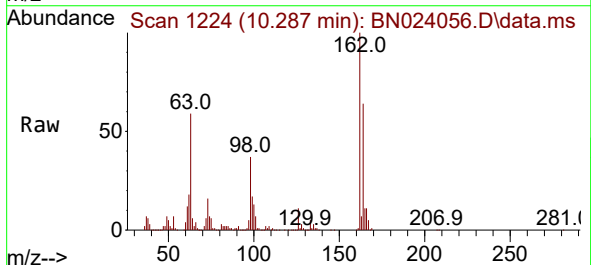



#30

Naphthalene

Concen: 34.026 ng/ul

RT: 10.687 min Scan# 1292

Delta R.T. -0.000 min

Lab File: BN024056.D

Acq: 16 Feb 2023 16:17

Instrument :

BNA_N

ClientSampleId :

SLCS878





Tgt Ion:128 Resp: 1371574

Ion Ratio Lower Upper

128 100

129 10.9 9.0 13.4

127 13.5 10.5 15.7

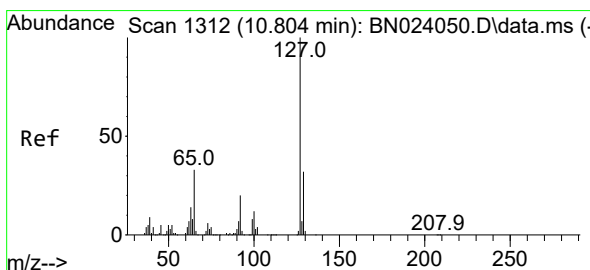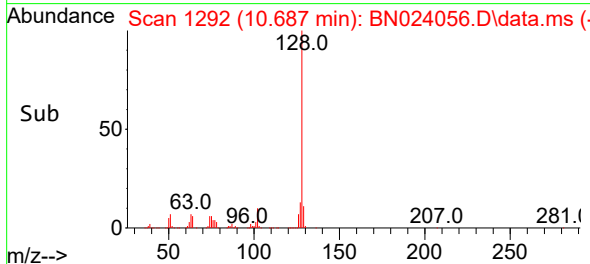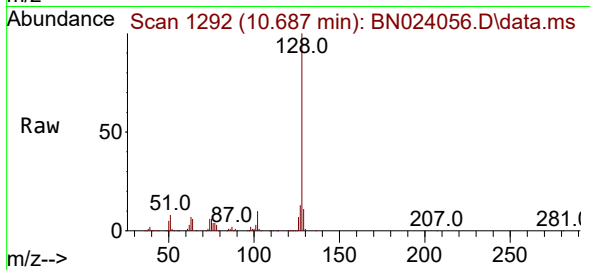

#32

4-Chloroaniline

Concen: 30.118 ng/ul

RT: 10.804 min Scan# 1312

Delta R.T. -0.000 min

Lab File: BN024056.D




Acq: 16 Feb 2023 16:17


Tgt Ion:127 Resp: 510234

Ion Ratio Lower Upper

127 100

129 29.9 25.8 38.6

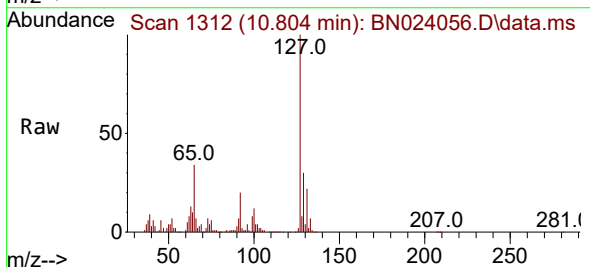



#33

Hexachlorobutadiene

Concen: 33.423 ng/ul

RT: 10.969 min Scan# 11

Delta R.T. -0.000 min

Lab File: BN024056.D

Acq: 16 Feb 2023 16:17

Instrument :

BNA_N

ClientSampleId :

SLCS878





Tgt Ion:225 Resp: 291855

Ion Ratio Lower Upper

225 100

223 63.8 49.0 73.4

227 64.4 50.1 75.1



#34

Caprolactam

Concen: 24.113 ng/ul

RT: 11.604 min Scan# 1448

Delta R.T. 0.018 min

Lab File: BN024056.D

Acq: 16 Feb 2023 16:17




Tgt Ion:113 Resp: 83498


Ion Ratio Lower Upper

113 100

55 156.3 132.3 198.5

56 119.1 103.3 154.9




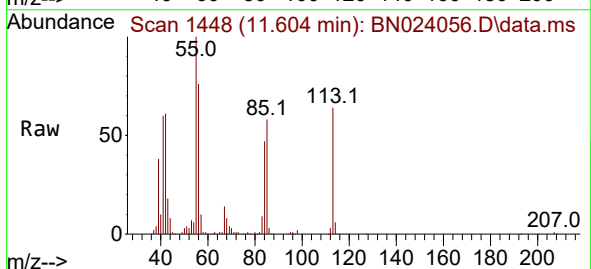




#35
 4-Chloro-3-methylphenol
 Concen: 37.495 ng/ul
 RT: 11.940 min Scan# 1505
 Delta R.T. 0.006 min
 Lab File: BN024056.D
 Acq: 16 Feb 2023 16:17




Instrument :
 BNA_N
 ClientSampleId :
 SLCS878


Tgt Ion:107 Resp: 479756
 Ion Ratio Lower Upper
 107 100
 144 26.2 20.6 30.8
 142 80.0 63.8 95.8



#36
 2-Methylnaphthalene
 Concen: 35.106 ng/ul
 RT: 12.304 min Scan# 1567
 Delta R.T. 0.006 min
 Lab File: BN024056.D
 Acq: 16 Feb 2023 16:17

Tgt Ion:142 Resp: 952781
 Ion Ratio Lower Upper
 142 100
 141 87.7 70.6 106.0


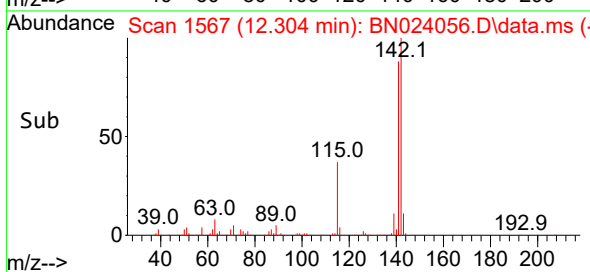

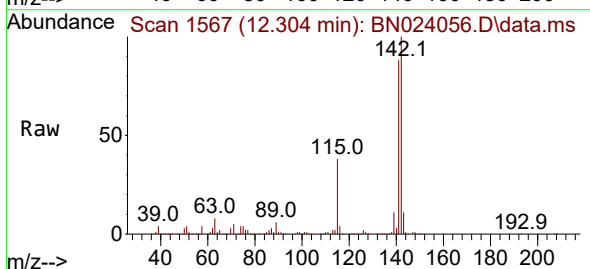




#37
1-Methylnaphthalene
Concen: 34.577 ng/ul
RT: 12.522 min Scan# 1604
Delta R.T. 0.000 min
Lab File: BN024056.D
Acq: 16 Feb 2023 16:17




Instrument :
BNA_N
ClientSampleId :
SLCS878


Tgt Ion:142 Resp: 954733
Ion Ratio Lower Upper
142 100
141 90.7 75.4 113.0
116 4.1 3.1 4.7

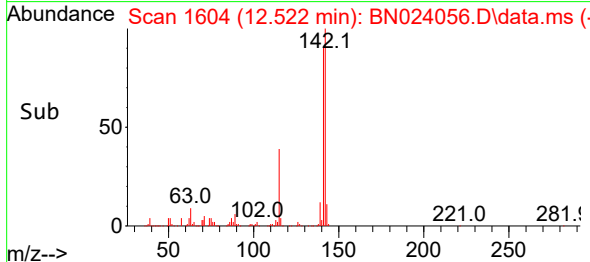

#39
1,2,4,5-Tetrachlorobenzene
Concen: 33.356 ng/ul
RT: 12.675 min Scan# 1630
Delta R.T. 0.006 min
Lab File: BN024056.D
Acq: 16 Feb 2023 16:17

Tgt Ion:216 Resp: 577019
Ion Ratio Lower Upper
216 100
214 71.6 60.5 90.7
179 19.2 16.0 24.0
108 16.0 13.8 20.8


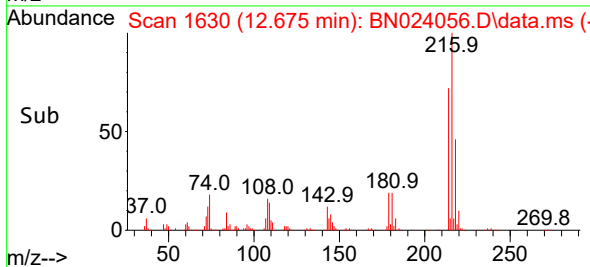

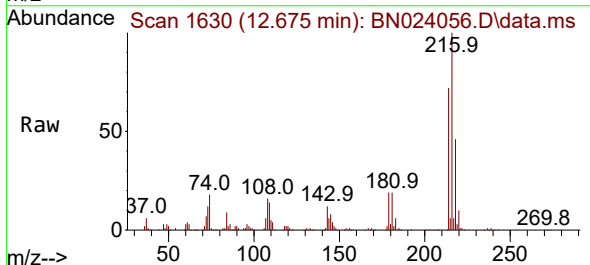




#40
Hexachlorocyclopentadiene
Concen: 30.374 ng/ul
RT: 12.646 min Scan# 1625
Delta R.T. -0.000 min
Lab File: BN024056.D
Acq: 16 Feb 2023 16:17




Instrument :
BNA_N
ClientSampleId :
SLCS878


Tgt Ion:237 Resp: 380723
Ion Ratio Lower Upper
237 100
235 62.2 52.0 78.0
272 13.1 10.1 15.1

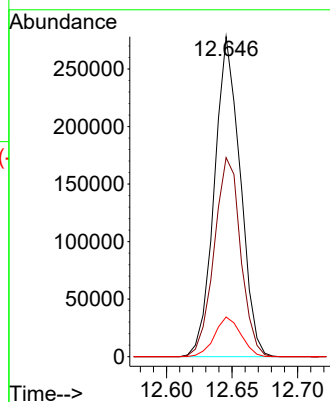

#41
2,4,6-Trichlorophenol
Concen: 34.401 ng/ul
RT: 12.916 min Scan# 1671
Delta R.T. 0.000 min
Lab File: BN024056.D
Acq: 16 Feb 2023 16:17

Tgt Ion:196 Resp: 377650
Ion Ratio Lower Upper
196 100
198 93.1 81.3 121.9
200 30.8 26.2 39.2









#42
2,4,5-Trichlorophenol
Concen: 34.794 ng/ul
RT: 12.987 min Scan# 1683
Delta R.T. 0.000 min
Lab File: BN024056.D
Acq: 16 Feb 2023 16:17




Instrument :
BNA_N
ClientSampleId :
SLCS878


Tgt Ion:196 Resp: 413632
Ion Ratio Lower Upper
196 100
198 96.1 76.0 114.0
200 30.9 24.0 36.0

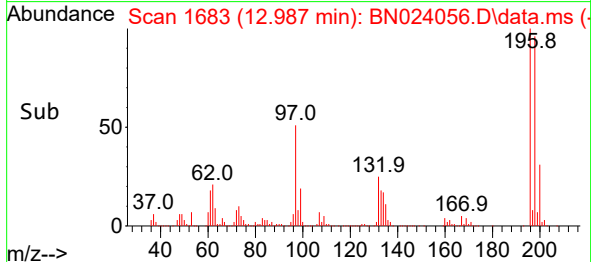

#43
1,1'-Biphenyl
Concen: 33.363 ng/ul
RT: 13.316 min Scan# 1739
Delta R.T. -0.000 min
Lab File: BN024056.D
Acq: 16 Feb 2023 16:17

Tgt Ion:154 Resp: 1311673
Ion Ratio Lower Upper
154 100
153 40.7 31.9 47.9
76 14.3 10.6 16.0




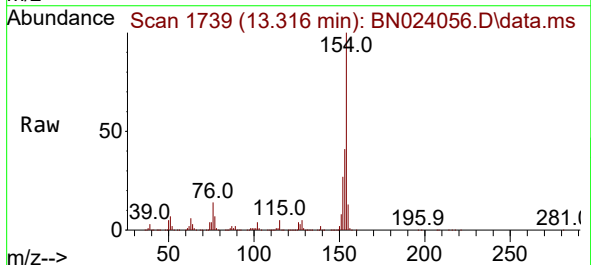


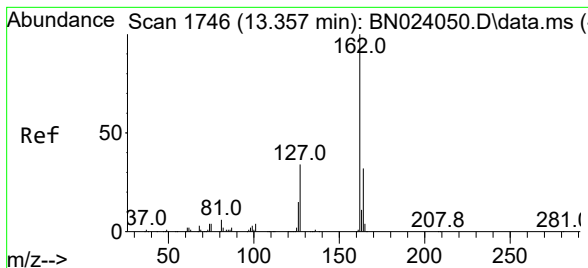

#44
2-Chloronaphthalene
Concen: 33.593 ng/ul
RT: 13.357 min Scan# 1746
Delta R.T. 0.000 min
Lab File: BN024056.D
Acq: 16 Feb 2023 16:17




Instrument :
BNA_N
ClientSampleId :
SLCS878


Tgt Ion:162 Resp: 1026665
Ion Ratio Lower Upper
162 100
164 32.4 26.4 39.6
127 38.4 30.6 45.8

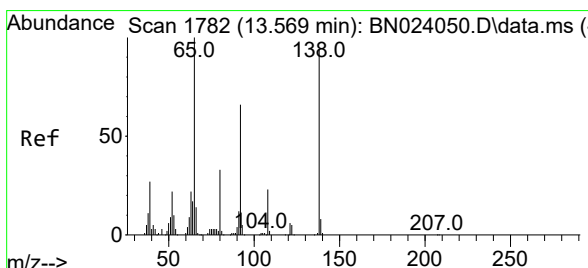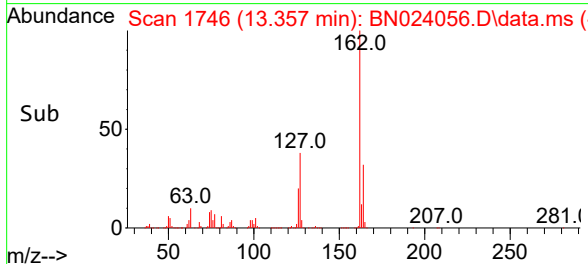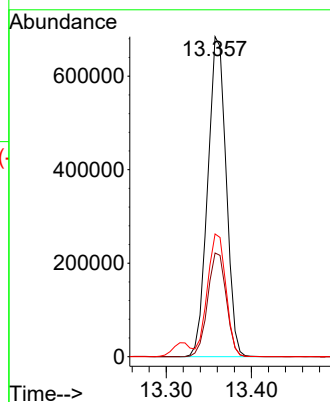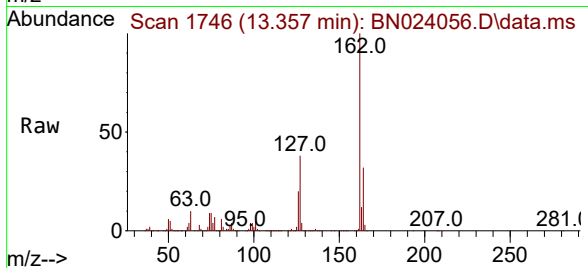

#45
2-Nitroaniline
Concen: 38.367 ng/ul
RT: 13.575 min Scan# 1783
Delta R.T. 0.006 min
Lab File: BN024056.D
Acq: 16 Feb 2023 16:17

Tgt Ion: 65 Resp: 334678
Ion Ratio Lower Upper
65 100
92 66.3 52.0 78.0
138 100.2 79.0 118.6

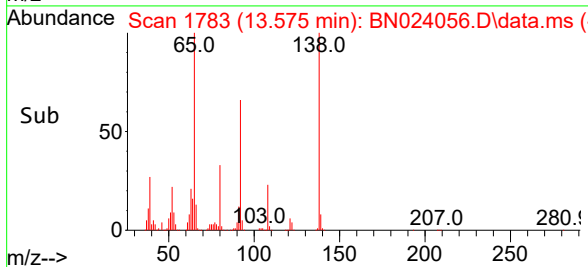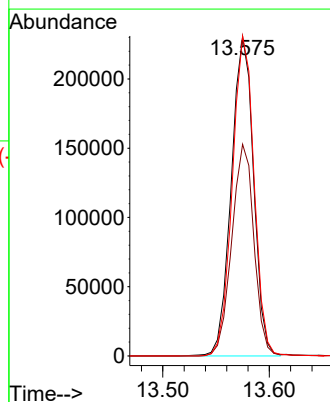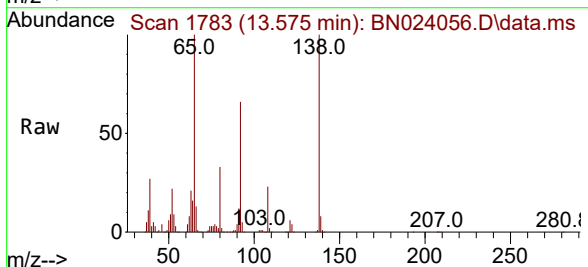



#47

Dimethylphthalate

Concen: 35.586 ng/ul

RT: 13.951 min Scan# 1847

Delta R.T. 0.006 min

Lab File: BN024056.D

Acq: 16 Feb 2023 16:17

Instrument :

BNA_N

ClientSampleId :

SLCS878





Tgt Ion:163 Resp: 1352794

Ion Ratio Lower Upper

163 100

194 4.4 3.5 5.3

164 10.0 7.8 11.8



#48

2,6-Dinitrotoluene

Concen: 37.977 ng/ul

RT: 14.075 min Scan# 1868

Delta R.T. 0.006 min

Lab File: BN024056.D

Acq: 16 Feb 2023 16:17




Tgt Ion:165 Resp: 282181


Ion Ratio Lower Upper

165 100

89 61.7 48.1 72.1

121 21.3 16.8 25.2






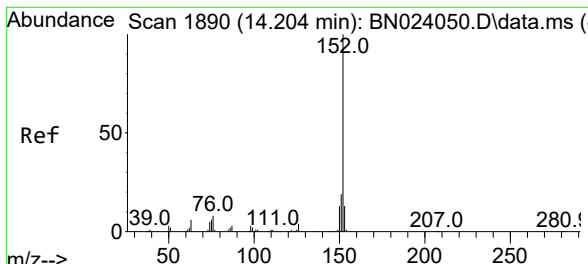


#50
 Acenaphthylene
 Concen: 34.978 ng/ul
 RT: 14.204 min Scan# 1890
 Delta R.T. 0.000 min
 Lab File: BN024056.D
 Acq: 16 Feb 2023 16:17

Instrument : BNA_N
 ClientSampleId : SLCS878

Tgt Ion:152 Resp: 1574404




Ion	Ratio	Lower	Upper
152	100		
151	19.5	15.3	22.9
153	13.2	10.6	16.0

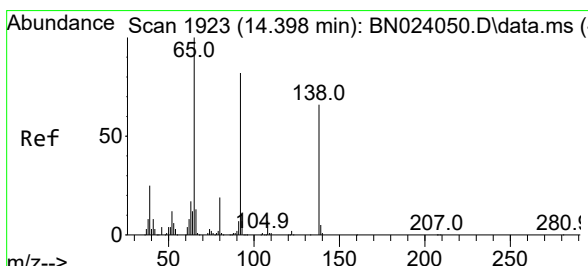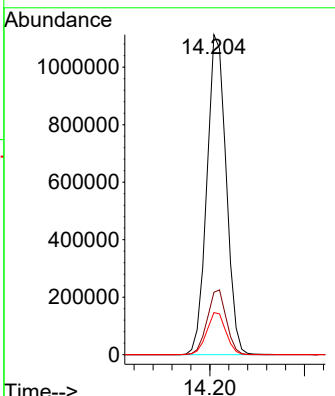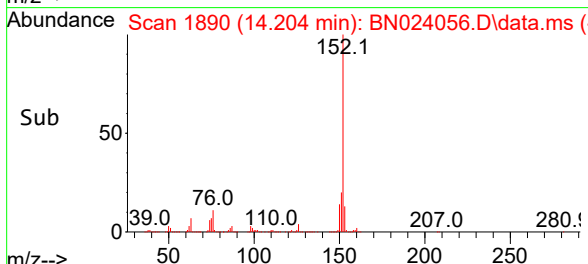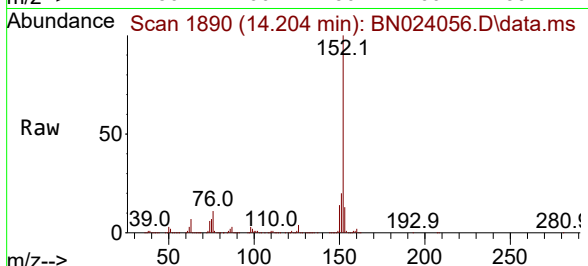


#51
 3-Nitroaniline
 Concen: 43.186 ng/ul
 RT: 14.404 min Scan# 1924
 Delta R.T. 0.006 min
 Lab File: BN024056.D
 Acq: 16 Feb 2023 16:17

Tgt Ion:138 Resp: 282595

Ion	Ratio	Lower	Upper
138	100		
108	10.1	8.2	12.4
92	122.6	92.6	138.8


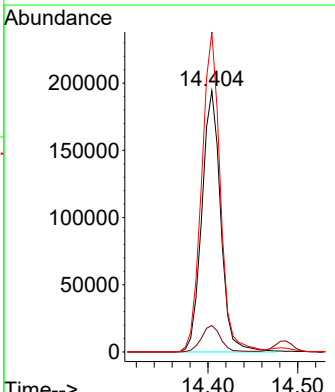
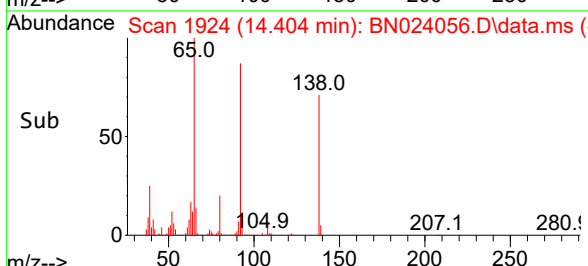
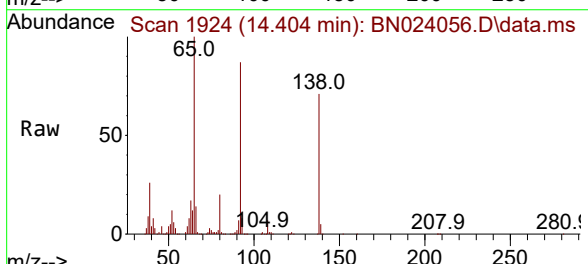




#52
Acenaphthene
Concen: 34.517 ng/ul
RT: 14.551 min Scan# 1949
Delta R.T. 0.006 min
Lab File: BN024056.D
Acq: 16 Feb 2023 16:17




Instrument :
BNA_N
ClientSampleId :
SLCS878


Tgt Ion:153 Resp: 1085276
Ion Ratio Lower Upper
153 100
152 48.1 37.4 56.2
154 90.1 71.5 107.3

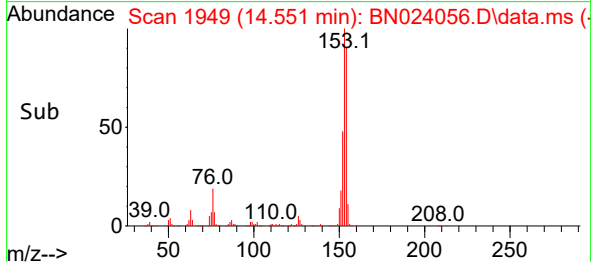

#53
2,4-Dinitrophenol
Concen: 34.661 ng/ul
RT: 14.610 min Scan# 1959
Delta R.T. 0.006 min
Lab File: BN024056.D
Acq: 16 Feb 2023 16:17

Tgt Ion:184 Resp: 173166
Ion Ratio Lower Upper
184 100
63 76.3 58.3 87.5
154 69.5 52.0 78.0









#55
4-Nitrophenol
Concen: 36.890 ng/ul
RT: 14.716 min Scan# 1976
Delta R.T. 0.006 min
Lab File: BN024056.D
Acq: 16 Feb 2023 16:17




Instrument :
BNA_N
ClientSampleId :
SLCS878


Tgt Ion:109 Resp: 214344
Ion Ratio Lower Upper
109 100
139 115.3 96.2 144.2
65 130.7 99.5 149.3



#56
Dibenzofuran
Concen: 34.806 ng/ul
RT: 14.887 min Scan# 2006
Delta R.T. 0.006 min
Lab File: BN024056.D
Acq: 16 Feb 2023 16:17

Tgt Ion:168 Resp: 1548242
Ion Ratio Lower Upper
168 100
139 37.1 30.2 45.2





#57

2,4-Dinitrotoluene

Concen: 38.689 ng/ul

RT: 14.863 min Scan# 2002

Delta R.T. 0.006 min

Lab File: BN024056.D

Acq: 16 Feb 2023 16:17

Instrument :

BNA_N

ClientSampleId :

SLCS878





Tgt Ion:165 Resp: 398984

Ion Ratio Lower Upper

165 100

63 49.6 37.8 56.8

182 2.9 2.2 3.2

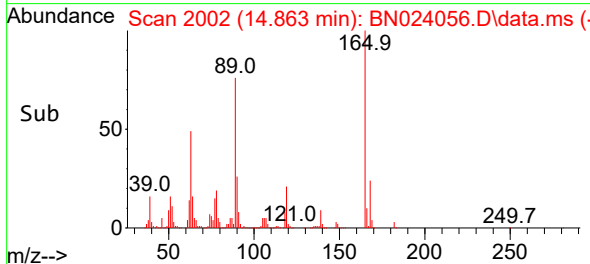

#58

2,3,4,6-Tetrachlorophenol

Concen: 35.646 ng/ul

RT: 15.116 min Scan# 2045

Delta R.T. 0.006 min

Lab File: BN024056.D

Acq: 16 Feb 2023 16:17

Tgt Ion:232 Resp: 368584




Ion Ratio Lower Upper


232 100

131 39.9 33.0 49.6

130 2.4 2.1 3.1

166 28.0 23.2 34.8

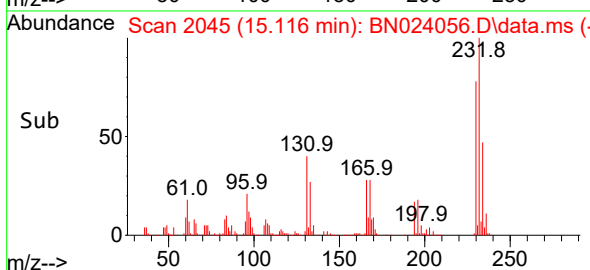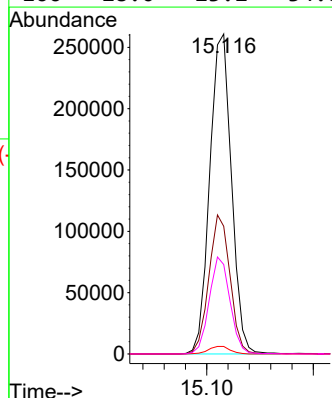

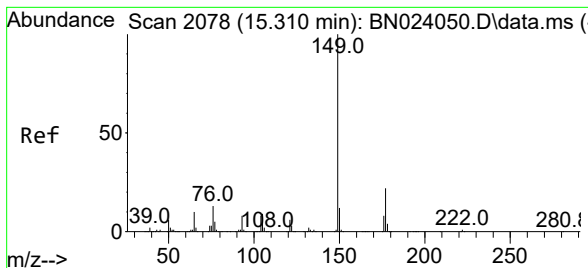

#59

Diethylphthalate

Concen: 35.207 ng/ul

RT: 15.316 min Scan# 2078

Delta R.T. 0.006 min

Lab File: BN024056.D

Acq: 16 Feb 2023 16:17

Instrument :

BNA_N

ClientSampleId :

SLCS878





Tgt Ion:149 Resp: 1306793

Ion Ratio Lower Upper

149 100

177 23.6 17.8 26.6

150 12.9 10.0 15.0

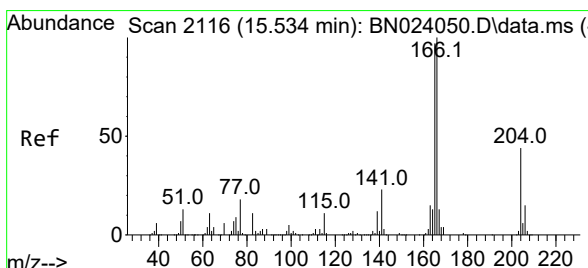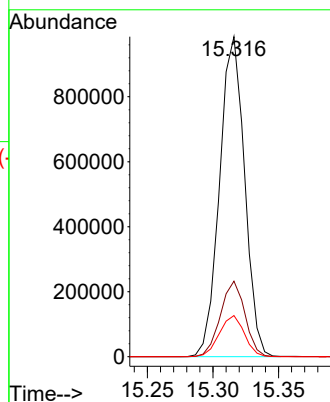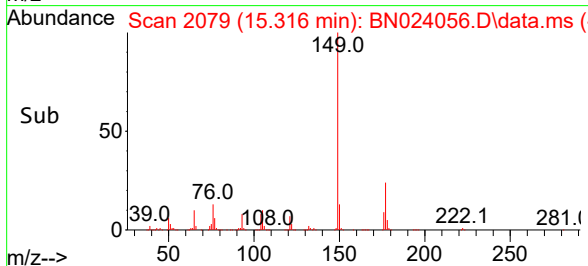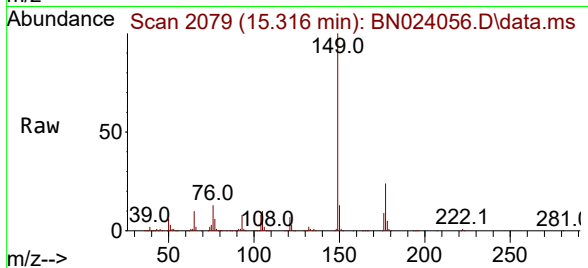

#61

Fluorene

Concen: 34.767 ng/ul

RT: 15.534 min Scan# 2116

Delta R.T. -0.000 min

Lab File: BN024056.D

Acq: 16 Feb 2023 16:17




Tgt Ion:166 Resp: 1267512


Ion Ratio Lower Upper

166 100

165 94.8 78.4 117.6

167 14.1 10.4 15.6


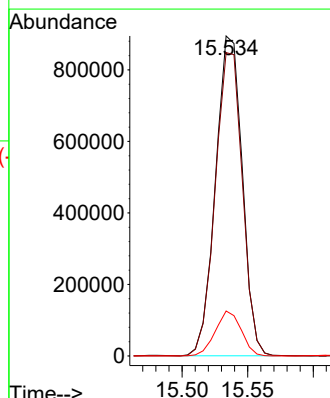
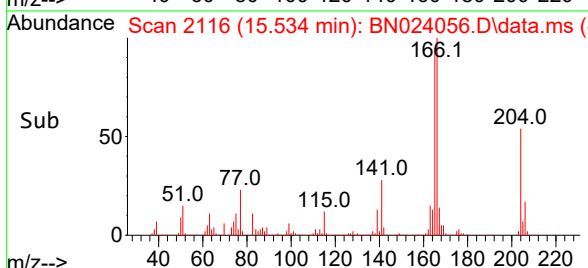
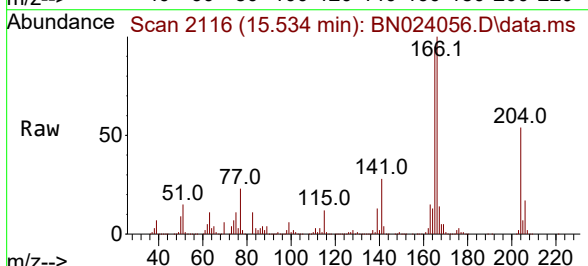




#62
4-Chlorophenyl-phenylether
Concen: 34.370 ng/ul
RT: 15.528 min Scan# 2115
Delta R.T. -0.000 min
Lab File: BN024056.D
Acq: 16 Feb 2023 16:17




Instrument :
BNA_N
ClientSampleId :
SLCS878


Tgt Ion:204 Resp: 659249
Ion Ratio Lower Upper
204 100
206 33.1 26.9 40.3
141 58.1 43.2 64.8

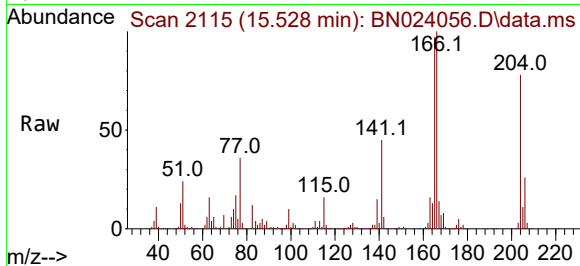

#63
4-Nitroaniline
Concen: 47.862 ng/ul
RT: 15.575 min Scan# 2123
Delta R.T. 0.012 min
Lab File: BN024056.D
Acq: 16 Feb 2023 16:17

Tgt Ion:138 Resp: 268345
Ion Ratio Lower Upper
138 100
92 51.8 42.5 63.7
108 92.1 70.6 105.8




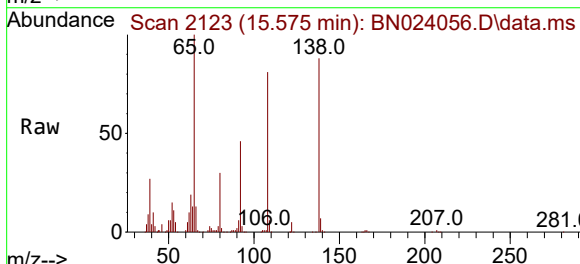




#66
4,6-Dinitro-2-methylphenol
Concen: 35.238 ng/ul
RT: 15.628 min Scan# 2131
Delta R.T. 0.006 min
Lab File: BN024056.D
Acq: 16 Feb 2023 16:17




Instrument :
BNA_N
ClientSampleId :
SLCS878


Tgt Ion:198 Resp: 256237
Ion Ratio Lower Upper
198 100
182 3.4 3.4 5.0
77 24.5 21.4 32.0

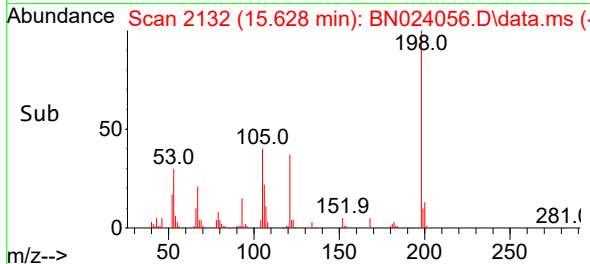

#67
N-Nitrosodiphenylamine
Concen: 34.031 ng/ul
RT: 15.745 min Scan# 2152
Delta R.T. -0.000 min
Lab File: BN024056.D
Acq: 16 Feb 2023 16:17

Tgt Ion:169 Resp: 1061375
Ion Ratio Lower Upper
169 100
168 65.4 54.2 81.2
167 36.3 28.7 43.1


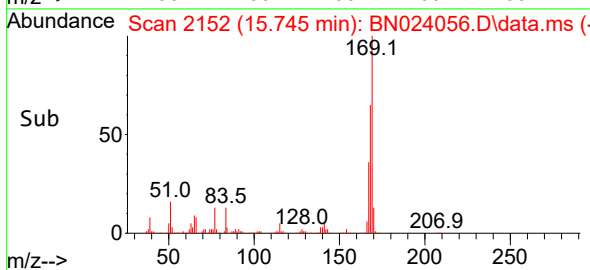

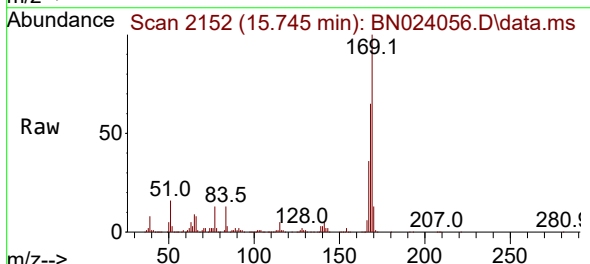




#68
4-Bromophenyl-phenylether
Concen: 34.064 ng/ul
RT: 16.428 min Scan# 21
Delta R.T. 0.006 min
Lab File: BN024056.D
Acq: 16 Feb 2023 16:17




Instrument :
BNA_N
ClientSampleId :
SLCS878


Tgt Ion:248 Resp: 431966
Ion Ratio Lower Upper
248 100
250 97.3 82.0 123.0
141 64.2 58.8 88.2



#69
Hexachlorobenzene
Concen: 34.772 ng/ul
RT: 16.539 min Scan# 2287
Delta R.T. 0.006 min
Lab File: BN024056.D
Acq: 16 Feb 2023 16:17

Tgt Ion:284 Resp: 503804
Ion Ratio Lower Upper
284 100
142 30.8 24.7 37.1
249 29.9 25.0 37.6

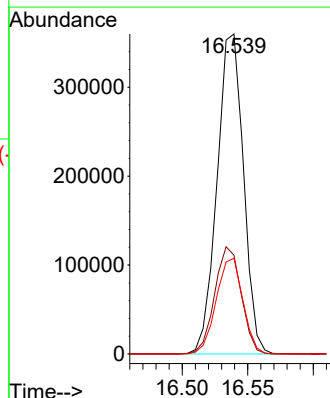



#70

Atrazine

Concen: 30.399 ng/ul

RT: 16.704 min Scan# 21

Delta R.T. 0.000 min

Lab File: BN024056.D

Acq: 16 Feb 2023 16:17

Instrument :

BNA_N

ClientSampleId :

SLCS878





Tgt Ion:200 Resp: 370381

Ion Ratio Lower Upper

200 100

173 24.8 20.3 30.5

215 49.1 41.0 61.6



#71

Pentachlorophenol

Concen: 32.856 ng/ul

RT: 16.886 min Scan# 2346

Delta R.T. 0.006 min

Lab File: BN024056.D

Acq: 16 Feb 2023 16:17




Tgt Ion:266 Resp: 302384


Ion Ratio Lower Upper

266 100

264 61.1 47.4 71.0

268 64.7 48.8 73.2





#72

Phenanthrene

Concen: 34.137 ng/ul

RT: 17.281 min Scan# 2413

Delta R.T. 0.006 min

Lab File: BN024056.D

Acq: 16 Feb 2023 16:17

Instrument :

BNA_N

ClientSampleId :

SLCS878





Tgt Ion:178 Resp: 1966566

Ion Ratio Lower Upper

178 100

179 15.4 13.6 20.4

176 19.2 15.8 23.6



#74

Anthracene

Concen: 34.834 ng/ul

RT: 17.369 min Scan# 2428

Delta R.T. -0.000 min

Lab File: BN024056.D

Acq: 16 Feb 2023 16:17




Tgt Ion:178 Resp: 2009326


Ion Ratio Lower Upper

178 100

179 15.0 12.1 18.1

176 18.4 14.4 21.6





#75

1,2,3,4-Tetrachlorobenzene

Concen: 32.850 ng/uL

RT: 13.281 min Scan# 11

Delta R.T. 0.000 min

Lab File: BN024056.D

Acq: 16 Feb 2023 16:17

Instrument :

BNA_N

ClientSampleId :

SLCS878





Tgt Ion:216 Resp: 570264

Ion Ratio Lower Upper

216 100

214 82.8 61.2 91.8

218 49.5 39.8 59.6



#76

Pentachlorobenzene

Concen: 32.334 ng/uL

RT: 14.804 min Scan# 1992

Delta R.T. 0.006 min

Lab File: BN024056.D

Acq: 16 Feb 2023 16:17




Tgt Ion:250 Resp: 557099


Ion Ratio Lower Upper

250 100

248 66.2 50.7 76.1

252 64.9 51.5 77.3

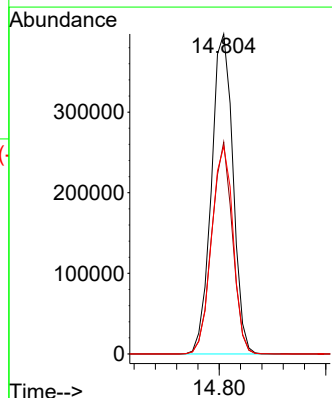







#77
 Carbazole
 Concen: 35.314 ng/ul
 RT: 17.645 min Scan# 2475
 Delta R.T. -0.000 min
 Lab File: BN024056.D
 Acq: 16 Feb 2023 16:17

Instrument :
 BNA_N
 ClientSampleId :
 SLCS878

Tgt Ion:167 Resp: 1755578




Ion	Ratio	Lower	Upper
167	100		
166	20.8	17.1	25.7
139	12.8	10.3	15.5

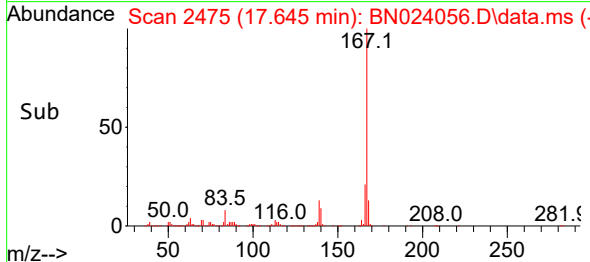


#78
 Di-n-butylphthalate
 Concen: 26.304 ng/ul
 RT: 18.204 min Scan# 2570
 Delta R.T. -0.000 min
 Lab File: BN024056.D
 Acq: 16 Feb 2023 16:17

Tgt Ion:149 Resp: 2183931

Ion	Ratio	Lower	Upper
149	100		
150	9.5	7.0	10.6
104	5.9	4.2	6.2

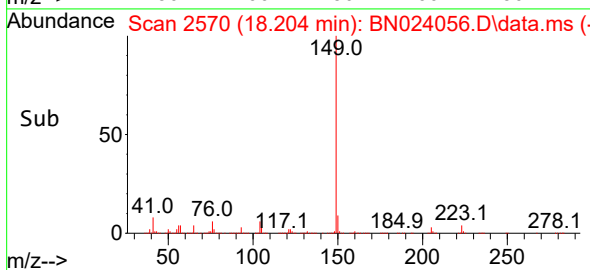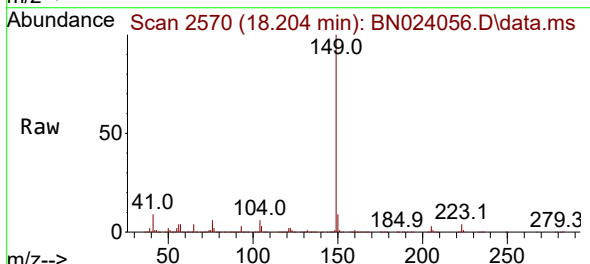



#80

Fluoranthene

Concen: 36.102 ng/ul

RT: 19.298 min Scan# 21

Delta R.T. 0.006 min

Lab File: BN024056.D

Acq: 16 Feb 2023 16:17

Instrument :

BNA_N

ClientSampleId :

SLCS878





Tgt Ion:202 Resp: 2326729

Ion Ratio Lower Upper

202 100

101 9.9 7.8 11.6

100 7.6 5.8 8.8



#82

Pyrene

Concen: 36.381 ng/ul

RT: 19.663 min Scan# 2818

Delta R.T. 0.006 min

Lab File: BN024056.D

Acq: 16 Feb 2023 16:17




Tgt Ion:202 Resp: 2386729


Ion Ratio Lower Upper

202 100

101 11.4 9.3 13.9

100 9.2 7.6 11.4

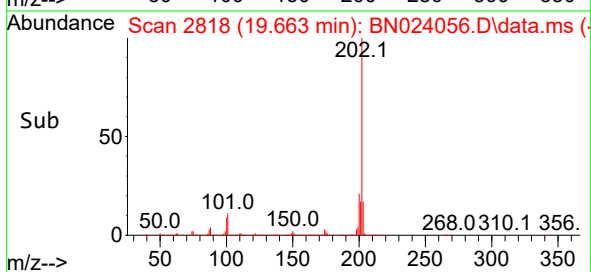



#83

Butylbenzylphthalate

Concen: 35.086 ng/ul

RT: 20.563 min Scan# 2971

Delta R.T. 0.000 min

Lab File: BN024056.D

Acq: 16 Feb 2023 16:17

Instrument :

BNA_N

ClientSampleId :

SLCS878





Tgt Ion:149 Resp: 901777

Ion Ratio Lower Upper

149 100

91 74.3 59.5 89.3

206 22.1 18.8 28.2

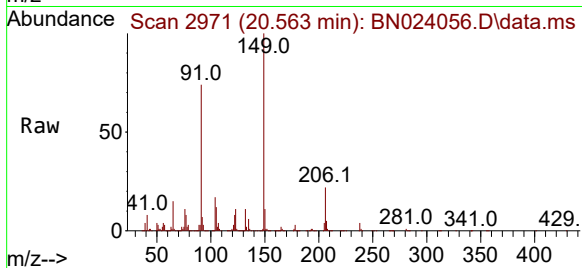

#84

3,3'-Dichlorobenzidine

Concen: 33.189 ng/ul

RT: 21.351 min Scan# 3105

Delta R.T. 0.006 min

Lab File: BN024056.D

Acq: 16 Feb 2023 16:17




Tgt Ion:252 Resp: 701999


Ion Ratio Lower Upper

252 100

254 57.5 48.4 72.6

126 9.3 7.4 11.0

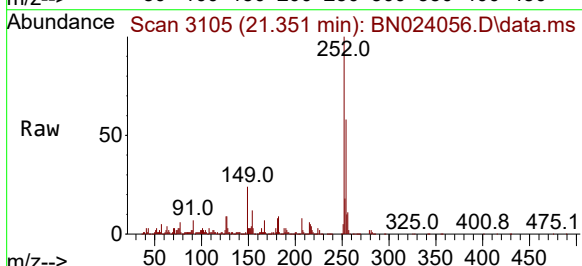



#85

Benzo(a)anthracene

Concen: 33.371 ng/ul

RT: 21.410 min Scan# 3115

Delta R.T. 0.000 min

Lab File: BN024056.D

Acq: 16 Feb 2023 16:17

Instrument :

BNA_N

ClientSampleId :

SLCS878





Tgt Ion:228 Resp: 2079329

Ion Ratio Lower Upper

228 100

229 19.9 15.8 23.6

226 28.6 21.3 31.9



#86

Bis(2-ethylhexyl)phthalate

Concen: 32.501 ng/ul

RT: 21.339 min Scan# 3103

Delta R.T. 0.006 min

Lab File: BN024056.D

Acq: 16 Feb 2023 16:17




Tgt Ion:149 Resp: 1239550


Ion Ratio Lower Upper

149 100

167 27.2 22.7 34.1

279 4.6 3.9 5.9


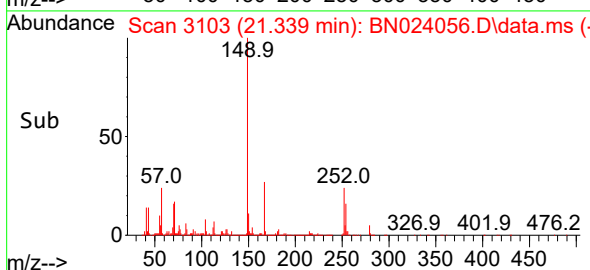






#87
Chrysene
Concen: 34.601 ng/ul
RT: 21.463 min Scan# 3124
Delta R.T. -0.000 min
Lab File: BN024056.D
Acq: 16 Feb 2023 16:17




Instrument :
BNA_N
ClientSampleId :
SLCS878


Tgt Ion:228 Resp: 1995162
Ion Ratio Lower Upper
228 100
226 29.1 24.5 36.7
229 19.7 15.6 23.4

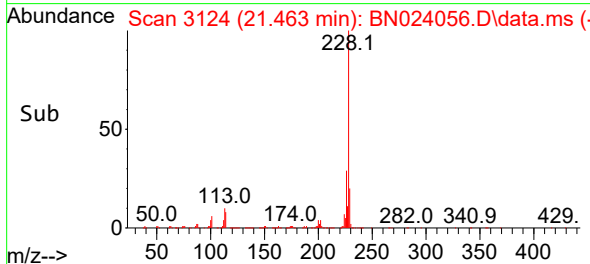

#89
Di-n-octyl phthalate
Concen: 35.220 ng/ul
RT: 22.257 min Scan# 3259
Delta R.T. 0.000 min
Lab File: BN024056.D
Acq: 16 Feb 2023 16:17

Tgt Ion:149 Resp: 1938678

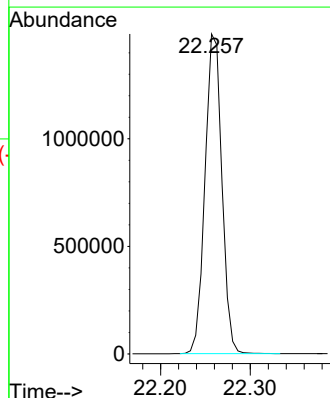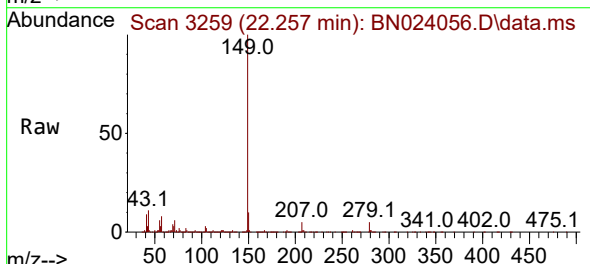



#90

Benzo(b)fluoranthene

Concen: 36.557 ng/ul

RT: 23.080 min Scan# 3399

Delta R.T. 0.000 min

Lab File: BN024056.D

Acq: 16 Feb 2023 16:17

Instrument :

BNA_N

ClientSampleId :

SLCS878





Tgt Ion:252 Resp: 1917598

Ion Ratio Lower Upper

252 100

253 21.9 16.4 24.6

125 8.8 6.8 10.2

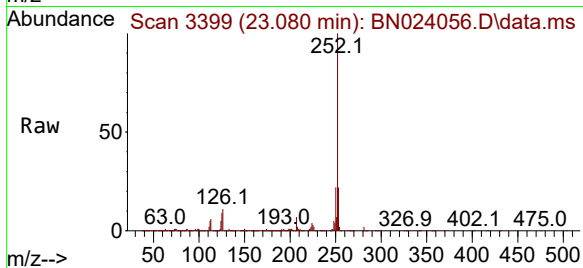

#91

Benzo(k)fluoranthene

Concen: 37.818 ng/ul

RT: 23.127 min Scan# 3407

Delta R.T. -0.000 min

Lab File: BN024056.D

Acq: 16 Feb 2023 16:17




Tgt Ion:252 Resp: 1890097


Ion Ratio Lower Upper

252 100

253 21.9 19.3 28.9

125 9.3 7.2 10.8

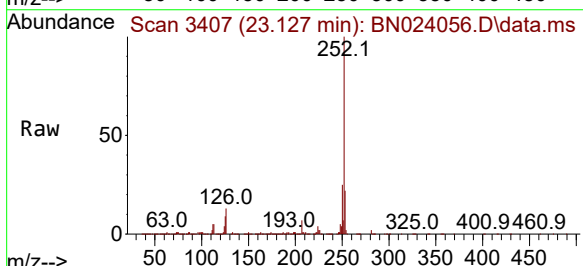



#93

Benzo(a)pyrene

Concen: 37.481 ng/ul

RT: 23.698 min Scan# 3

Delta R.T. 0.006 min

Lab File: BN024056.D

Acq: 16 Feb 2023 16:17

Instrument :

BNA_N

ClientSampleId :

SLCS878





Tgt Ion:252 Resp: 1669170

Ion Ratio Lower Upper

252 100

253 19.9 17.6 26.4

125 9.4 7.1 10.7



#94

Indeno(1,2,3-cd)pyrene

Concen: 35.240 ng/ul

RT: 26.268 min Scan# 3941

Delta R.T. 0.018 min

Lab File: BN024056.D

Acq: 16 Feb 2023 16:17




Tgt Ion:276 Resp: 2025600


Ion Ratio Lower Upper

276 100

138 21.0 16.4 24.6

277 24.3 20.6 30.8





#95

Dibenzo(a,h)anthracene

Concen: 35.696 ng/ul

RT: 26.280 min Scan# 3943

Delta R.T. 0.000 min

Lab File: BN024056.D

Acq: 16 Feb 2023 16:17

Instrument :

BNA_N

ClientSampleId :

SLCS878





Tgt Ion:278 Resp: 1702599

Ion Ratio Lower Upper

278 100

139 14.8 11.6 17.4

279 23.3 19.9 29.9



#96

Benzo(g,h,i)perylene

Concen: 34.781 ng/ul

RT: 27.027 min Scan# 4070

Delta R.T. 0.018 min

Lab File: BN024056.D

Acq: 16 Feb 2023 16:17

Tgt Ion:276 Resp: 1616870

Ion Ratio Lower Upper

276 100

138 18.2 15.4 23.2

277 22.0 17.8 26.8

