
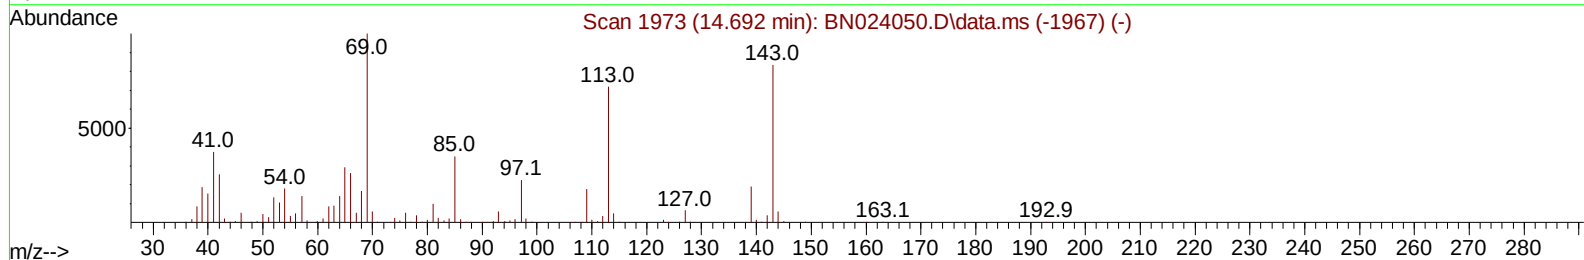
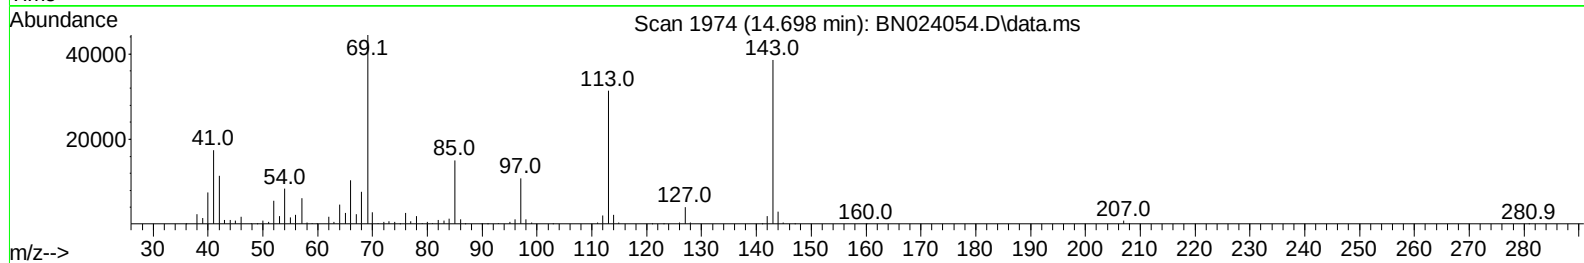


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021623\
Data File : BN024054.D
Acq On : 16 Feb 2023 15:01
Operator : CG/JU
Sample : 01534-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Quant Time: Feb 17 05:36:35 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020623.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Feb 17 05:33:41 2023
Response via : Initial Calibration

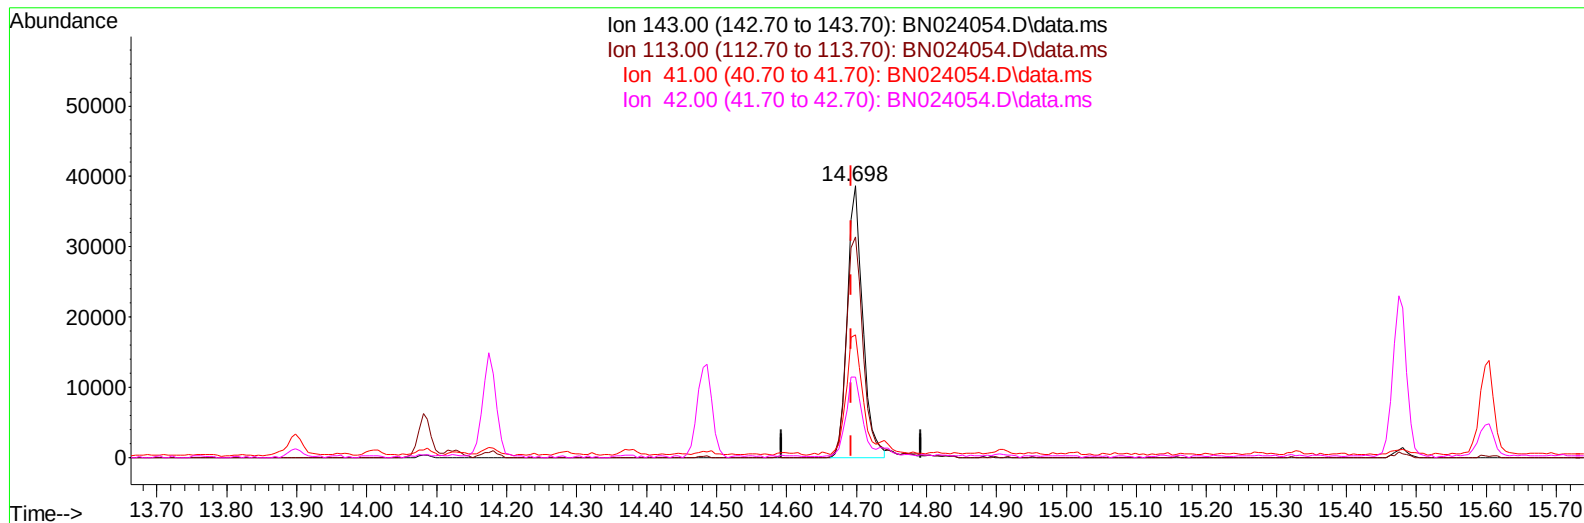

TIC: BN024054.D\data.ms

(54) 4-Nitrophenol-d4 (S)




14.698min (+ 0.006) 9.26 ng/ul

response 58830

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	80.30	81.26
41.00	44.70	45.27
42.00	29.50	29.58

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021623\
Data File : BN024054.D
Acq On : 16 Feb 2023 15:01
Operator : CG/JU
Sample : 01534-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Quant Time: Feb 17 05:36:35 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020623.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Feb 17 05:33:41 2023
Response via : Initial Calibration

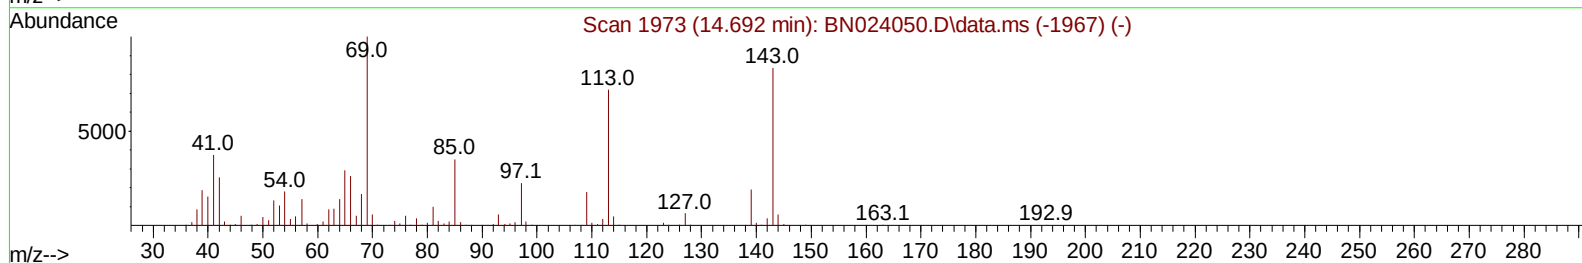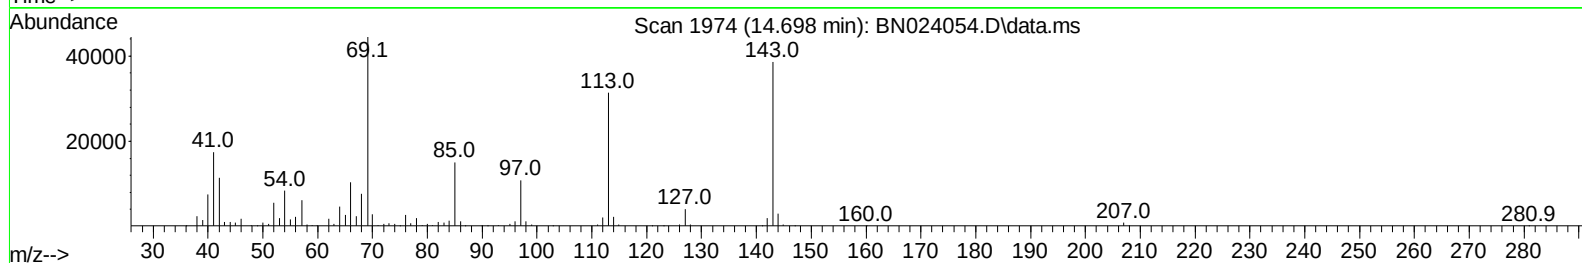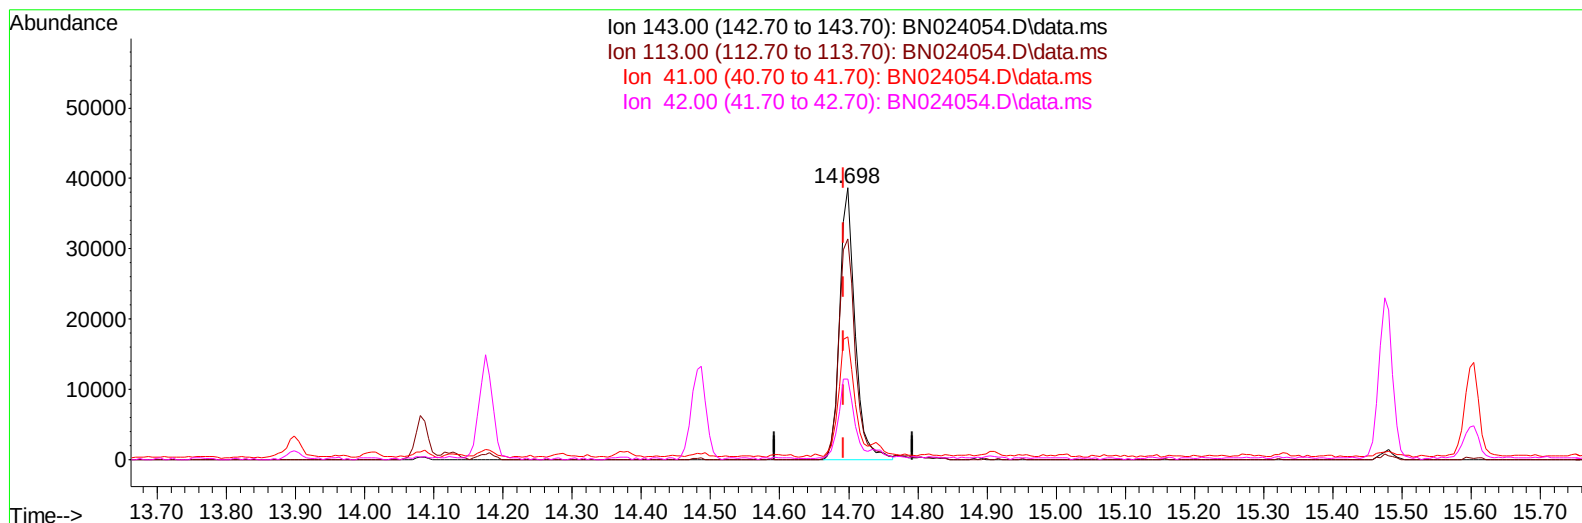

TIC: BN024054.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.698min (+ 0.006) 9.42 ng/ul m

response 59847

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	80.30	81.26
41.00	44.70	45.27
42.00	29.50	29.58

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021623\
 Data File : BN024054.D
 Acq On : 16 Feb 2023 15:01
 Operator : CG/JU
 Sample : 01534-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Quant Time: Feb 17 05:36:35 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020623.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Feb 17 05:33:41 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.828	152	166351	20.000	ng/ul	0.00
20) Naphthalene-d8	10.634	136	726272	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.486	164	477820	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.233	188	1129406	20.000	ng/ul	0.00
79) Chrysene-d12	21.427	240	1057395	20.000	ng/ul	0.00
88) Perylene-d12	23.810	264	1069991	20.000	ng/ul	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.222	96	22045	5.359	ng/uL	0.00
4) Pyridine-d5	3.652	84	127329	11.158	ng/ul	0.00
7) Phenol-d5	6.999	99	138770	9.758	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.163	67	277280	30.898	ng/ul	0.00
11) 2-Chlorophenol-d4	7.357	132	286464	25.900	ng/ul	0.00
15) 4-Methylphenol-d8	8.546	113	218608	19.677	ng/ul	0.00
21) Nitrobenzene-d5	8.999	128	169561	29.245	ng/ul	0.00
24) 2-Nitrophenol-d4	9.722	143	178884	27.477	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.257	165	321824	26.527	ng/ul	0.00
31) 4-Chloroaniline-d4	10.781	131	376842	22.983	ng/ul	0.00
46) Dimethylphthalate-d6	13.898	166	1162282	31.472	ng/ul	0.00
49) Acenaphthylene-d8	14.175	160	1238852	30.280	ng/ul	0.00
54) 4-Nitrophenol-d4	14.698	143	59847m	9.421	ng/ul	0.00
60) Fluorene-d10	15.481	176	1012936	32.576	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.604	200	207002	26.528	ng/ul	0.00
73) Anthracene-d10	17.333	188	1756603	34.143	ng/ul	0.00
81) Pyrene-d10	19.627	212	2205424	34.625	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.662	264	1935686	35.361	ng/ul	0.02
Target Compounds						
78) Di-n-butylphthalate	18.204	149	337387	3.894	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021623\
Data File : BN024054.D
Acq On : 16 Feb 2023 15:01
Operator : CG/JU
Sample : 01534-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Quant Time: Feb 17 05:36:35 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020623.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Feb 17 05:33:41 2023
Response via : Initial Calibration

