

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021623\
 Data File : BN024054.D
 Acq On : 16 Feb 2023 15:01
 Operator : CG/JU
 Sample : 01534-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0B47

Quant Time: Feb 17 05:36:35 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020623.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Feb 17 05:33:41 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.828	152	166351	20.000	ng/u1	0.00
20) Naphthalene-d8	10.634	136	726272	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.486	164	477820	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.233	188	1129406	20.000	ng/u1	0.00
79) Chrysene-d12	21.427	240	1057395	20.000	ng/u1	0.00
88) Perylene-d12	23.810	264	1069991	20.000	ng/u1	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.222	96	22045	5.359	ng/uL	0.00
4) Pyridine-d5	3.652	84	127329	11.158	ng/u1	0.00
7) Phenol-d5	6.999	99	138770	9.758	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.163	67	277280	30.898	ng/u1	0.00
11) 2-Chlorophenol-d4	7.357	132	286464	25.900	ng/u1	0.00
15) 4-Methylphenol-d8	8.546	113	218608	19.677	ng/u1	0.00
21) Nitrobenzene-d5	8.999	128	169561	29.245	ng/u1	0.00
24) 2-Nitrophenol-d4	9.722	143	178884	27.477	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.257	165	321824	26.527	ng/u1	0.00
31) 4-Chloroaniline-d4	10.781	131	376842	22.983	ng/u1	0.00
46) Dimethylphthalate-d6	13.898	166	1162282	31.472	ng/u1	0.00
49) Acenaphthylene-d8	14.175	160	1238852	30.280	ng/u1	0.00
54) 4-Nitrophenol-d4	14.698	143	59847m	9.421	ng/u1	0.00
60) Fluorene-d10	15.481	176	1012936	32.576	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.604	200	207002	26.528	ng/u1	0.00
73) Anthracene-d10	17.333	188	1756603	34.143	ng/u1	0.00
81) Pyrene-d10	19.627	212	2205424	34.625	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.662	264	1935686	35.361	ng/u1	0.02
Target Compounds						
78) Di-n-butylphthalate	18.204	149	337387	3.894	ng/u1	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021623\
Data File : BN024054.D
Acq On : 16 Feb 2023 15:01
Operator : CG/JU
Sample : 01534-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0B47

Quant Time: Feb 17 05:36:35 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020623.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Feb 17 05:33:41 2023
Response via : Initial Calibration

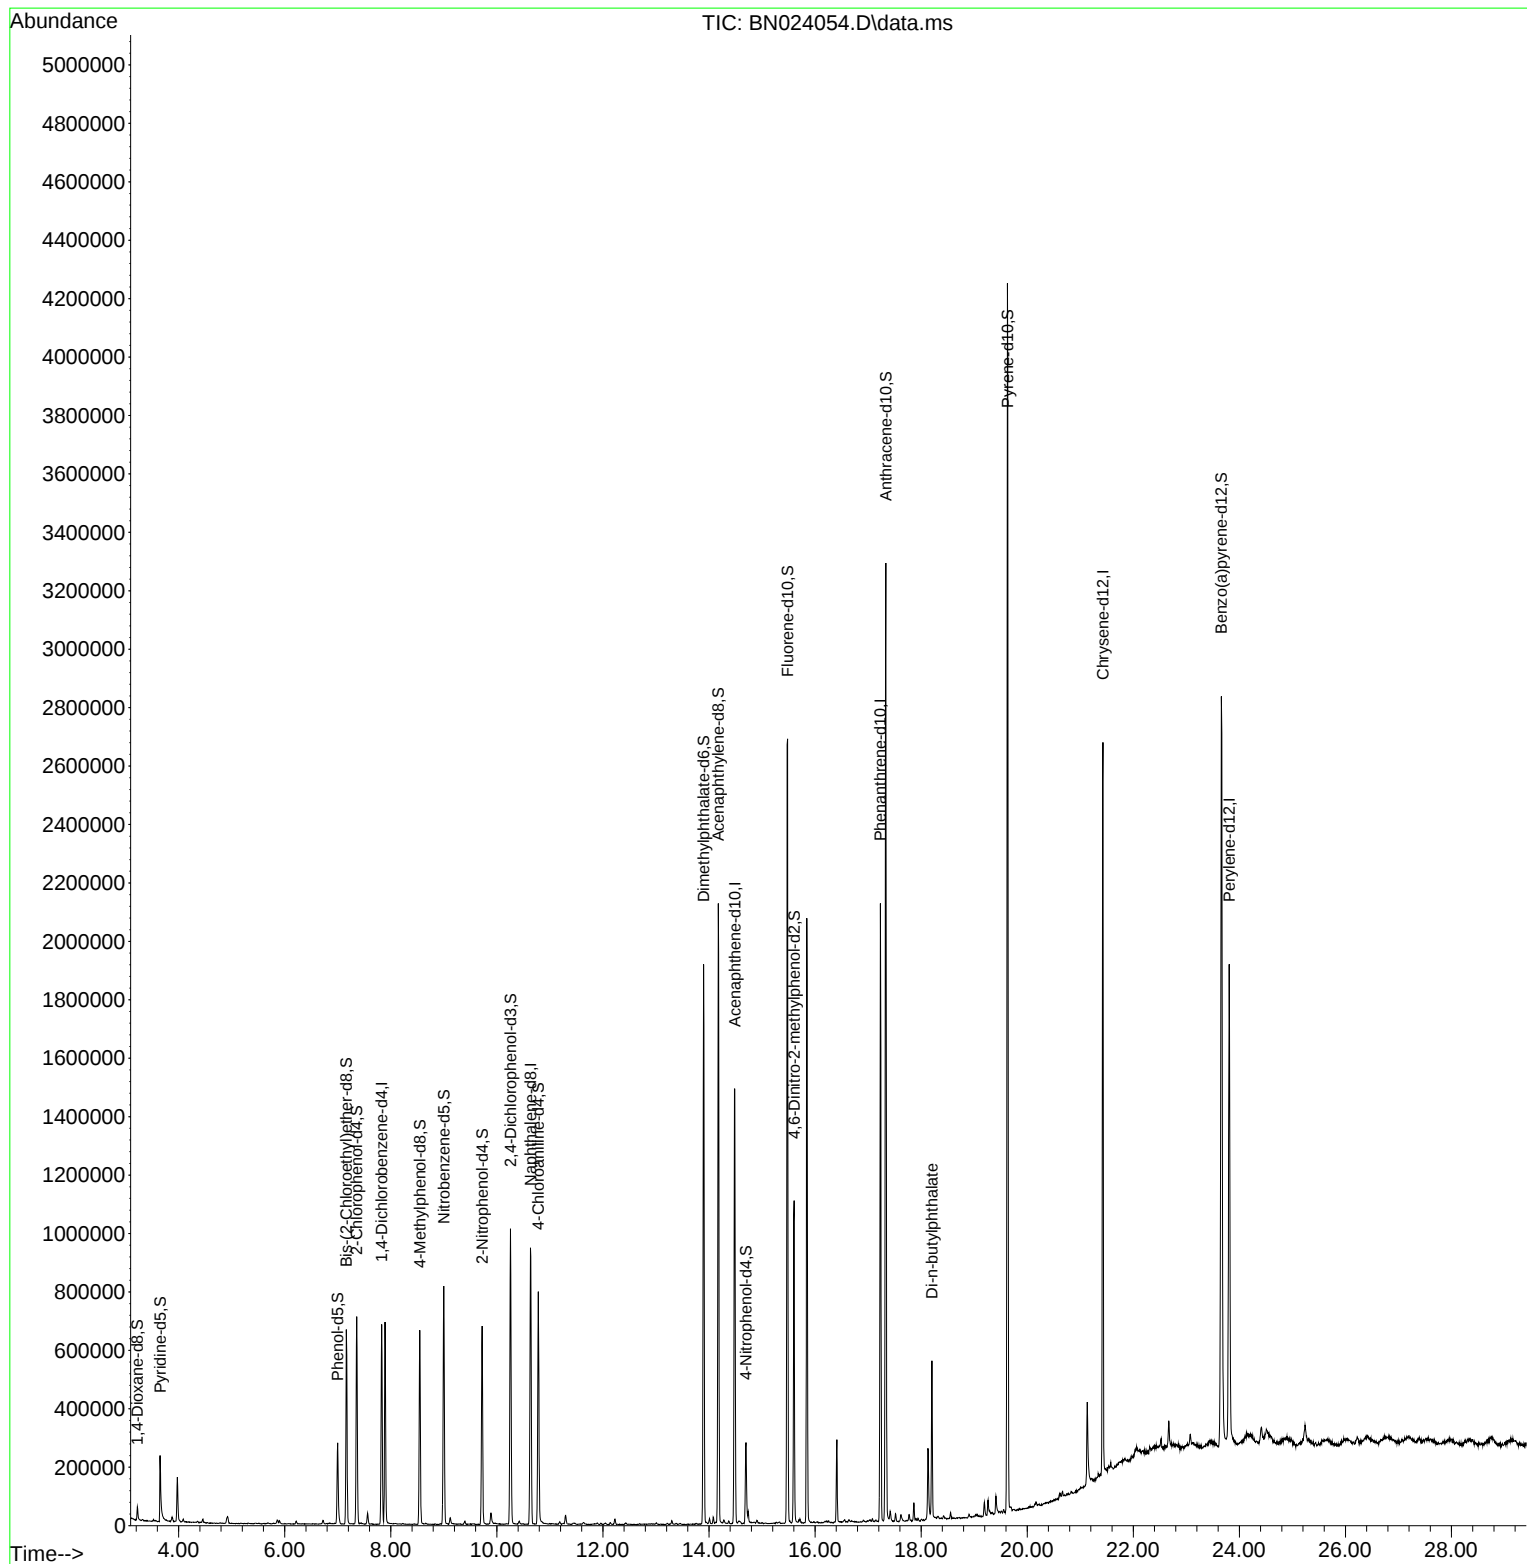

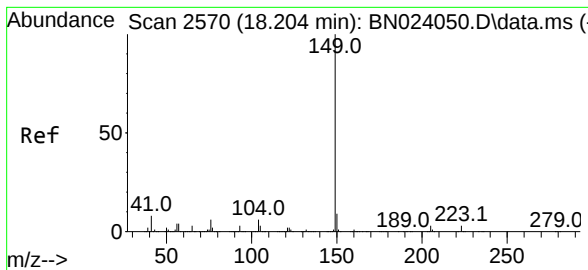

#78
 Di-n-butylphthalate
 Concen: 3.894 ng/ul
 RT: 18.204 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: BN024054.D
 Acq: 16 Feb 2023 15:01

Instrument :
 BNA_N
 ClientSampleId :
 C0B47

Tgt Ion:149 Resp: 337387
 Ion Ratio Lower Upper
 149 100
 150 8.6 7.0 10.6
 104 6.1 4.2 6.2

