

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN021623\  
 Data File : BN024051.D  
 Acq On : 16 Feb 2023 13:08  
 Operator : CG/JU  
 Sample : PB150871BL  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 SBLK871

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\SFAM-EPA-BN020623.M  
 Title : SVOA CALIBRATION

Signal : TIC: BN024051.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 3.223       | 20            | 23          | 33           | rVB      | 42999          | 58856         | 1.37%           | 0.133%        |
| 2         | 3.646       | 92            | 95          | 117          | rBV      | 497158         | 776742        | 18.13%          | 1.754%        |
| 3         | 3.975       | 148           | 151         | 157          | rVB      | 11135          | 16788         | 0.39%           | 0.038%        |
| 4         | 6.999       | 659           | 665         | 676          | rBV      | 704208         | 1081659       | 25.25%          | 2.443%        |
| 5         | 7.163       | 687           | 693         | 702          | rBV      | 595753         | 880347        | 20.55%          | 1.988%        |
| 6         | 7.358       | 719           | 726         | 735          | rBV      | 749643         | 1122256       | 26.19%          | 2.535%        |
| 7         | 7.828       | 799           | 806         | 813          | rBV      | 635533         | 969173        | 22.62%          | 2.189%        |
| 8         | 8.546       | 921           | 928         | 941          | rBV      | 884820         | 1355247       | 31.63%          | 3.061%        |
| 9         | 8.999       | 997           | 1005        | 1018         | rBV      | 711139         | 1107990       | 25.86%          | 2.503%        |
| 10        | 9.722       | 1120          | 1128        | 1141         | rBV      | 598526         | 953997        | 22.27%          | 2.155%        |
| 11        | 10.257      | 1212          | 1219        | 1231         | rBV      | 912529         | 1444101       | 33.71%          | 3.262%        |
| 12        | 10.634      | 1275          | 1283        | 1293         | rBV      | 885890         | 1449449       | 33.83%          | 3.274%        |
| 13        | 10.781      | 1301          | 1308        | 1324         | rBV      | 873208         | 1441914       | 33.66%          | 3.257%        |
| 14        | 12.228      | 1549          | 1554        | 1562         | rVB2     | 13520          | 20934         | 0.49%           | 0.047%        |
| 15        | 13.381      | 1745          | 1750        | 1755         | rVB6     | 3186           | 5083          | 0.12%           | 0.011%        |
| 16        | 13.898      | 1830          | 1838        | 1850         | rBV      | 1702275        | 2218987       | 51.79%          | 5.012%        |
| 17        | 14.175      | 1878          | 1885        | 1896         | rBV      | 1813722        | 2500597       | 58.37%          | 5.648%        |
| 18        | 14.481      | 1930          | 1937        | 1946         | rBV      | 1417072        | 2025016       | 47.27%          | 4.574%        |
| 19        | 14.692      | 1966          | 1973        | 1994         | rBV      | 760366         | 1112379       | 25.96%          | 2.513%        |
| 20        | 15.475      | 2098          | 2106        | 2121         | rBV      | 2251043        | 3231399       | 75.42%          | 7.299%        |
| 21        | 15.598      | 2121          | 2127        | 2140         | rVV      | 829204         | 1093958       | 25.53%          | 2.471%        |
| 22        | 15.716      | 2143          | 2147        | 2152         | rVB      | 11171          | 12466         | 0.29%           | 0.028%        |
| 23        | 17.234      | 2398          | 2405        | 2414         | rBV      | 1884457        | 2521518       | 58.85%          | 5.695%        |
| 24        | 17.334      | 2415          | 2422        | 2437         | rVV      | 2626316        | 3580816       | 83.58%          | 8.088%        |
| 25        | 19.192      | 2734          | 2738        | 2744         | rVB      | 31222          | 41652         | 0.97%           | 0.094%        |
| 26        | 19.263      | 2746          | 2750        | 2756         | rVV      | 26800          | 36753         | 0.86%           | 0.083%        |
| 27        | 19.628      | 2806          | 2812        | 2827         | rBV      | 3378944        | 4284322       | 100.00%         | 9.677%        |
| 28        | 21.422      | 3112          | 3117        | 3125         | rBV      | 2203849        | 2669819       | 62.32%          | 6.030%        |
| 29        | 23.657      | 3489          | 3497        | 3512         | rVB2     | 1788448        | 3805515       | 88.82%          | 8.596%        |
| 30        | 23.816      | 3517          | 3524        | 3533         | rVV      | 1345404        | 2453175       | 57.26%          | 5.541%        |




Sum of corrected areas: 44272908

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN021623\  
Data File : BN024051.D  
Acq On : 16 Feb 2023 13:08  
Operator : CG/JU  
Sample : PB150871BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
SBLK871

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\SFAM-EPA-BN020623.M  
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

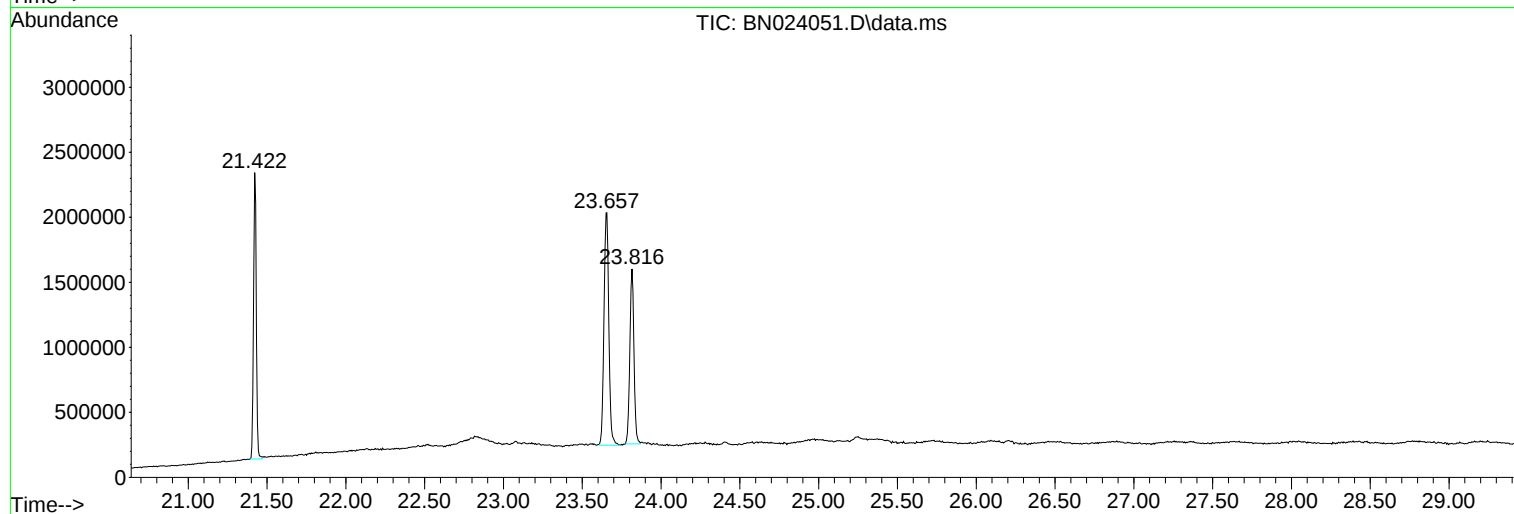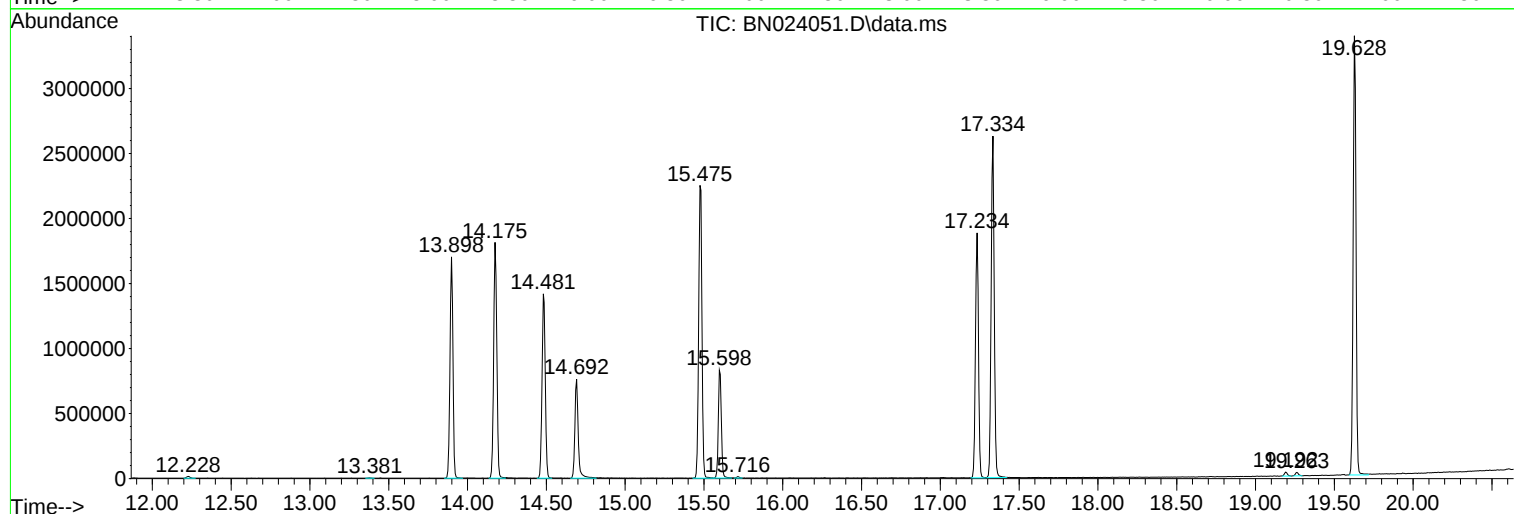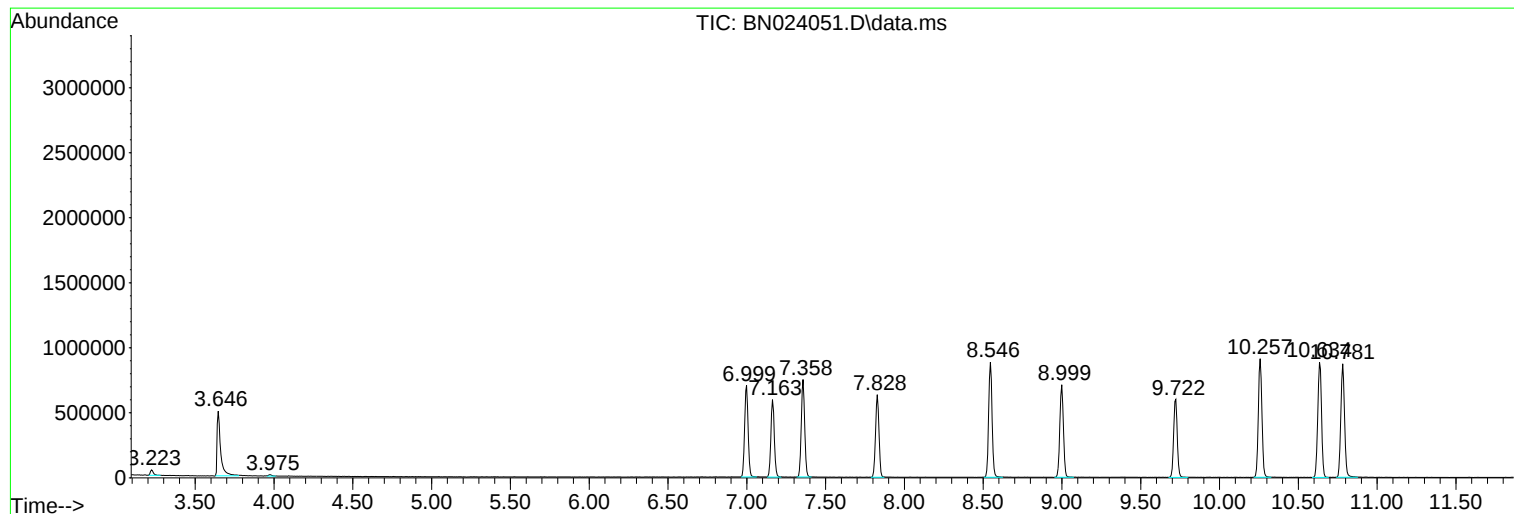

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN021623\  
Data File : BN024051.D  
Acq On : 16 Feb 2023 13:08  
Operator : CG/JU  
Sample : PB150871BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
SBLK871

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\SFAM-EPA-BN020623.M  
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN021623\  
Data File : BN024051.D  
Acq On : 16 Feb 2023 13:08  
Operator : CG/JU  
Sample : PB150871BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
SBLK871

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\SFAM-EPA-BN020623.M  
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |
|------------------|----|---------|-------|----------|-----------------------|
|                  |    |         |       | #        | RT Resp Conc          |