


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021624\
Data File : BN029826.D
Acq On : 16 Feb 2024 14:12
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN012924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Feb 16 23:52:05 2024

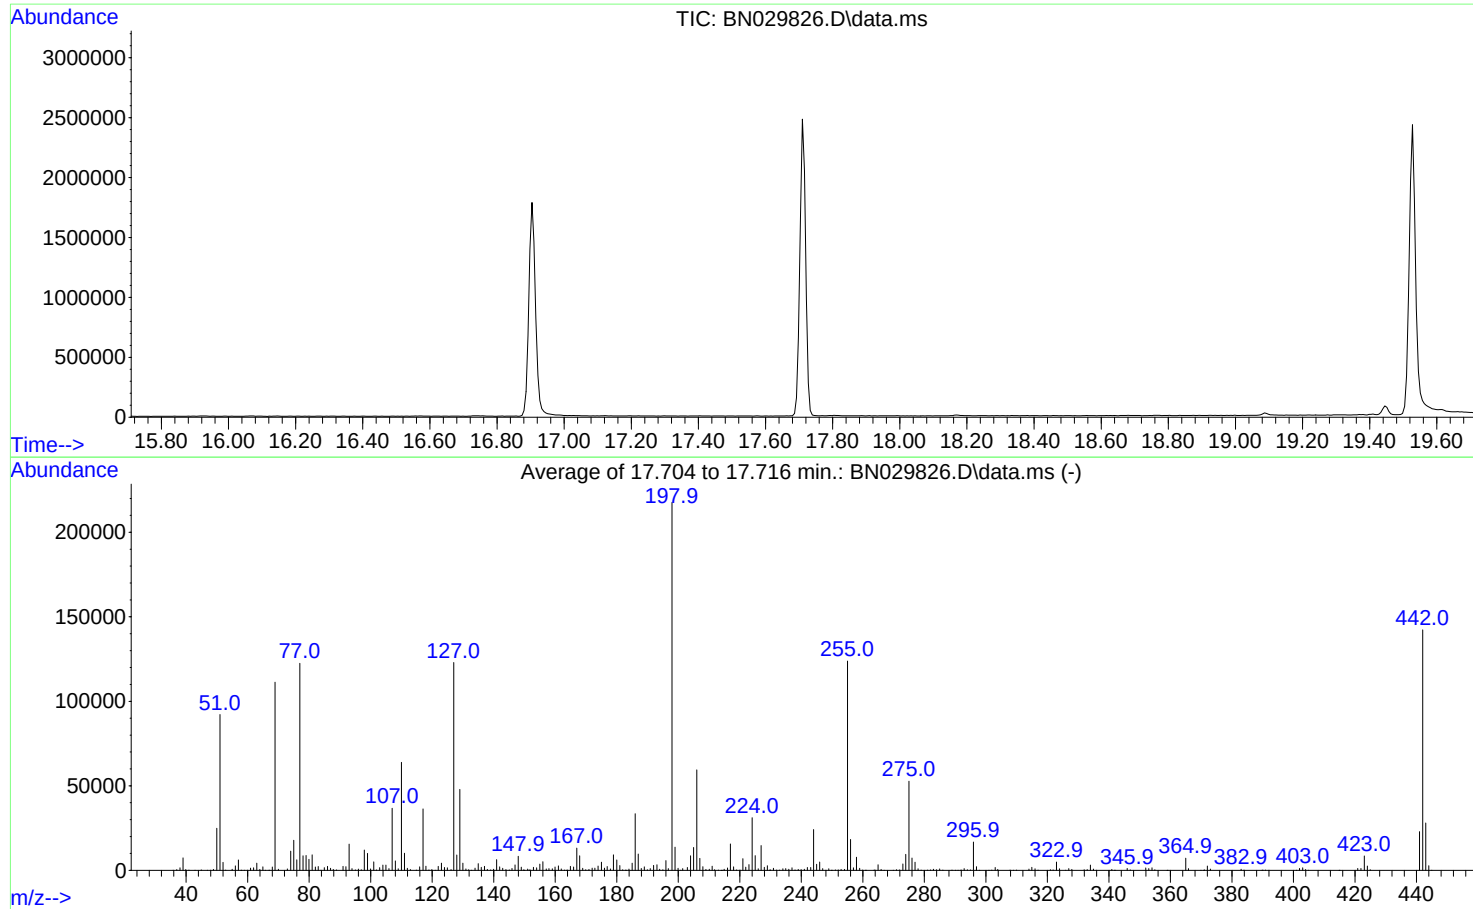




AutoFind: Scans 2485, 2486, 2487; Background Corrected with Scan 2478

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.4	92201	PASS
68	69	0.00	2	1.8	1978	PASS
69	198	0.00	100	51.1	111280	PASS
70	69	0.00	2	0.6	625	PASS
127	198	10	80	56.5	123000	PASS
197	198	0.00	2	0.5	1018	PASS
198	198	100	100	100.0	217621	PASS
199	198	5	9	6.3	13746	PASS
275	198	10	60	24.2	52715	PASS
365	198	1	100	3.3	7200	PASS
441	198	0.01	100	10.5	22945	PASS
442	442	50	100	100.0	142299	PASS
443	442	15	24	19.7	28011	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021624\
Data File : BN029826.D
Acq On : 16 Feb 2024 14:12
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Feb 17 01:09:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 17 01:09:53 2024
Response via : Initial Calibration

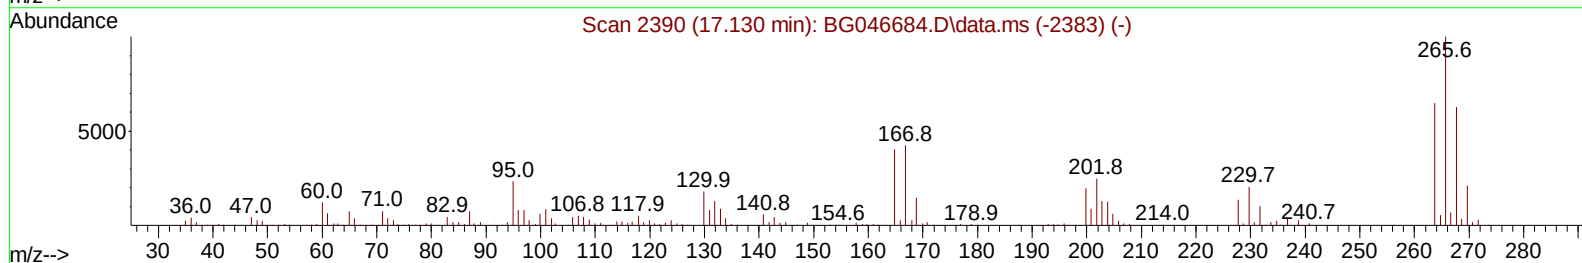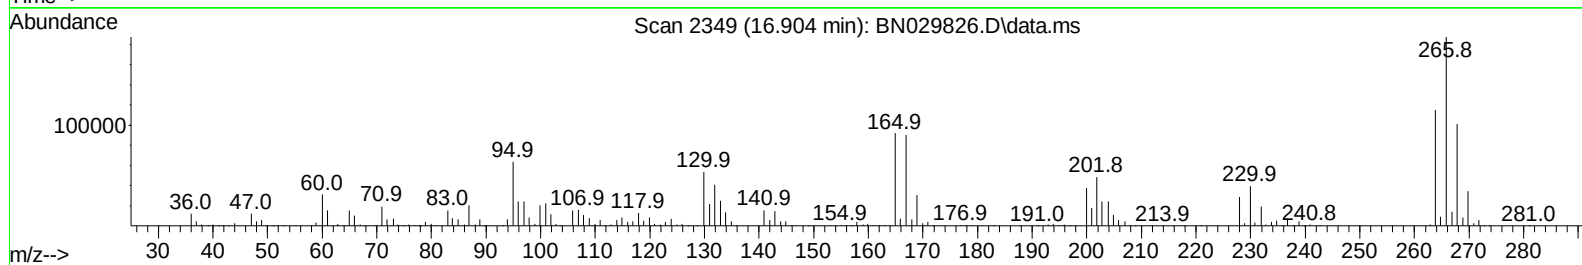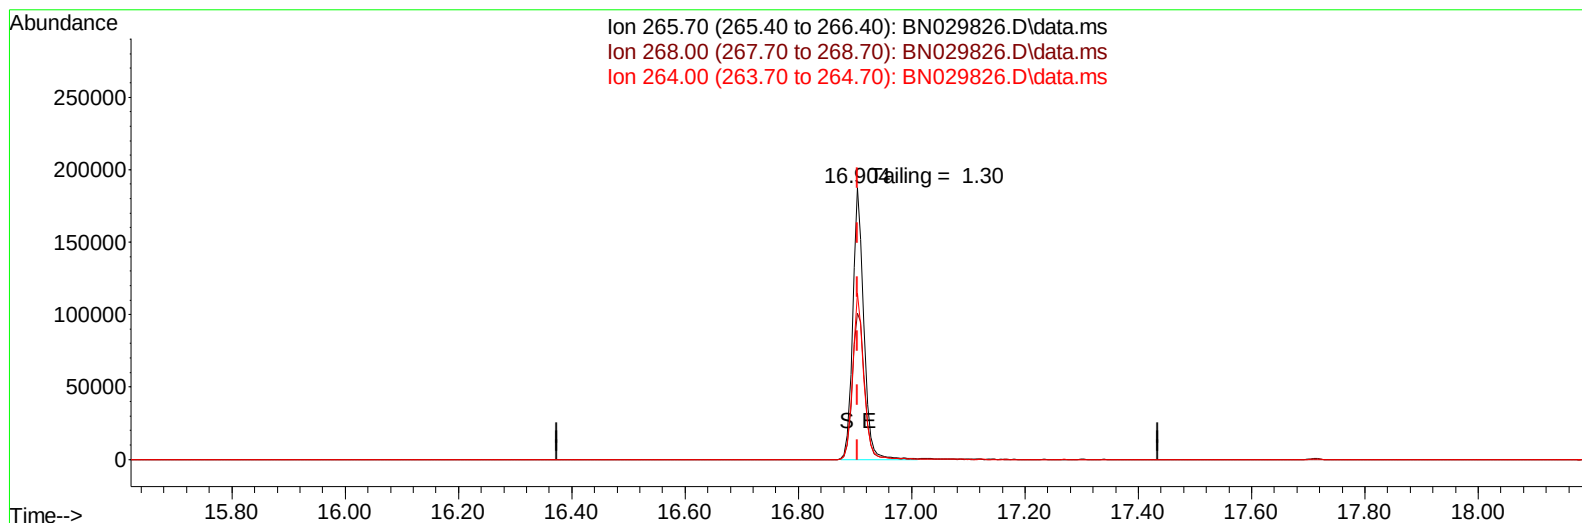

TIC: BN029826.D\data.ms

(70) Pentachlorophenol (C)

16.904min (0.000) 20219.59 ng




response 254996

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	53.98
264.00	61.60	61.25
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021624\
Data File : BN029826.D
Acq On : 16 Feb 2024 14:12
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Feb 17 01:09:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 17 01:09:53 2024
Response via : Initial Calibration

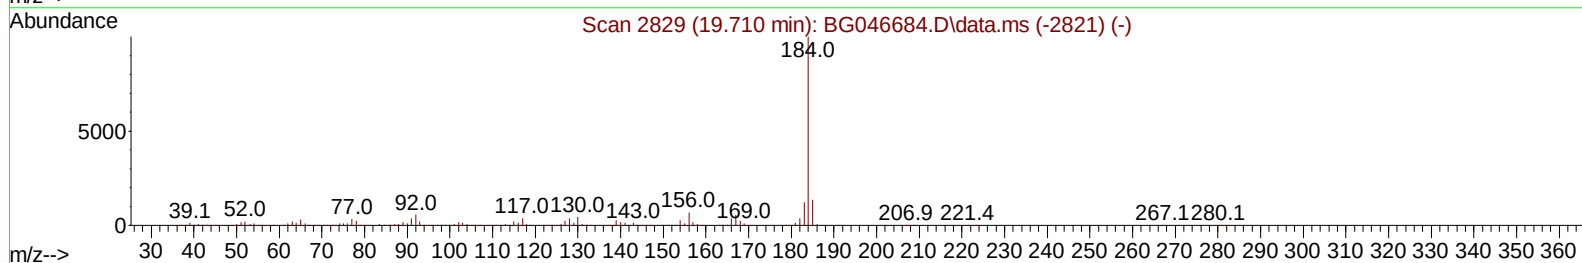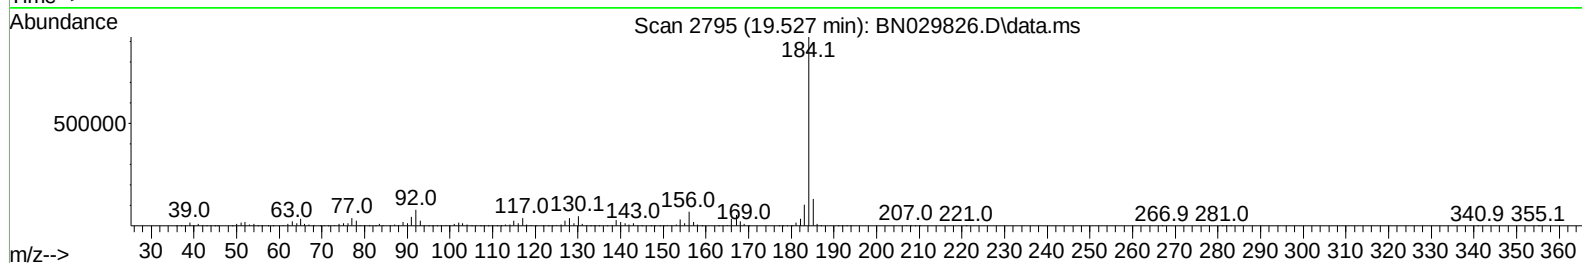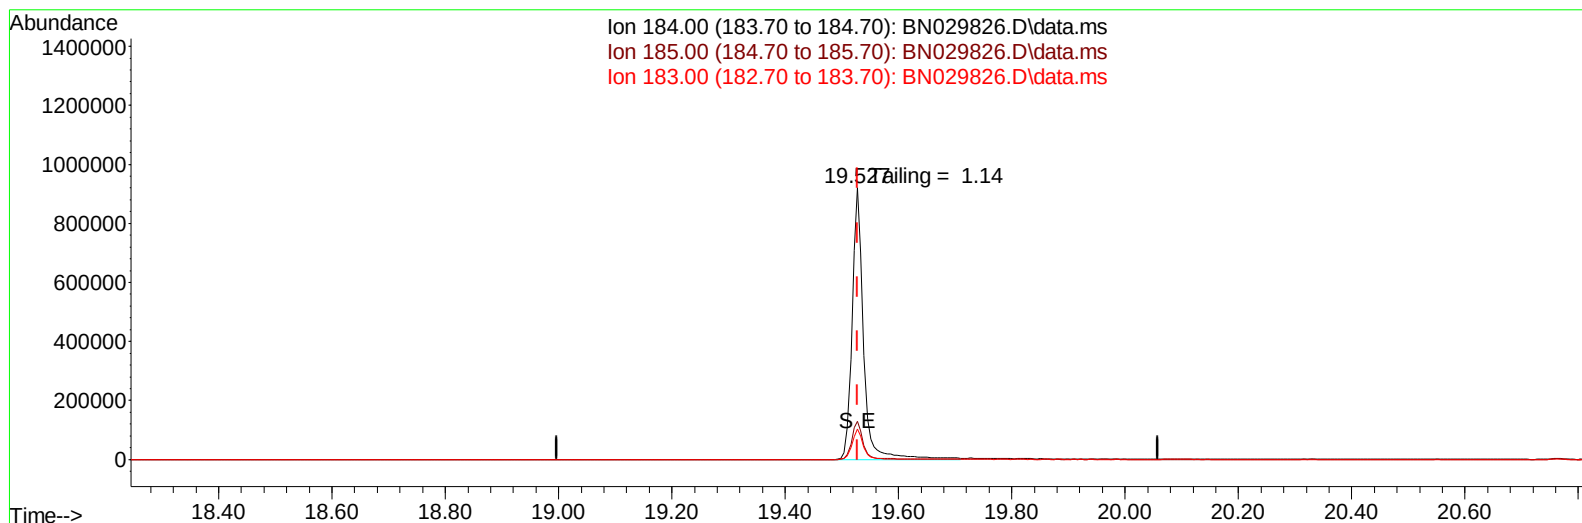

TIC: BN029826.D\data.ms

(77) Benzidine

19.527min (0.000) 0.00 ng

response 1304163

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.14
183.00	13.20	11.22
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/16/2024	BNA_N	<u>BN029826.D</u>
Compound Name	Response	Retention Time
DDT	609306	20.763
DDD	81293	20.322
DDE	3874	19.81
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
85167	694473	12.26

Instrument :
BNA_N
ClientSampleId :
DFTPP