

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021722\
 Data File : BN018640.D
 Acq On : 17 Feb 2022 22:41
 Operator : CG/JU
 Sample : N1507-14
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGZF7

Quant Time: Feb 18 00:35:45 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN021622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Feb 16 16:48:14 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.916	152	217637	20.000	ng/ul	0.00
20) Naphthalene-d8	10.722	136	847318	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.551	164	463709	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.287	188	806255	20.000	ng/ul	0.00
79) Chrysene-d12	21.463	240	593654	20.000	ng/ul	0.00
88) Perylene-d12	23.863	264	575578	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	0.000	96	0d	0.000	ng/uL	
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	0.000	99	0	0.000	ng/ul	
9) Bis-(2-Chloroethyl)eth...	0.000	67	0d	0.000	ng/ul	
11) 2-Chlorophenol-d4	0.000	132	0	0.000	ng/ul	
15) 4-Methylphenol-d8	0.000	113	0d	0.000	ng/ul	
21) Nitrobenzene-d5	0.000	128	0	0.000	ng/ul	
24) 2-Nitrophenol-d4	0.000	143	0	0.000	ng/ul	
28) 2,4-Dichlorophenol-d3	0.000	165	0	0.000	ng/ul	
31) 4-Chloroaniline-d4	0.000	131	0d	0.000	ng/ul	
46) Dimethylphthalate-d6	0.000	166	0	0.000	ng/ul	
49) Acenaphthylene-d8	0.000	160	0	0.000	ng/ul	
54) 4-Nitrophenol-d4	0.000	143	0	0.000	ng/ul	
60) Fluorene-d10	0.000	176	0	0.000	ng/ul	
65) 4,6-Dinitro-2-methylph...	0.000	200	0	0.000	ng/ul	
73) Anthracene-d10	0.000	188	0d	0.000	ng/ul	
81) Pyrene-d10	0.000	212	0d	0.000	ng/ul	
92) Benzo(a)pyrene-d12	0.000	264	0d	0.000	ng/ul	
Target Compounds						
					Qvalue	
72) Phenanthrene	17.334	178	47211	1.037	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021722\
Data File : BN018640.D
Acq On : 17 Feb 2022 22:41
Operator : CG/JU
Sample : N1507-14
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGZF7

Quant Time: Feb 18 00:35:45 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN021622.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 16 16:48:14 2022
Response via : Initial Calibration

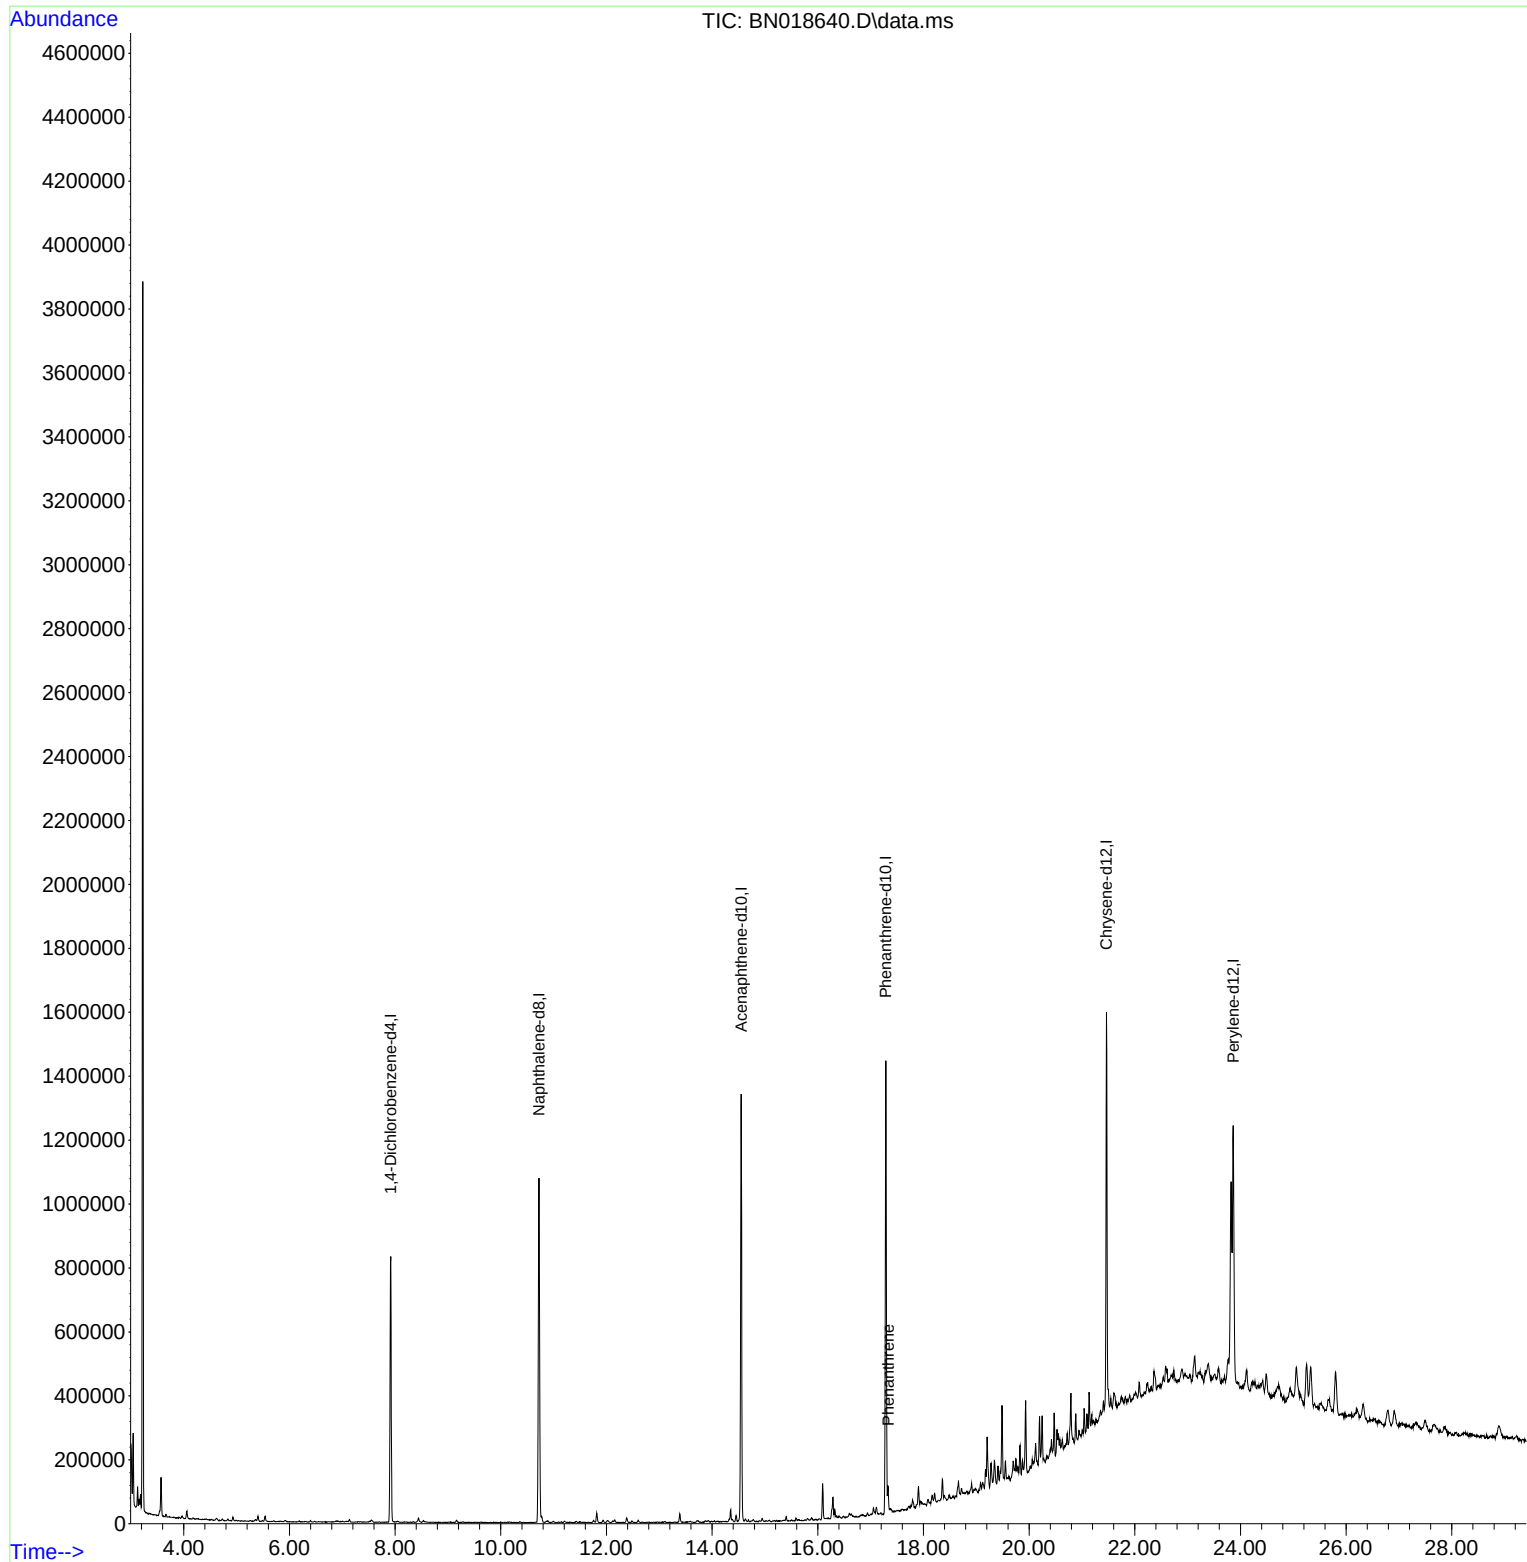

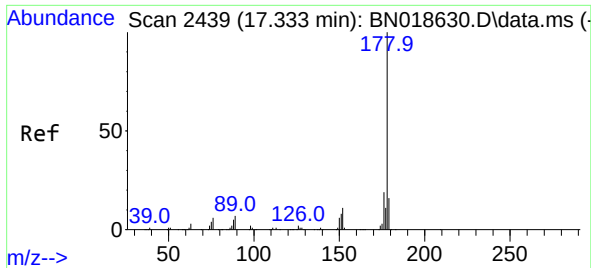

#72

Phenanthrene

Concen: 1.037 ng/ul

RT: 17.334 min Scan# 2439

Delta R.T. 0.006 min

Lab File: BN018640.D


Acq: 17 Feb 2022 22:41

Instrument :

BNA_N

ClientSampleId :

BGZF7

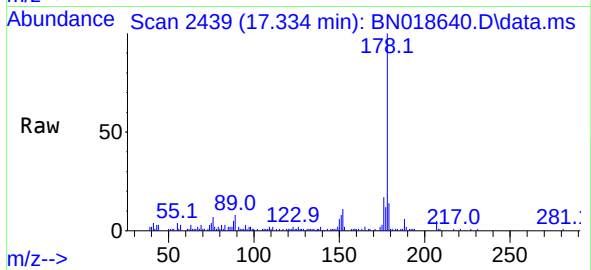

Tgt Ion:178 Resp: 47211

Ion	Ratio	Lower	Upper
-----	-------	-------	-------

178	100		
-----	-----	--	--

179	13.8	12.2	18.4
-----	------	------	------

176	17.1	14.6	21.8
-----	------	------	------

