

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021722\
 Data File : BN018644.D
 Acq On : 18 Feb 2022 01:06
 Operator : CG/JU
 Sample : N1506-16
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGZG4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN021622.M
 Title : SVOA CALIBRATION

Signal : TIC: BN018644.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.040	6	9	16	rVB	217448	236634	6.36%	1.366%
2	3.122	20	23	26	rVV2	64168	72949	1.96%	0.421%
3	3.152	26	28	31	rVV	29500	35894	0.96%	0.207%
4	3.181	31	33	35	rVV	42226	37084	1.00%	0.214%
5	3.222	35	40	45	rVB	3584035	3723247	100.00%	21.498%
6	3.569	95	99	104	rVB	141267	170966	4.59%	0.987%
7	3.663	112	115	120	rVB5	8389	10380	0.28%	0.060%
8	3.969	162	167	176	rVV	30721	47578	1.28%	0.275%
9	4.058	177	182	191	rVB2	31264	56508	1.52%	0.326%
10	4.181	198	203	207	rBV	8797	13164	0.35%	0.076%
11	4.246	211	214	217	rVV3	7431	9400	0.25%	0.054%
12	4.287	218	221	226	rVB4	4865	6870	0.18%	0.040%
13	4.599	269	274	286	rVB2	122649	197523	5.31%	1.141%
14	4.728	292	296	301	rVB3	6847	10418	0.28%	0.060%
15	4.834	309	314	320	rVB2	12721	19032	0.51%	0.110%
16	4.928	326	330	335	rVB	25366	34395	0.92%	0.199%
17	4.999	338	342	345	rVB5	6471	10045	0.27%	0.058%
18	5.034	345	348	355	rBV5	4423	6817	0.18%	0.039%
19	5.257	382	386	391	rBV5	5592	8297	0.22%	0.048%
20	5.357	395	403	405	rVV3	11722	22595	0.61%	0.130%
21	5.405	407	411	417	rVB	31887	46344	1.24%	0.268%
22	5.487	421	425	428	rBV2	5151	6827	0.18%	0.039%
23	5.540	428	434	440	rVV	18150	28433	0.76%	0.164%
24	5.710	455	463	468	rVB6	8805	17590	0.47%	0.102%
25	5.769	468	473	477	rBV7	3452	6037	0.16%	0.035%
26	5.822	477	482	486	rBV4	7674	10738	0.29%	0.062%
27	5.910	492	497	504	rVB5	6715	11890	0.32%	0.069%
28	6.181	537	543	550	rBV4	9934	17779	0.48%	0.103%
29	6.304	562	564	571	rVB4	4477	7163	0.19%	0.041%
30	6.399	574	580	588	rVB3	9108	16335	0.44%	0.094%
31	6.475	588	593	596	rBV5	4794	7184	0.19%	0.041%
32	6.551	602	606	610	rBV5	4532	7280	0.20%	0.042%
33	6.881	659	662	665	rBV4	4086	6093	0.16%	0.035%
34	7.010	681	684	689	rVB5	4624	7116	0.19%	0.041%
35	7.134	701	705	713	rVB4	9444	14926	0.40%	0.086%
36	7.251	719	725	729	rBV8	3085	6917	0.19%	0.040%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021722\
 Data File : BN018644.D
 Acq On : 18 Feb 2022 01:06
 Operator : CG/JU
 Sample : N1506-16
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGZG4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN021622.M
 Title : SVOA CALIBRATION

37	7.304	730	734	737	rVV4	5632	9243	0.25%	0.053%
38	7.346	737	741	746	rVV6	4226	6817	0.18%	0.039%
39	7.393	746	749	756	rVB7	3800	7902	0.21%	0.046%
40	7.481	761	764	771	rVV7	4584	8531	0.23%	0.049%

41	7.569	771	779	785	rVB3	9626	21536	0.58%	0.124%
42	7.916	829	838	849	rBV	838734	1358695	36.49%	7.845%
43	8.057	855	862	868	rVB4	8965	18978	0.51%	0.110%
44	8.469	929	932	937	rVV5	6404	9583	0.26%	0.055%
45	8.563	944	948	952	rVV4	4692	8549	0.23%	0.049%

46	9.163	1045	1050	1055	rVV4	4935	7146	0.19%	0.041%
47	9.293	1068	1072	1077	rVB7	4409	7550	0.20%	0.044%
48	9.616	1121	1127	1131	rVB6	3420	6238	0.17%	0.036%
49	9.940	1175	1182	1184	rBV5	3531	7070	0.19%	0.041%
50	10.010	1190	1194	1199	rVB7	4630	6787	0.18%	0.039%

51	10.722	1307	1315	1321	rBV	1042028	1743148	46.82%	10.065%
52	10.775	1321	1324	1330	rVV	56259	86348	2.32%	0.499%
53	10.863	1334	1339	1343	rBV5	6491	12541	0.34%	0.072%
54	10.992	1357	1361	1366	rVB6	5904	10246	0.28%	0.059%
55	11.145	1383	1387	1391	rVV5	5954	8744	0.23%	0.050%

56	11.204	1393	1397	1404	rVB6	7617	14284	0.38%	0.082%
57	11.428	1431	1435	1441	rBV8	6758	13101	0.35%	0.076%
58	11.498	1441	1447	1452	rBV6	5083	9353	0.25%	0.054%
59	11.651	1466	1473	1479	rBV9	3733	7796	0.21%	0.045%
60	11.763	1488	1492	1498	rBV4	3526	7356	0.20%	0.042%

61	11.816	1498	1501	1507	rVB5	3300	6586	0.18%	0.038%
62	12.157	1554	1559	1566	rVB4	5888	10270	0.28%	0.059%
63	12.381	1593	1597	1604	rVB	16601	27030	0.73%	0.156%
64	12.598	1629	1634	1642	rVB	8981	14662	0.39%	0.085%
65	13.386	1763	1768	1774	rBV2	18370	27086	0.73%	0.156%

66	13.875	1844	1851	1855	rBV6	7100	11428	0.31%	0.066%
67	14.457	1945	1950	1955	rBV2	9375	14910	0.40%	0.086%
68	14.551	1955	1966	1974	rBV	1303365	1912718	51.37%	11.044%
69	14.945	2028	2033	2038	rVB3	14375	19743	0.53%	0.114%
70	15.086	2050	2057	2060	rVB8	3244	6558	0.18%	0.038%

71	15.404	2107	2111	2116	rBV2	10680	13020	0.35%	0.075%
72	15.592	2138	2143	2147	rBV6	6104	8857	0.24%	0.051%
73	15.810	2174	2180	2183	rBV6	5063	6692	0.18%	0.039%
74	15.886	2190	2193	2200	rBV9	3207	6445	0.17%	0.037%
75	16.022	2212	2216	2219	rBV6	3767	6631	0.18%	0.038%

76	16.263	2253	2257	2259	rBV3	19744	26930	0.72%	0.155%
----	--------	------	------	------	------	-------	-------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021722\
 Data File : BN018644.D
 Acq On : 18 Feb 2022 01:06
 Operator : CG/JU
 Sample : N1506-16
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGZG4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN021622.M
 Title : SVOA CALIBRATION

77	16.286	2259	2261	2266	rVB3	16606	20484	0.55%	0.118%
78	17.057	2388	2392	2397	rBV3	11822	18965	0.51%	0.110%
79	17.104	2397	2400	2405	rVB4	11206	16730	0.45%	0.097%
80	17.286	2425	2431	2436	rBV	1343409	1916503	51.47%	11.066%
81	17.327	2436	2438	2443	rVB	82534	100833	2.71%	0.582%
82	17.792	2514	2517	2520	rBV3	13031	17128	0.46%	0.099%
83	17.904	2533	2536	2540	rVB5	16863	20596	0.55%	0.119%
84	18.163	2578	2580	2584	rVB3	11842	14438	0.39%	0.083%
85	18.216	2585	2589	2594	rVB	19225	26485	0.71%	0.153%
86	18.357	2609	2613	2618	rBV2	55529	84800	2.28%	0.490%
87	18.645	2658	2662	2672	rBV2	29744	54126	1.45%	0.313%
88	18.910	2705	2707	2710	rVB4	18092	18384	0.49%	0.106%
89	19.116	2739	2742	2748	rBV4	20252	39344	1.06%	0.227%
90	19.180	2749	2753	2754	rVV3	43792	54004	1.45%	0.312%
91	19.204	2754	2757	2764	rVB3	78797	113166	3.04%	0.653%
92	19.280	2766	2770	2774	rBV2	32293	53029	1.42%	0.306%
93	19.339	2777	2780	2786	rVB	88572	121446	3.26%	0.701%
94	19.486	2801	2805	2809	rBV	122851	157519	4.23%	0.910%
95	19.551	2813	2816	2820	rVB5	37182	42956	1.15%	0.248%
96	19.827	2860	2863	2867	rVB3	53447	63116	1.70%	0.364%
97	19.933	2877	2881	2888	rVB2	110304	146555	3.94%	0.846%
98	20.198	2923	2926	2929	rBV4	56505	63133	1.70%	0.365%
99	21.462	3136	3141	3146	rBV	1346708	1719064	46.17%	9.926%
100	23.862	3543	3549	3560	rVB	954132	1970469	52.92%	11.378%




Sum of corrected areas: 17318829

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021722\
Data File : BN018644.D
Acq On : 18 Feb 2022 01:06
Operator : CG/JU
Sample : N1506-16
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGZG4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN021622.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

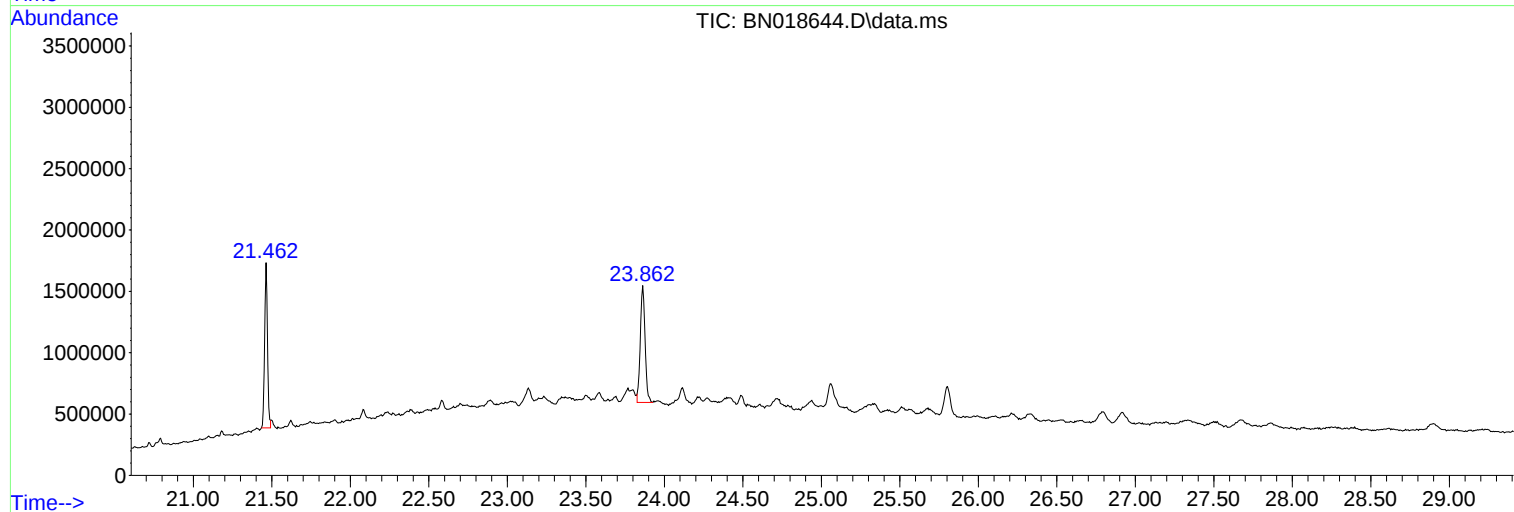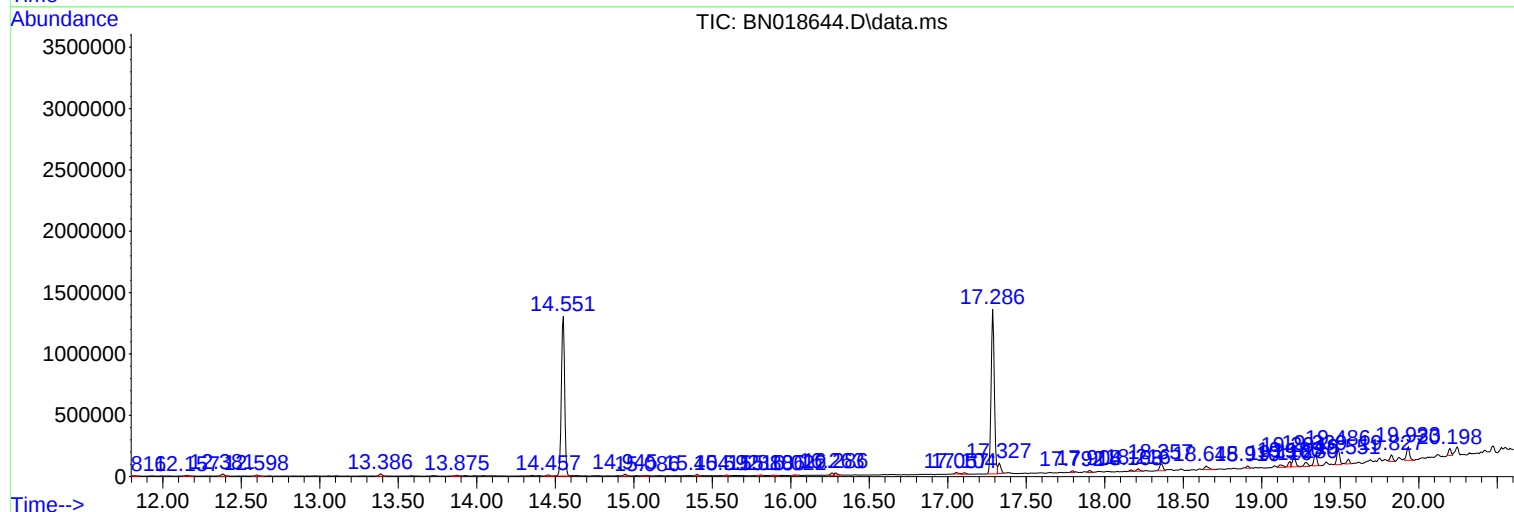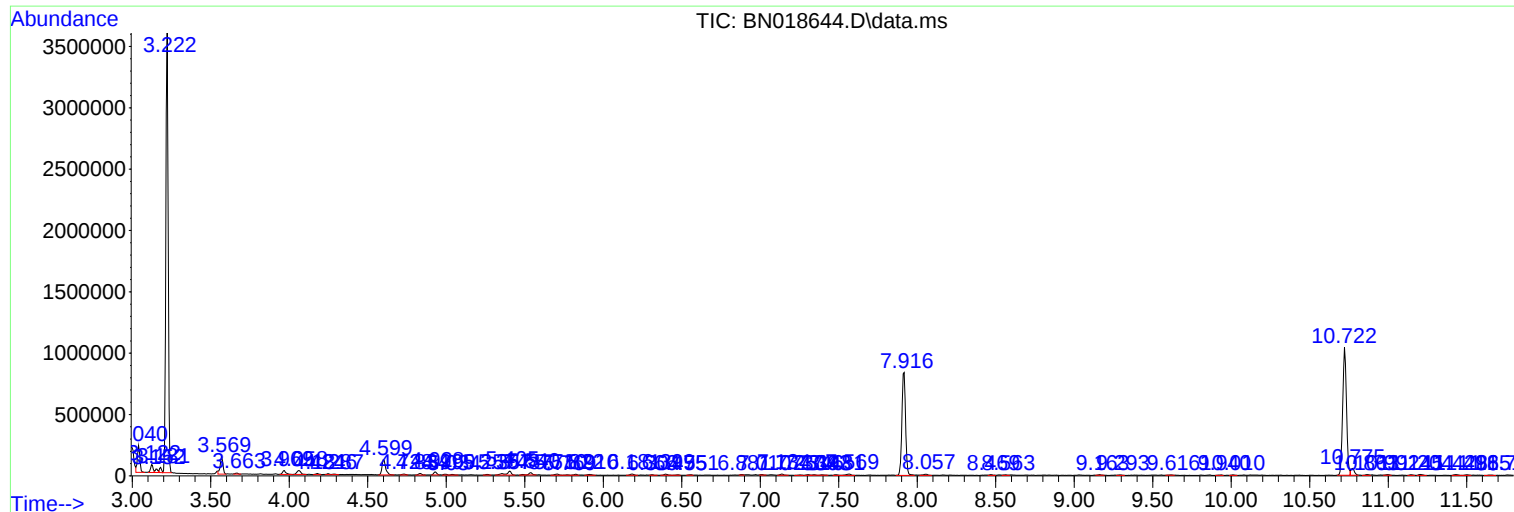

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021722\
Data File : BN018644.D
Acq On : 18 Feb 2022 01:06
Operator : CG/JU
Sample : N1506-16
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGZG4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN021622.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021722\
Data File : BN018644.D
Acq On : 18 Feb 2022 01:06
Operator : CG/JU
Sample : N1506-16
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGZG4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN021622.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc