
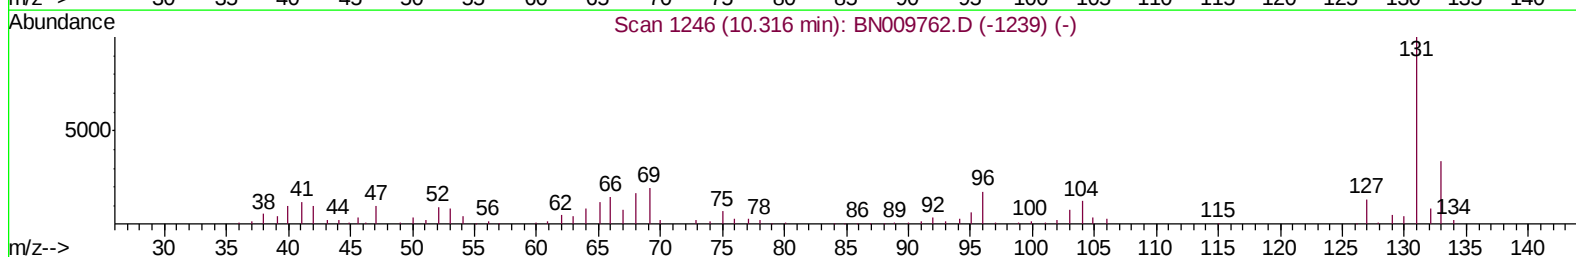
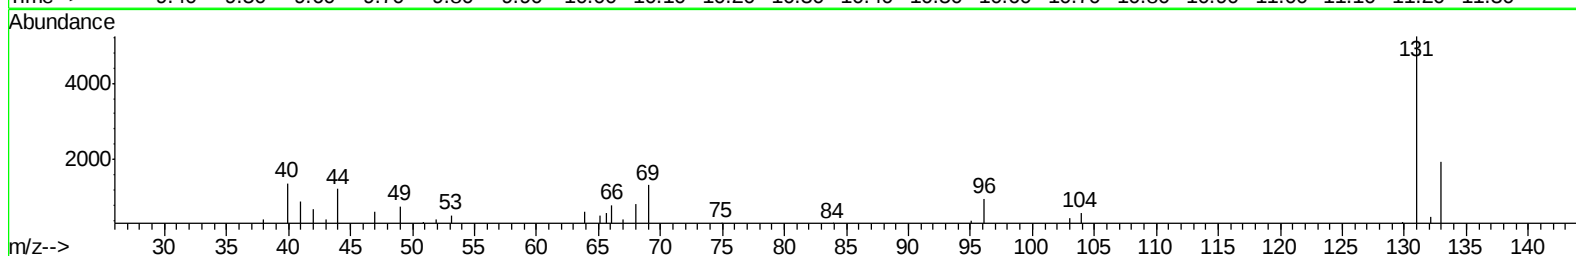


Data File : BN009764.D
Acq On : 19 Feb 2020 04:25
Operator : CG/JU
Sample : L1541-16
Misc :
ALS Vial : 23 Sample Multiplier: 1

Quant Time: Feb 19 05:46:08 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 19 04:46:48 2020
Response via : Initial Calibration

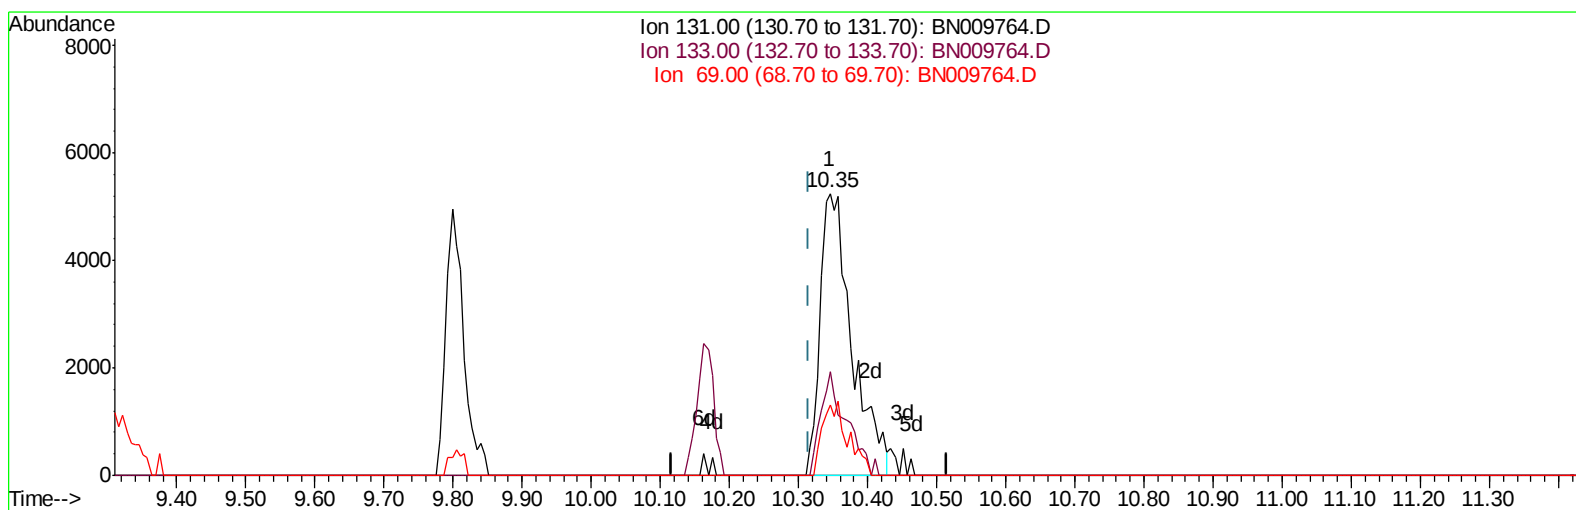

TIC: BN009764.D

(29) 4-Chloroaniline-d4 (S)

10.346min (+0.029) 2.11ng/ul m

response 16643

Ion	Exp%	Act%
131.00	100	100
133.00	33.00	36.89
69.00	22.10	25.09
0.00	0.00	0.00