

Data File : BN009747.D

Acq On : 18 Feb 2020 17:38

Operator : CG/JU

Sample : SSTDCCC020

Misc :

ALS Vial : 2 Sample Multiplier: 1




Quant Time: Feb 19 02:51:40 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M

Quant Title : SVOA CALIBRATION

QLast Update : Wed Feb 19 02:49:03 2020

Response via : Initial Calibration

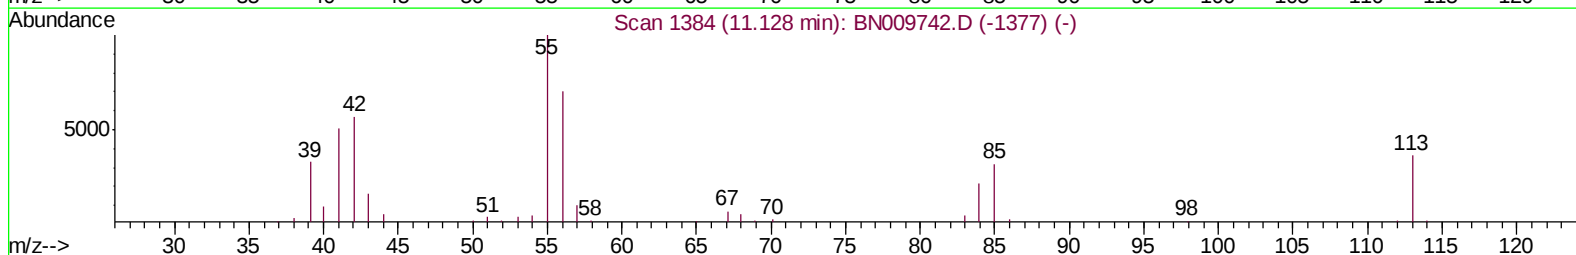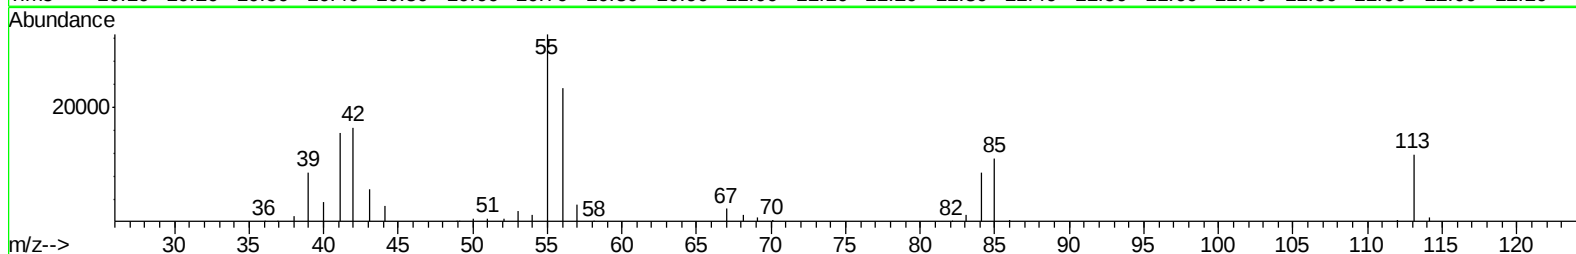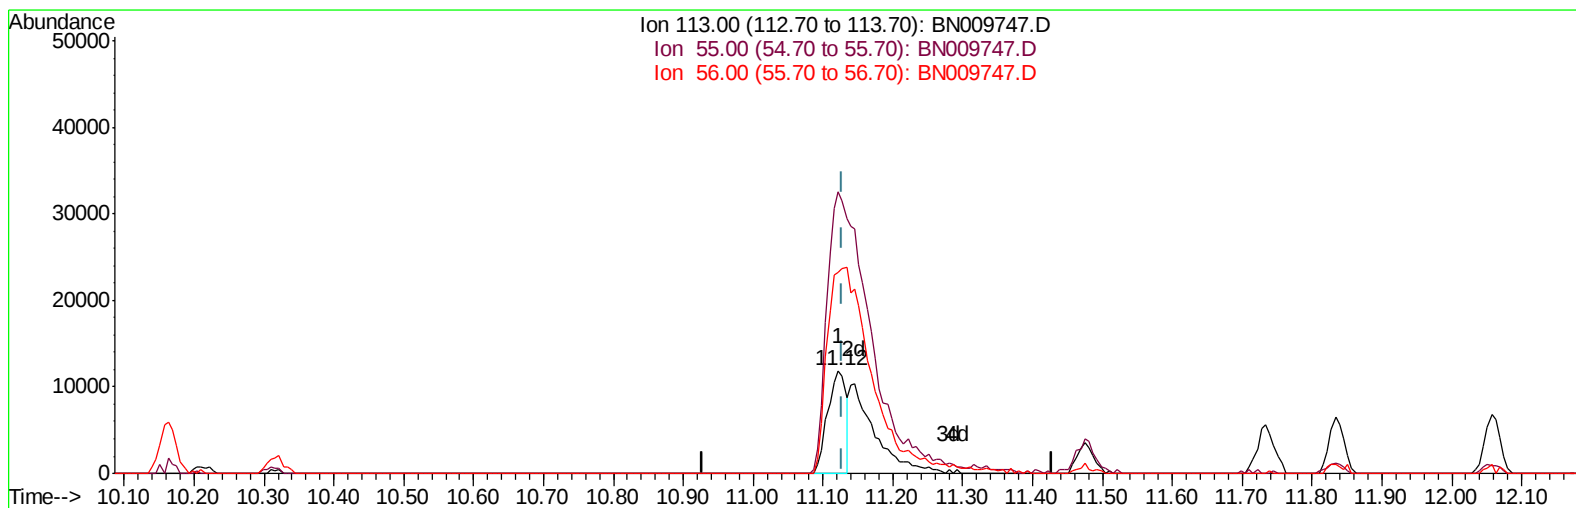

TIC: BN009747.D

(32) Caprolactam

11.122min (-0.006) 8.51ng/ul

response 21352

Ion	Exp%	Act%
113.00	100	100
55.00	261.40	274.24
56.00	202.00	196.21
0.00	0.00	0.00