
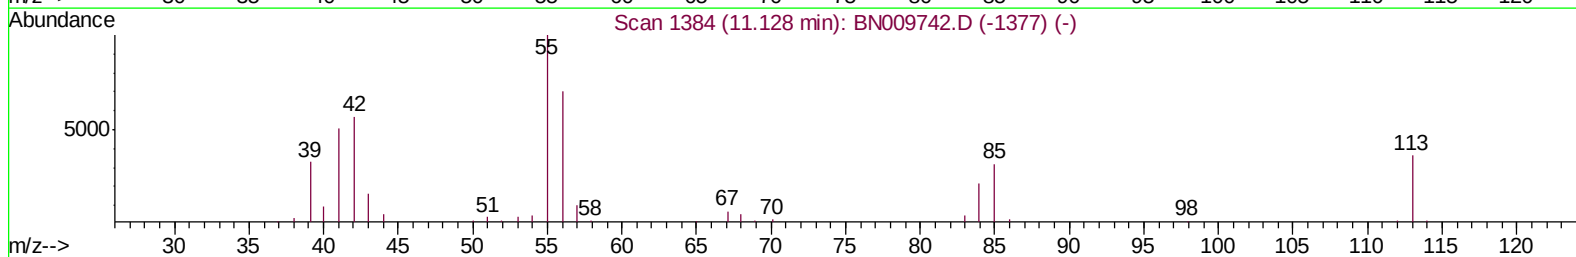
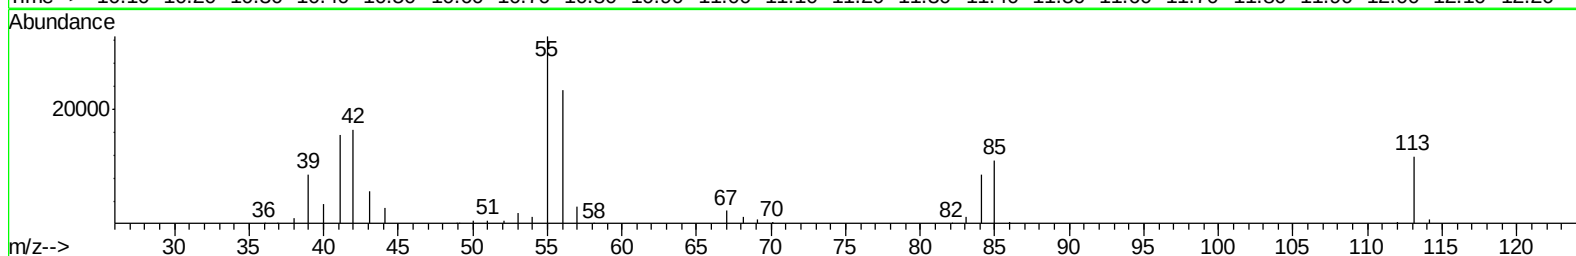


Data File : BN009747.D
Acq On : 18 Feb 2020 17:38
Operator : CG/JU
Sample : SSTDCCC020
Misc :
ALS Vial : 2 Sample Multiplier: 1

Quant Time: Feb 19 02:51:40 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 19 02:49:03 2020
Response via : Initial Calibration

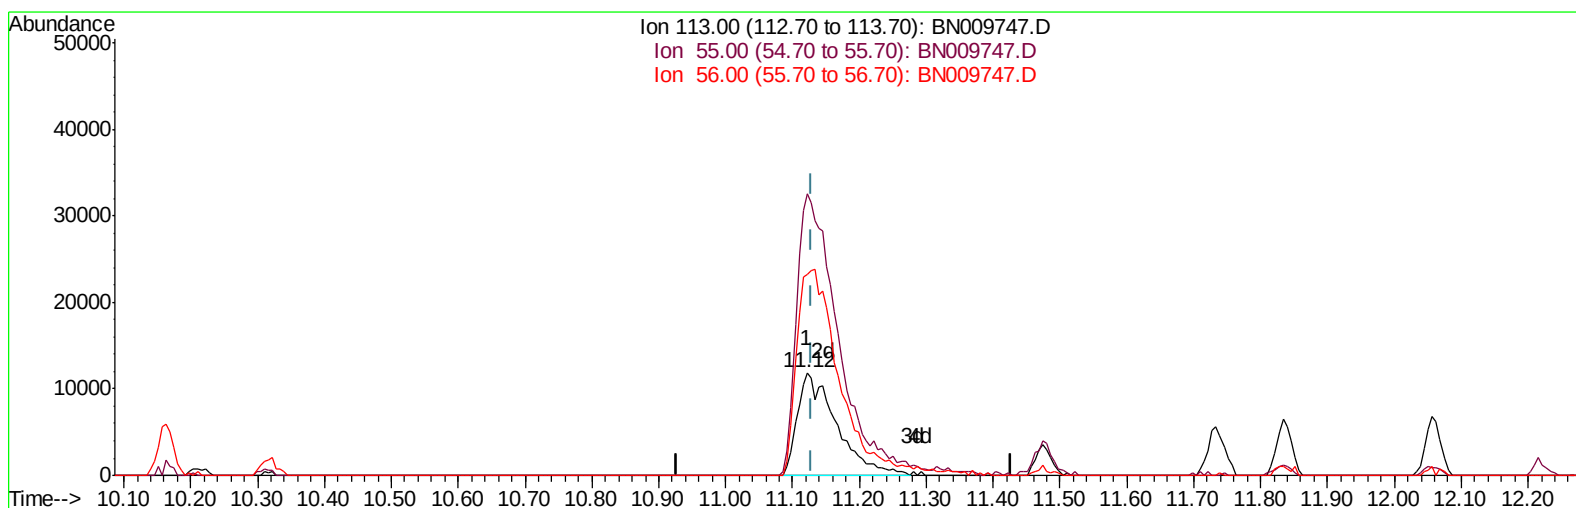

TIC: BN009747.D

(32) Caprolactam

11.122min (-0.006) 19.20ng/ul m

response 48166

Ion	Exp%	Act%
113.00	100	100
55.00	261.40	274.24
56.00	202.00	196.21
0.00	0.00	0.00