
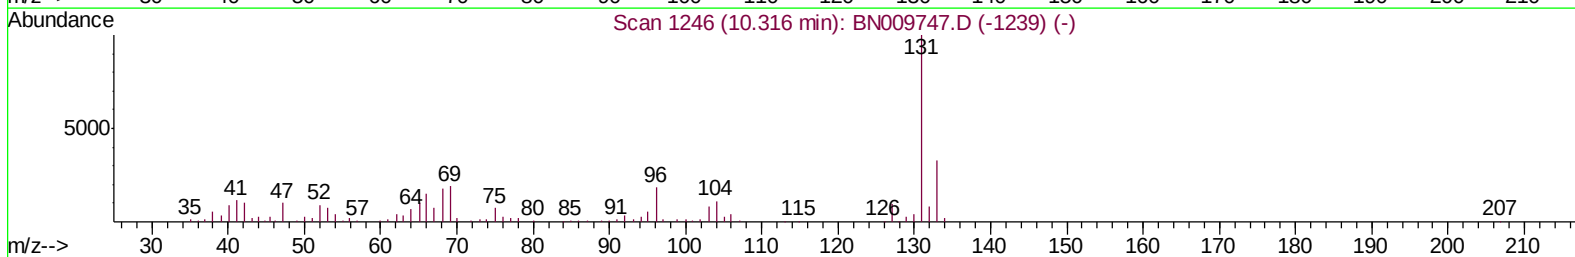
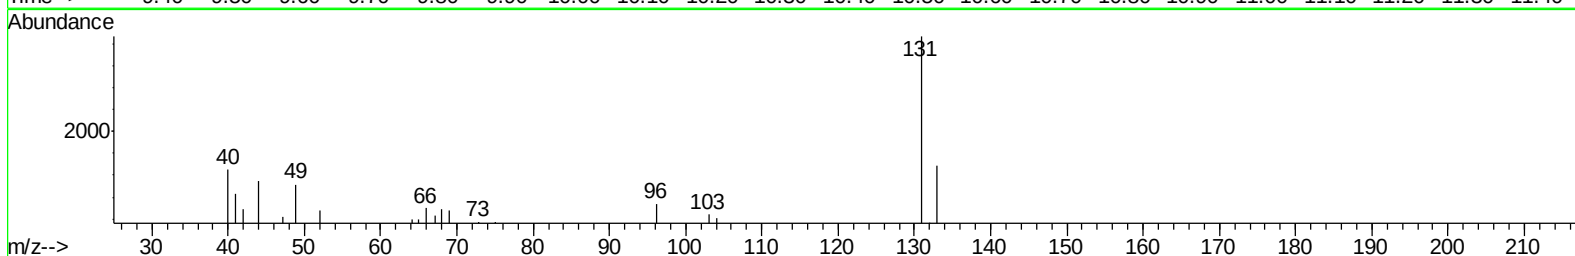


Data File : BN009753.D
Acq On : 18 Feb 2020 21:14
Operator : CG/JU
Sample : L1541-06
Misc :
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Feb 19 03:40:08 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 19 03:37:25 2020
Response via : Initial Calibration

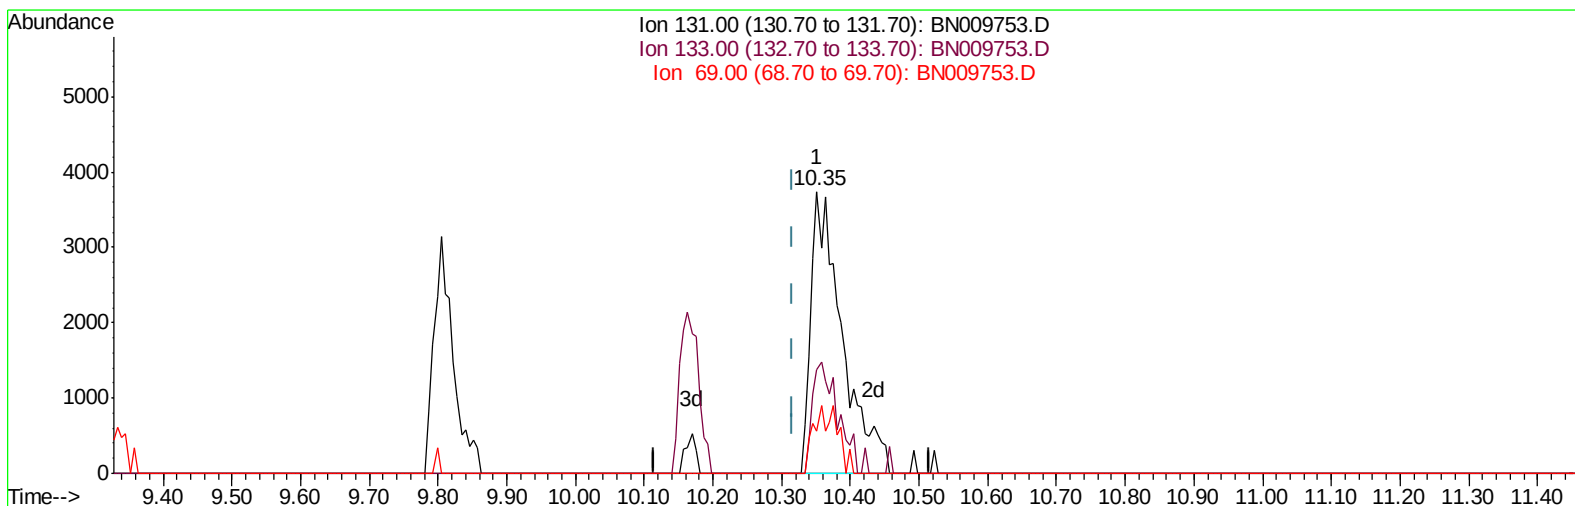

TIC: BN009753.D

(29) 4-Chloroaniline-d4 (S)

10.352min (+0.036) 1.33ng/ul m

response 11791

Ion	Exp%	Act%
131.00	100	100
133.00	33.00	36.63
69.00	22.10	14.82#
0.00	0.00	0.00