
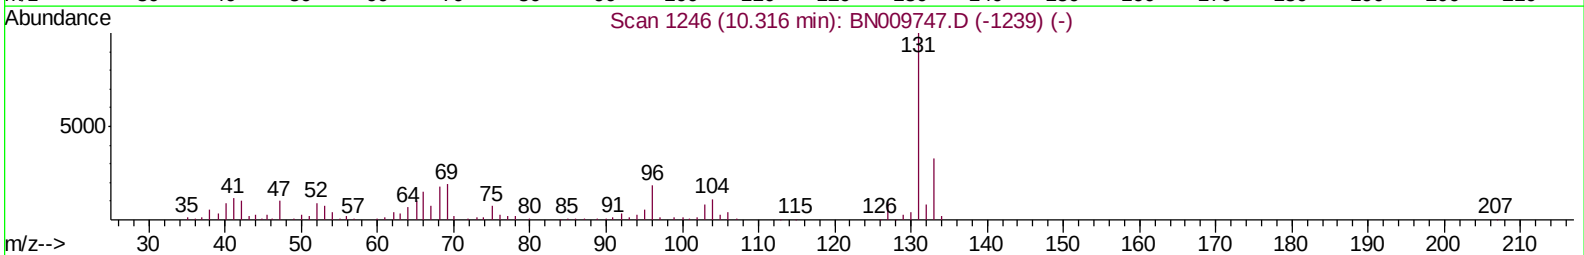
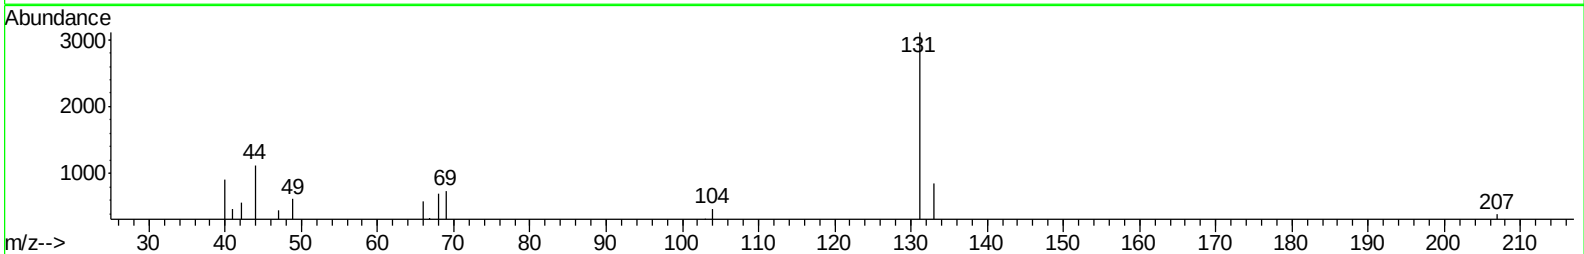


Data File : BN009754.D
Acq On : 18 Feb 2020 21:50
Operator : CG/JU
Sample : L1541-07
Misc :
ALS Vial : 13 Sample Multiplier: 1

Quant Time: Feb 19 03:40:15 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 19 03:37:25 2020
Response via : Initial Calibration

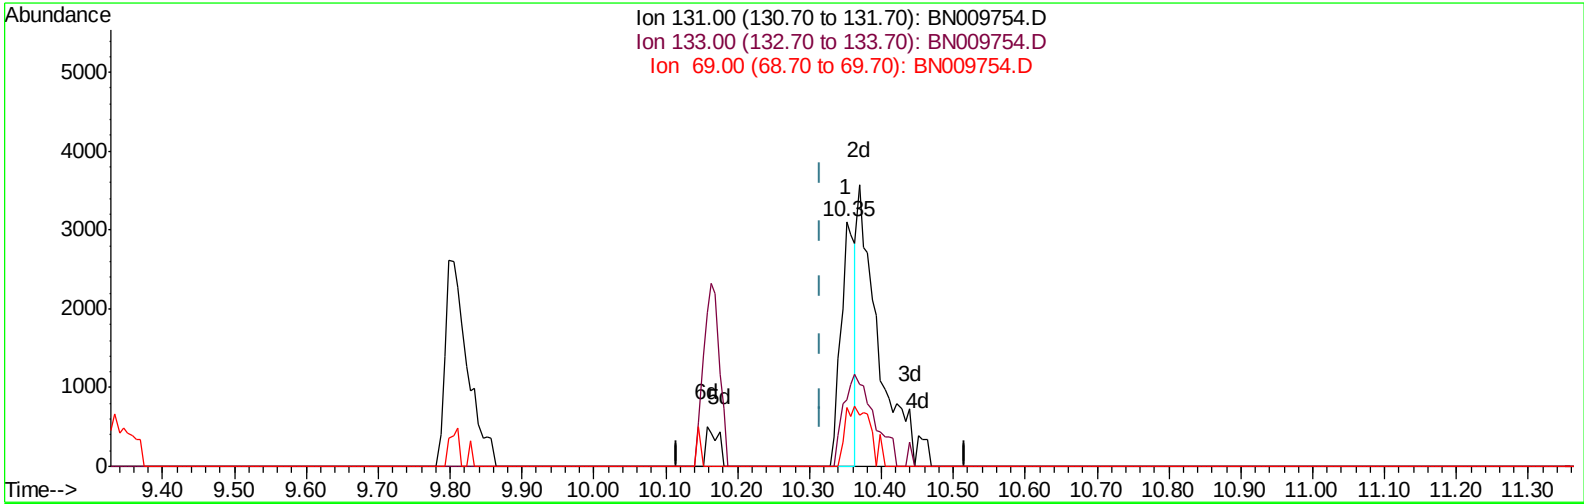

TIC: BN009754.D

(29) 4-Chloroaniline-d4 (S)
10.352min (+0.036) 0.53ng/ul
response 4446

Ion	Exp%	Act%
131.00	100	100
133.00	33.00	27.40
69.00	22.10	23.89
0.00	0.00	0.00