
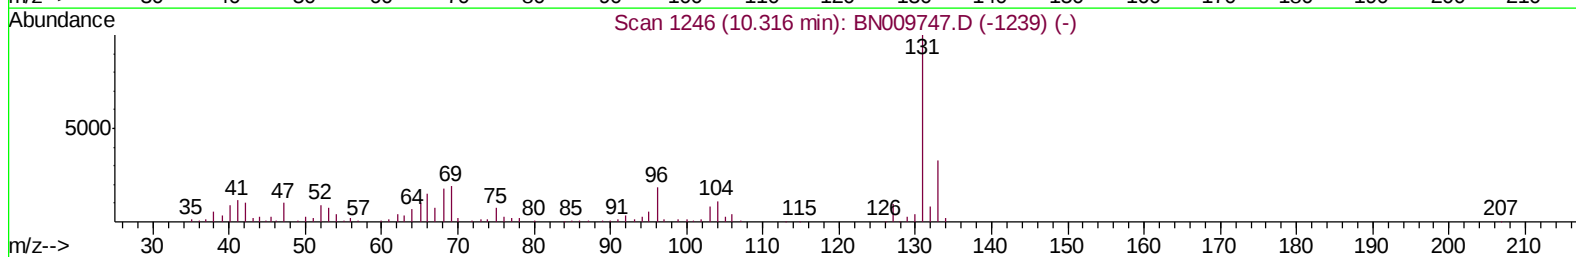
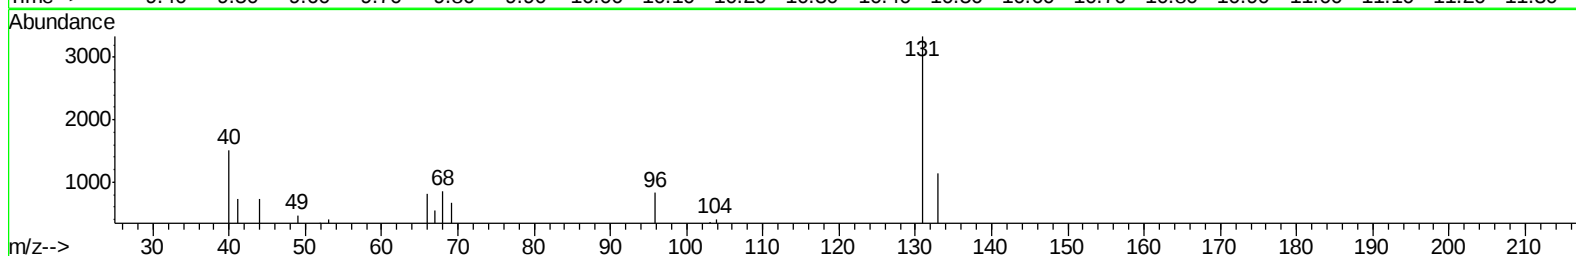


Data File : BN009756.D  
Acq On : 18 Feb 2020 23:02  
Operator : CG/JU  
Sample : L1541-09  
Misc :  
ALS Vial : 15 Sample Multiplier: 1

Quant Time: Feb 19 03:40:27 2020  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_N\METHODS\SOM-EPA-BN021220MA.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Wed Feb 19 03:37:25 2020  
Response via : Initial Calibration

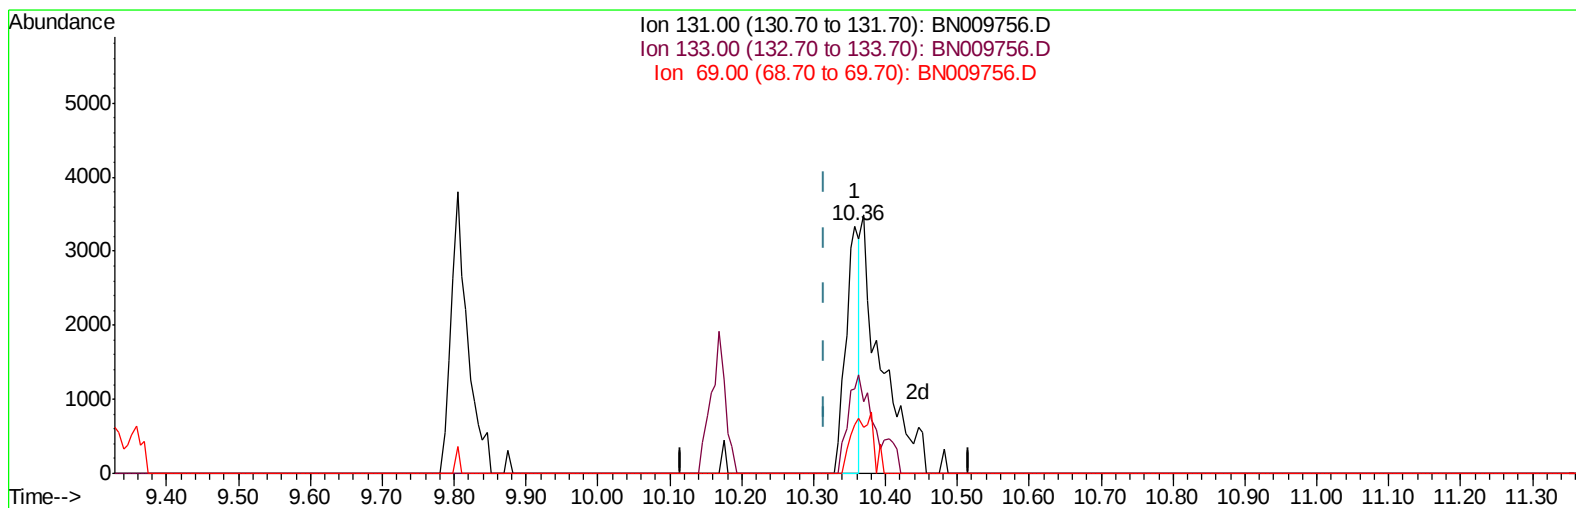

TIC: BN009756.D

(29) 4-Chloroaniline-d4 (S)  
10.357min (+0.042) 0.70ng/ul  
response 4618

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 131.00 | 100   | 100   |
| 133.00 | 33.00 | 34.03 |
| 69.00  | 22.10 | 19.89 |
| 0.00   | 0.00  | 0.00  |