
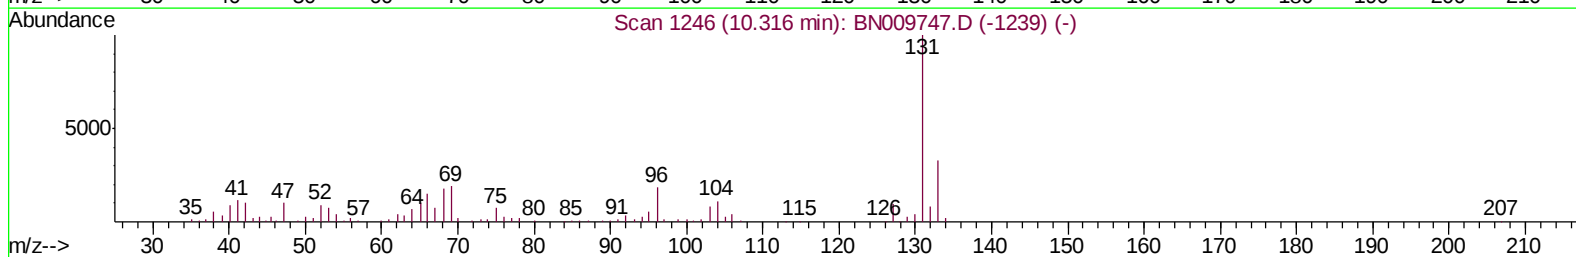
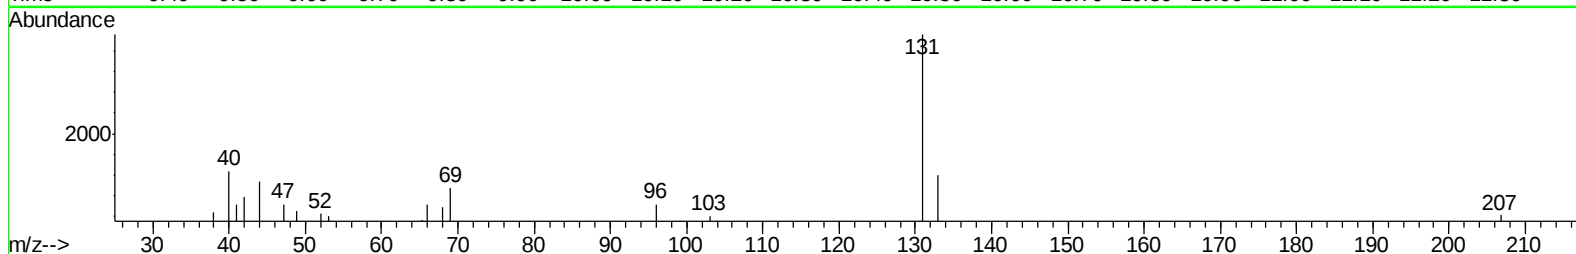


Data File : BN009760.D
Acq On : 19 Feb 2020 01:26
Operator : CG/JU
Sample : L1541-13
Misc :
ALS Vial : 19 Sample Multiplier: 1

Quant Time: Feb 19 03:40:53 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 19 03:37:25 2020
Response via : Initial Calibration

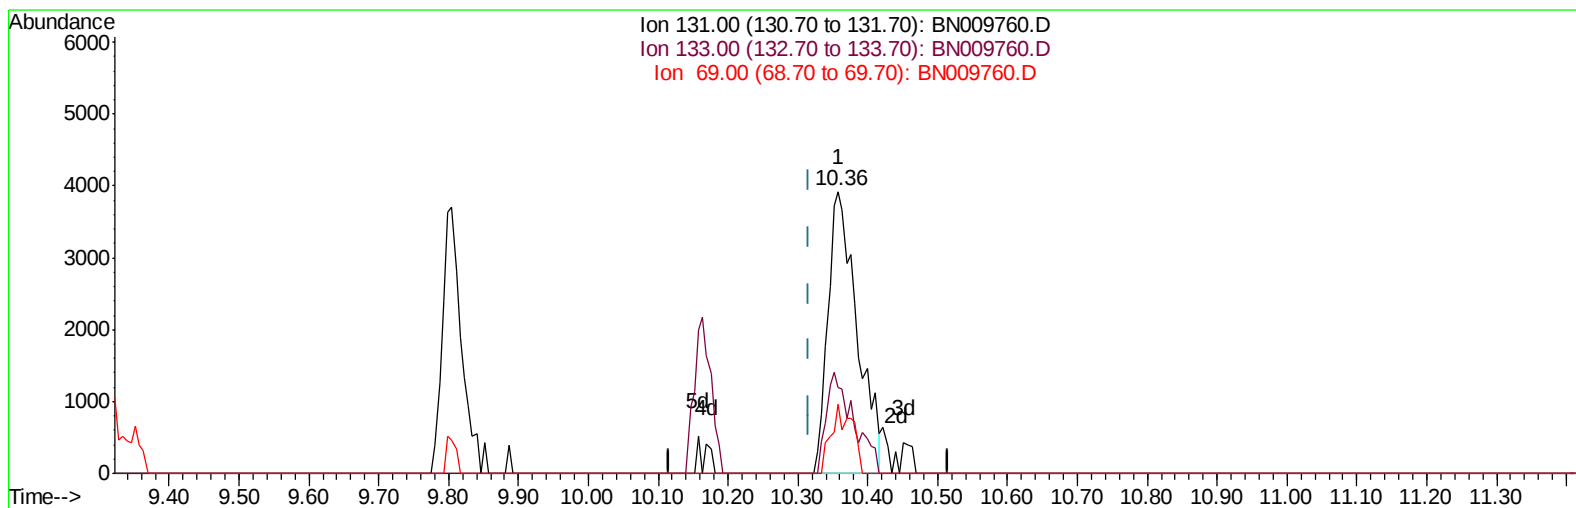

TIC: BN009760.D

(29) 4-Chloroaniline-d4 (S)

10.357min (+0.042) 1.39ng/ul m

response 11324

Ion	Exp%	Act%
131.00	100	100
133.00	33.00	30.26
69.00	22.10	24.42
0.00	0.00	0.00