
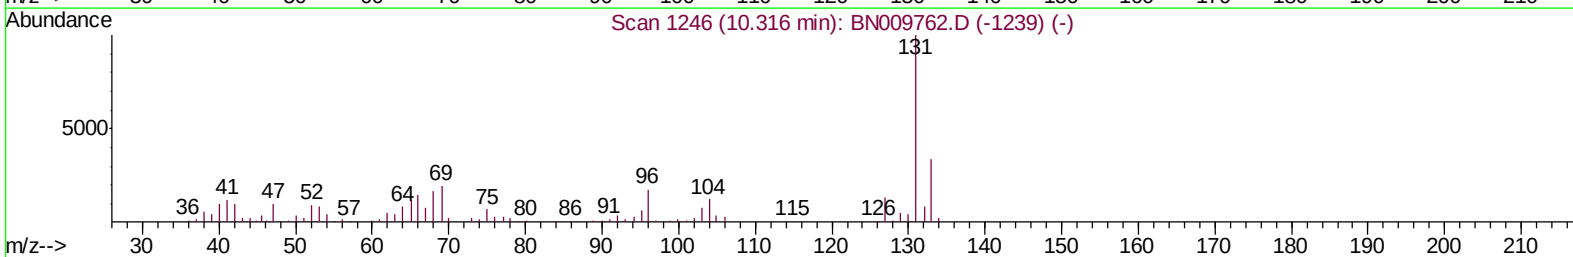
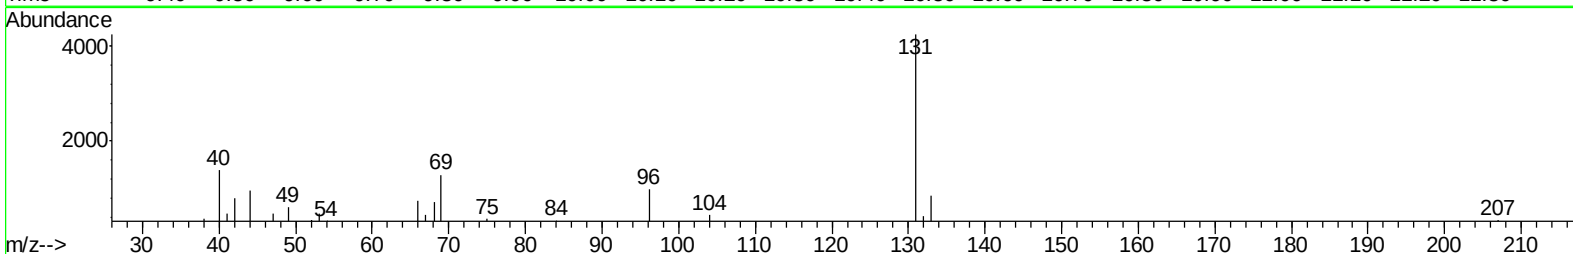


Data File : BN009766.D
Acq On : 19 Feb 2020 05:36
Operator : CG/JU
Sample : L1541-18
Misc :
ALS Vial : 25 Sample Multiplier: 1

Quant Time: Feb 19 08:16:03 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 19 04:46:48 2020
Response via : Initial Calibration

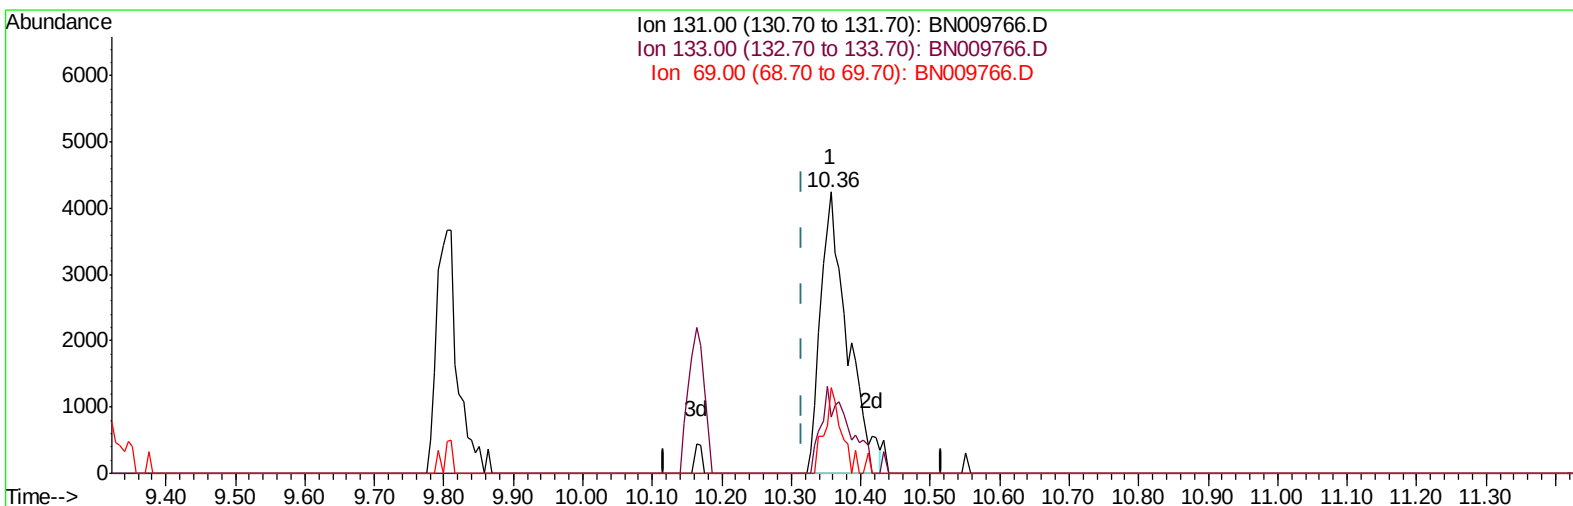

TIC: BN009766.D

(29) 4-Chloroaniline-d4 (S)

10.357min (+0.041) 1.36ng/ul m

response 11557

Ion	Exp%	Act%
131.00	100	100
133.00	33.00	19.86#
69.00	22.10	30.41#
0.00	0.00	0.00