

Data File : BN009750.D
Acq On : 18 Feb 2020 19:26
Operator : CG/JU
Sample : PB126856BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK56

Quant Time: Feb 19 03:39:41 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 19 03:37:25 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.42	152	105402	20.00	ng/ul	0.00
18) Naphthalene-d8	10.16	136	431463	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.05	164	269435	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.81	188	571398	20.00	ng/ul	0.00
78) Chrysene-d12	21.03	240	568279	20.00	ng/ul	0.00
86) Perylene-d12	23.13	264	575612	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.05	96	16892	6.59	ng/uL	0.00
5) Phenol-d5	6.62	99	290250	32.37	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.77	67	210327	34.00	ng/ul	0.00
9) 2-Chlorophenol-d4	6.96	132	230603	34.17	ng/ul	0.00
13) 4-Methylphenol-d8	8.13	113	227944	31.96	ng/ul	0.00
19) Nitrobenzene-d5	8.56	128	110385	34.97	ng/ul	0.00
22) 2-Nitrophenol-d4	9.27	143	119486	34.60	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.80	165	213413	32.15	ng/ul	0.00
29) 4-Chloroaniline-d4	10.32	131	302370	40.54	ng/ul	0.00
44) Dimethylphthalate-d6	13.48	166	711798	35.37	ng/ul	0.00
47) Acenaphthylene-d8	13.74	160	785846	33.15	ng/ul	0.00
52) 4-Nitrophenol-d4	14.29	143	99253	27.00	ng/ul	0.00
58) Fluorene-d10	15.06	176	604075	34.76	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.22	200	85165	23.99	ng/ul	0.00
71) Anthracene-d10	16.91	188	923704	35.27	ng/ul	0.00
79) Pyrene-d10	19.22	212	1021142	34.38	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.01	264	1021591	35.54	ng/ul	0.00


Target Compounds					Qvalue	
15) N-Nitroso-di-n-propylamine	8.12	70	6516	1.073	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BN009750.D
Acq On : 18 Feb 2020 19:26
Operator : CG/JU
Sample : PB126856BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK56

Quant Time: Feb 19 03:39:41 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 19 03:37:25 2020
Response via : Initial Calibration

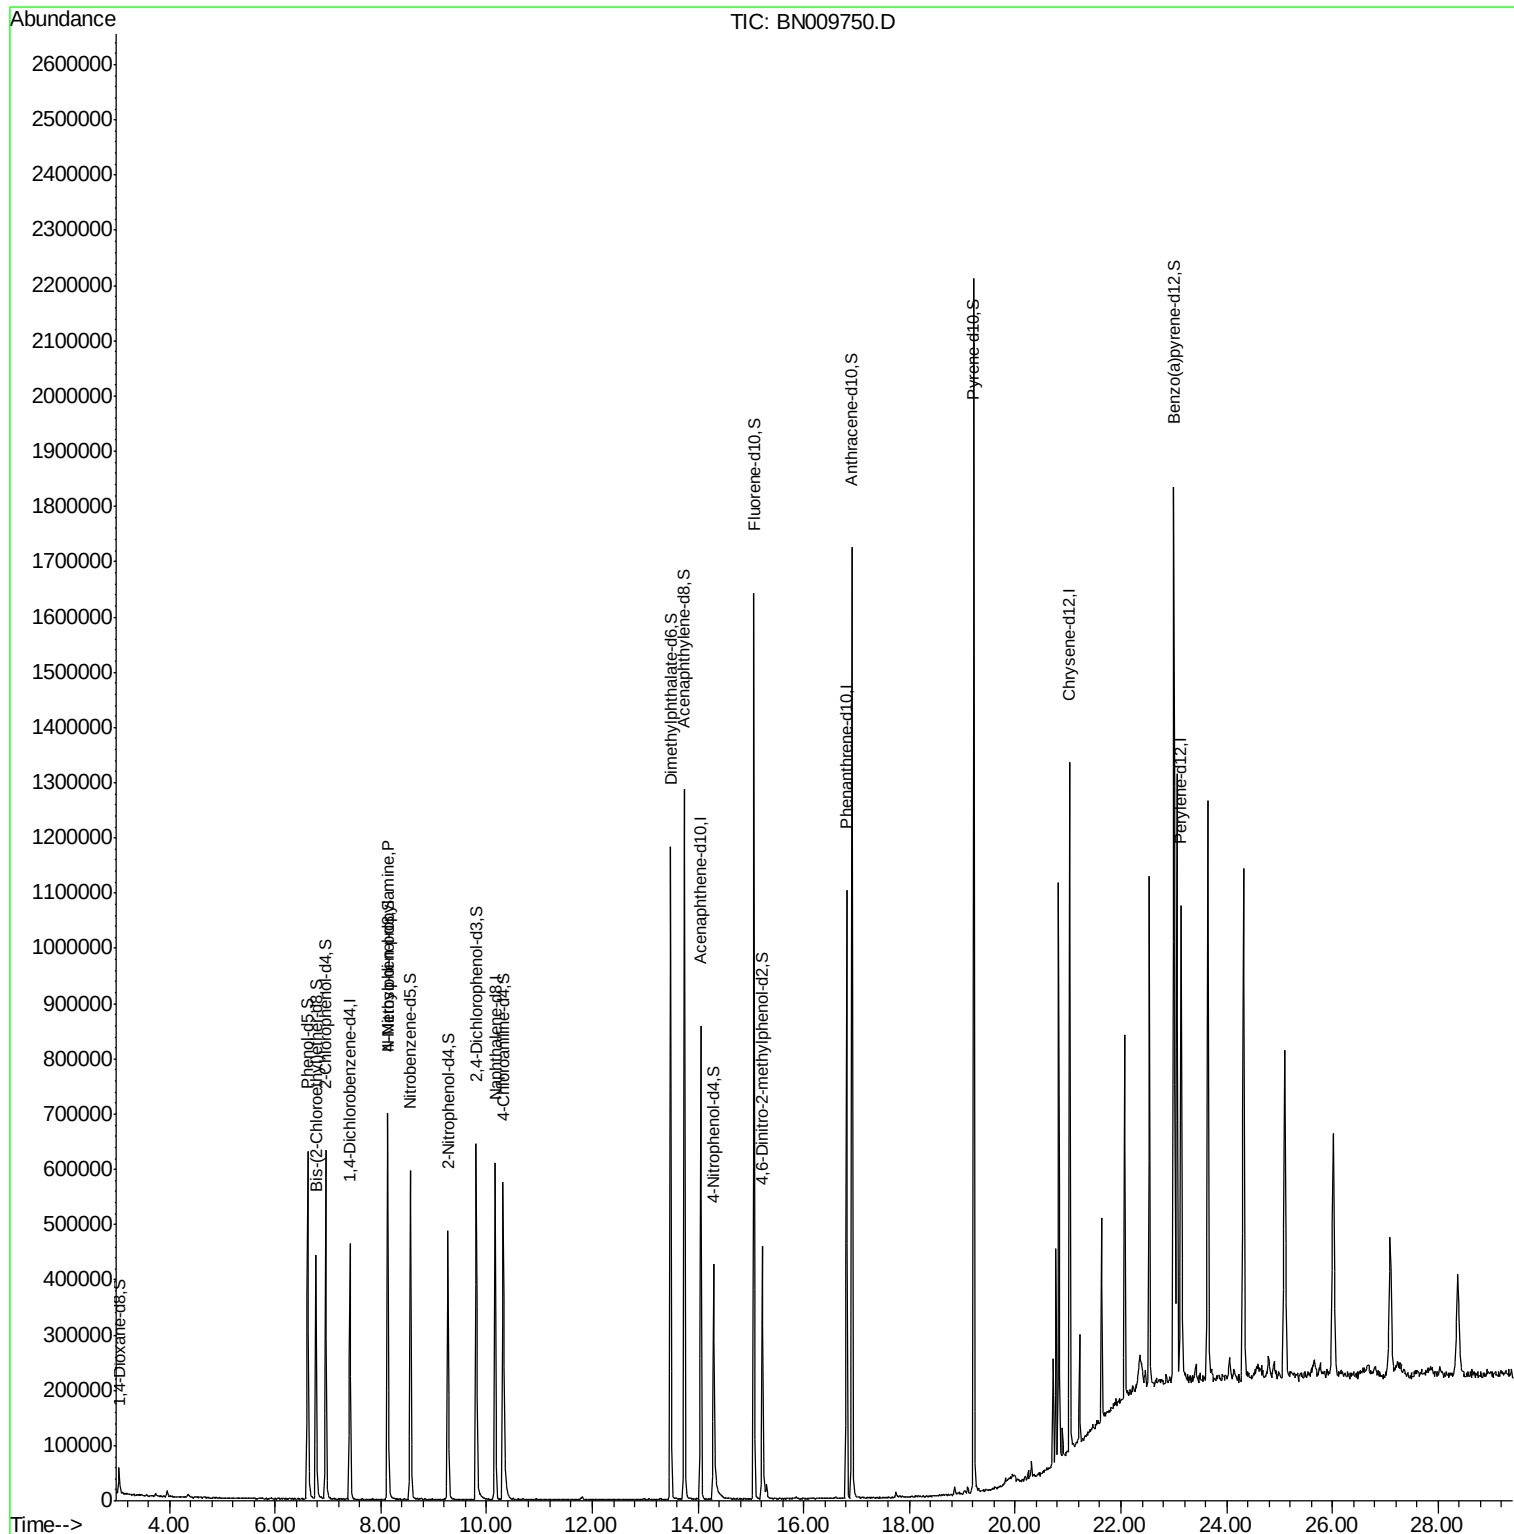

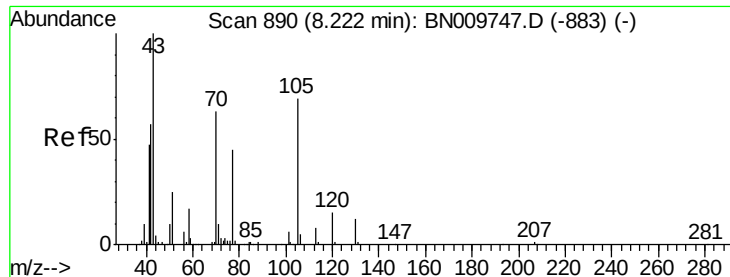

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.073 ng/ul
 RT: 8.12 min Scan# 873
 Delta R.T. -0.10 min
 Lab File: BN009750.D
 Acq: 18 Feb 2020 19:26

Instrument :
 BNA_N
 ClientSampleId :
 SBLK56

Tgt Ion: 70 Resp: 6516
 Ion Ratio Lower Upper
 70 100
 42 513.1 72.6 108.8#
 101 0.0 7.7 11.5#
 130 0.0 14.7 22.1#

