

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN021820\
 Data File : BN009753.D
 Acq On : 18 Feb 2020 21:14
 Operator : CG/JU
 Sample : L1541-06
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBD34

Manual Integrations
 APPROVED

mohammad
 2/20/2020 8:57:54 AM

Quant Time: Feb 19 03:57:00 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Feb 19 03:37:25 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.42	152	121324	20.00	ng/ul	0.00
18) Naphthalene-d8	10.16	136	513701	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.05	164	327540	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.81	188	706985	20.00	ng/ul	0.00
78) Chrysene-d12	21.03	240	683667	20.00	ng/ul	0.00
86) Perylene-d12	23.13	264	704040	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.05	96	14444	4.90	ng/uL	0.00
5) Phenol-d5	6.62	99	56114	5.44	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.78	67	195459	27.45	ng/ul	0.00
9) 2-Chlorophenol-d4	6.96	132	172903	22.26	ng/ul	0.00
13) 4-Methylphenol-d8	8.13	113	106103	12.93	ng/ul	0.00
19) Nitrobenzene-d5	8.56	128	105415	28.05	ng/ul	0.00
22) 2-Nitrophenol-d4	9.27	143	112147	27.28	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.80	165	186326	23.57	ng/ul	0.00
29) 4-Chloroaniline-d4	10.35	131	11791m	1.33	ng/ul	0.04
44) Dimethylphthalate-d6	13.48	166	732973	29.96	ng/ul	0.00
47) Acenaphthylene-d8	13.74	160	835257	28.99	ng/ul	0.00
52) 4-Nitrophenol-d4	14.31	143	17117	3.83	ng/ul	0.02
58) Fluorene-d10	15.06	176	654749	31.00	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.21	200	116992	26.64	ng/ul	0.00
71) Anthracene-d10	16.91	188	1110374	34.26	ng/ul	0.00
79) Pyrene-d10	19.22	212	1281181	35.85	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.00	264	1304756	37.11	ng/ul	0.00

Target Compounds					Ovalue	
45) Dimethylphthalate	13.53	163	26356	1.032	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN021820\
Data File : BN009753.D
Acq On : 18 Feb 2020 21:14
Operator : CG/JU
Sample : L1541-06
Misc :
ALS Vial : 12 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
DBD34

Manual Integrations
APPROVED

mohammad
2/20/2020 8:57:54 AM

Quant Time: Feb 19 03:57:00 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 19 03:37:25 2020
Response via : Initial Calibration

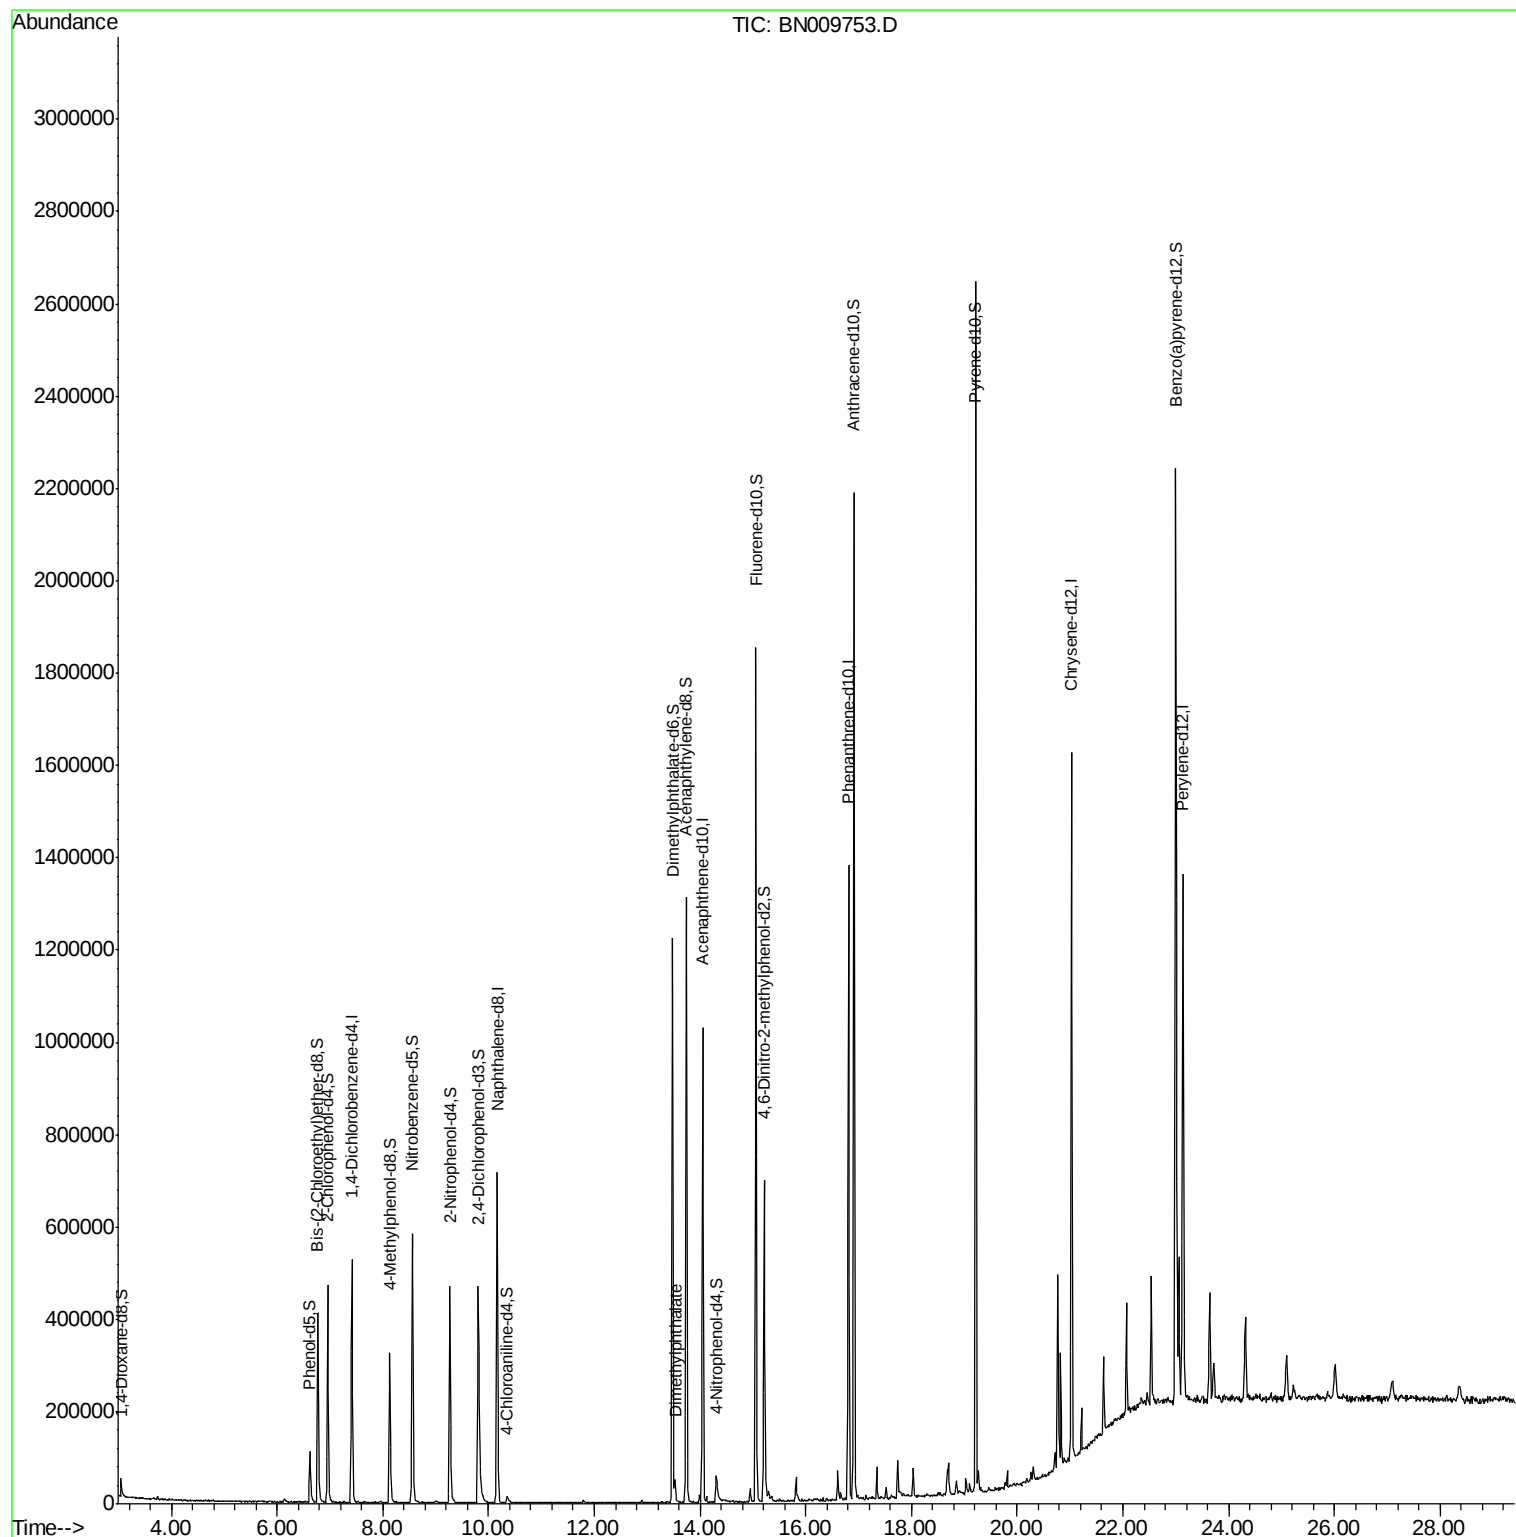

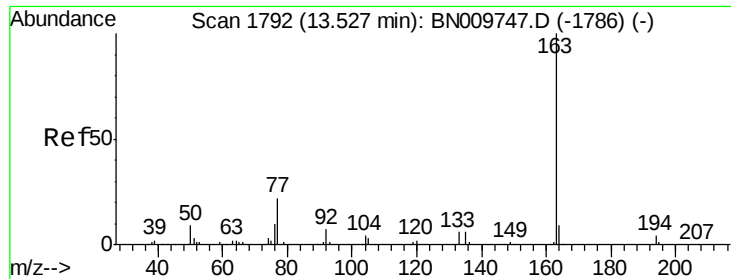

#45
 Dimethylphthalate
 Concen: 1.032 ng/ul
 RT: 13.53 min Scan# 1792
 Delta R.T. 0.00 min
 Lab File: BN009753.D
 Acq: 18 Feb 2020 21:14

Instrument :
 BNA_N
 ClientSampleId :
 DBD34

Tot Ion:	163	Resp:	26356
Ion Ratio	Lower	Upper	
163	100		
194	4.7	3.4	5.0
164	9.8	8.0	12.0

Manual Integrations
 APPROVED

mohammad
 2/20/2020 8:57:54 AM

