

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN021820\
 Data File : BN009767.D
 Acq On : 19 Feb 2020 06:12
 Operator : CG/JU
 Sample : L1555-01
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBD80

Manual Integrations
 APPROVED

mohammad
 2/20/2020 8:58:26 AM

Quant Time: Feb 19 08:24:09 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Feb 19 04:46:48 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.41	152	129252	20.00	ng/ul	0.00
18) Naphthalene-d8	10.16	136	521686	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.05	164	324503	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.81	188	684685	20.00	ng/ul	0.00
78) Chrysene-d12	21.03	240	646290	20.00	ng/ul	0.00
86) Perylene-d12	23.13	264	666010	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.05	96	17897	5.69	ng/uL	0.00
5) Phenol-d5	6.62	99	76397	6.95	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.77	67	253961	33.47	ng/ul	0.00
9) 2-Chlorophenol-d4	6.95	132	232149	28.05	ng/ul	0.00
13) 4-Methylphenol-d8	8.13	113	145643	16.65	ng/ul	0.00
19) Nitrobenzene-d5	8.56	128	140631	36.85	ng/ul	0.00
22) 2-Nitrophenol-d4	9.27	143	152746	36.58	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.80	165	251955	31.39	ng/ul	0.00
29) 4-Chloroaniline-d4	10.36	131	12437m	1.38	ng/ul	0.04
44) Dimethylphthalate-d6	13.48	166	936939	38.66	ng/ul	0.00
47) Acenaphthylene-d8	13.74	160	1083948	37.97	ng/ul	0.00
52) 4-Nitrophenol-d4	14.31	143	23703m	5.35	ng/ul	0.02
58) Fluorene-d10	15.06	176	815489	38.97	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.21	200	136368	32.06	ng/ul	0.00
71) Anthracene-d10	16.91	188	1314830	41.89	ng/ul	0.00
79) Pyrene-d10	19.22	212	1440814	42.65	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.00	264	1427079	42.91	ng/ul	0.00

Target Compounds				Ovalue	
45) Dimethylphthalate	13.53	163	33734	1.334	ng/ul# 96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN021820\
Data File : BN009767.D
Acq On : 19 Feb 2020 06:12
Operator : CG/JU
Sample : L1555-01
Misc :
ALS Vial : 26 Sample Multiplier: 1




Instrument :
BNA_N
ClientSampleId :
DBD80

Manual Integrations
APPROVED

mohammad
2/20/2020 8:58:26 AM

Quant Time: Feb 19 08:24:09 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 19 04:46:48 2020
Response via : Initial Calibration

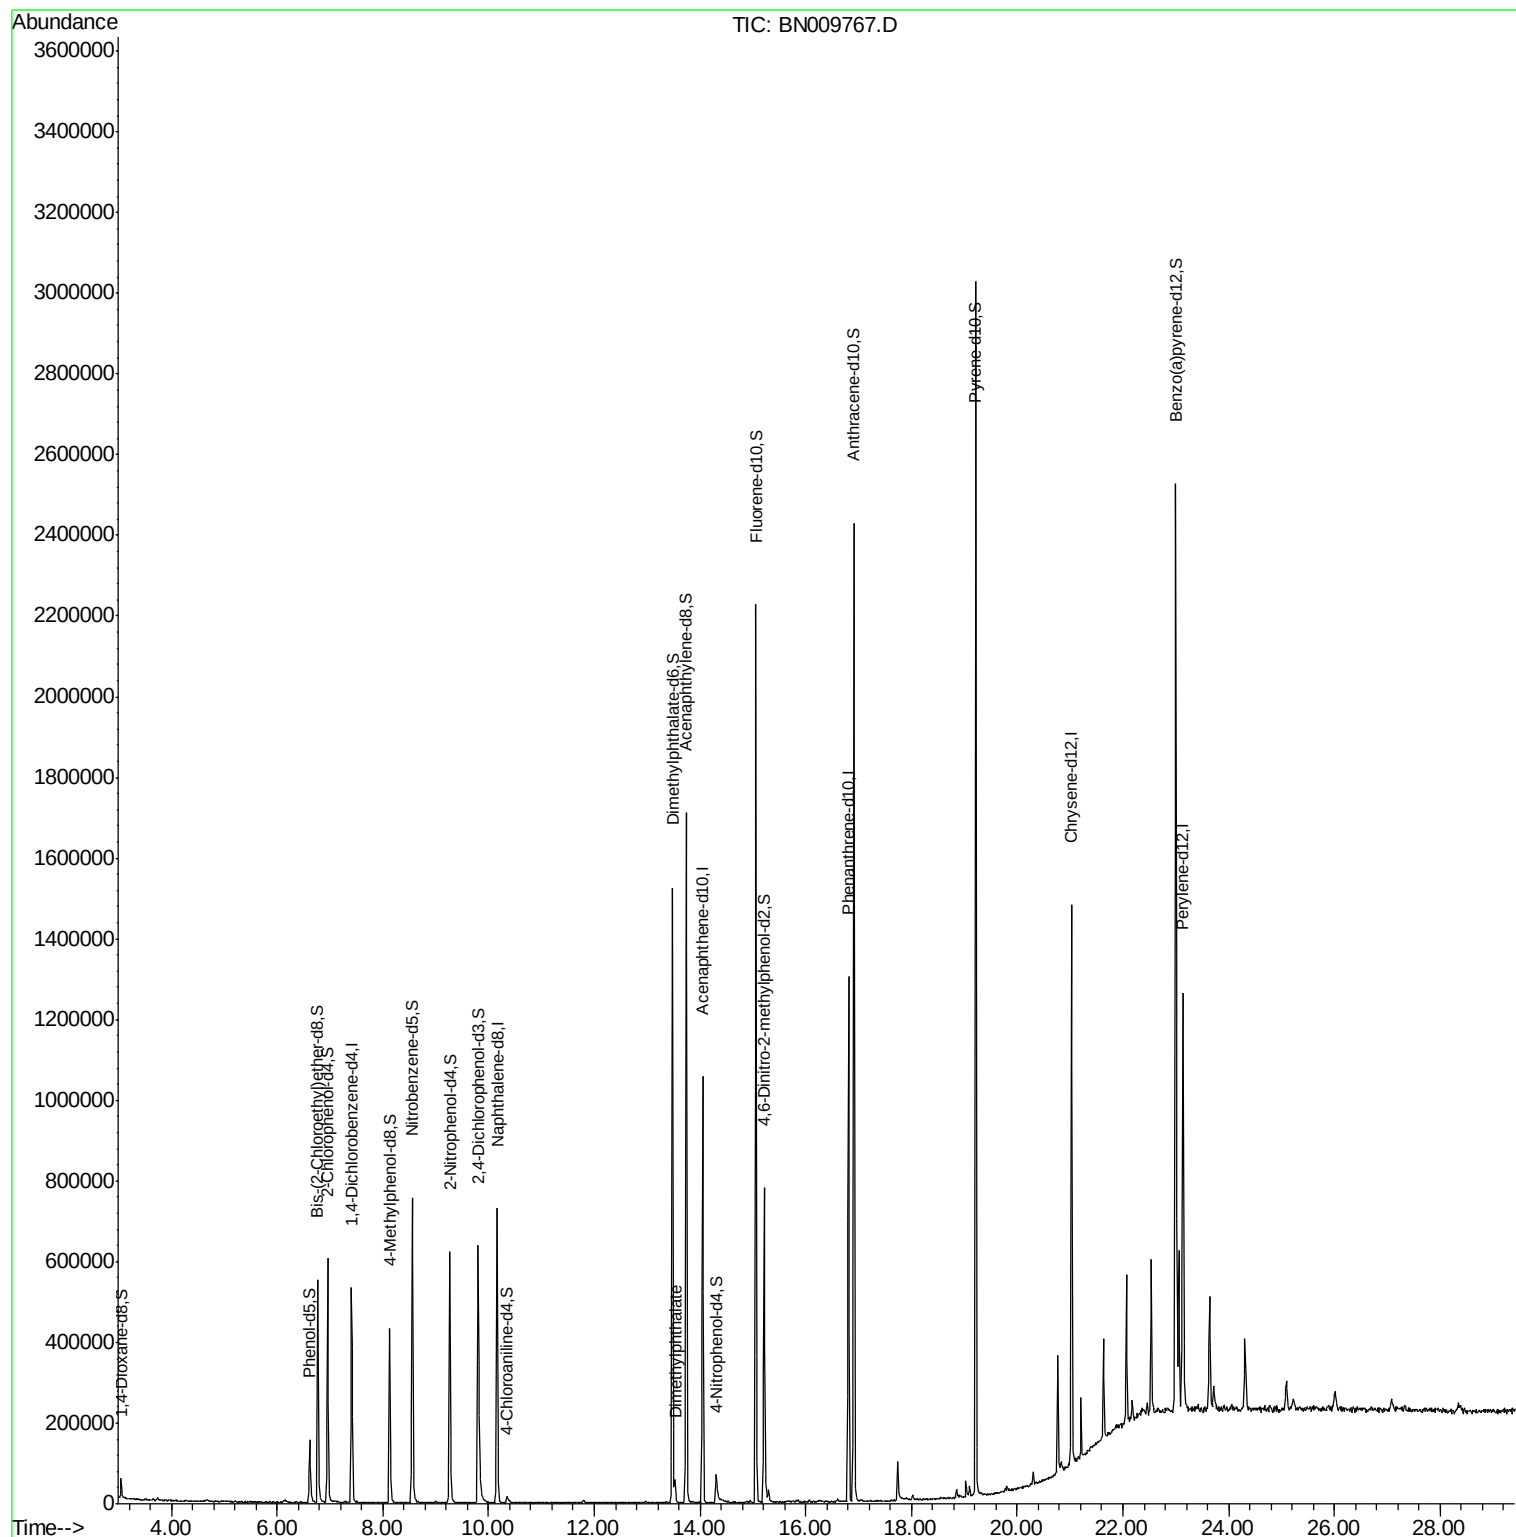

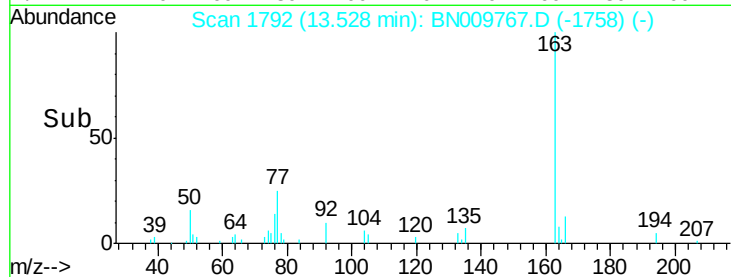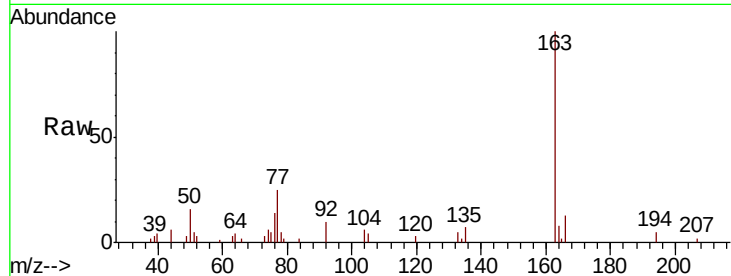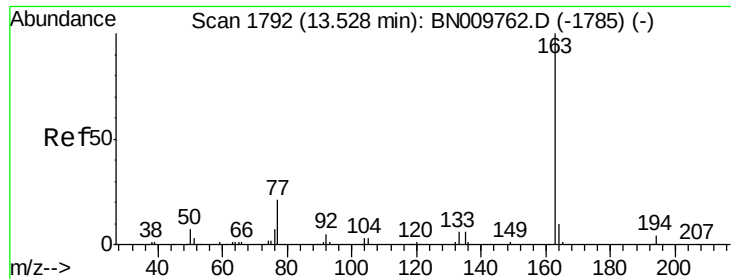

#45
 Dimethylphthalate
 Concen: 1.334 ng/ul
 RT: 13.53 min Scan# 1792
 Delta R.T. -0.00 min
 Lab File: BN009767.D
 Acq: 19 Feb 2020 06:12

Instrument :
 BNA_N
 ClientSampleId :
 DBD80

Tot Ion	Ratio	Resp	Lower	Upper
163	100	33734		
194	5.4		3.4	5.0#
164	8.5		8.0	12.0

Manual Integrations
 APPROVED

mohammad
 2/20/2020 8:58:26 AM

